

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF080218\
 Data File : VF059834.D
 Acq On : 3 Aug 2018 12:24
 Operator : VA/AP
 Sample : J4285-05
 Misc : 5.47g/5mL/MSVOA F/SOIL
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 KG-PIT-2

Quant Time: Aug 03 13:51:20 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F073018S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 31 15:23:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.03	168	282102	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.76	114	433602	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.91	117	399607	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.62	152	210501	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.02	65	189555	37.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	74.78%	
35) Dibromofluoromethane	4.29	113	166494	36.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	73.94%	
50) Toluene-d8	7.71	98	365276	34.78	ug/l	0.00
Spiked Amount	50.000		Recovery	=	69.56%	
62) 4-Bromofluorobenzene	11.50	95	173756	29.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	59.78%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF080218\
Data File : VF059834.D
Acq On : 3 Aug 2018 12:24
Operator : VA/AP
Sample : J4285-05
Misc : 5.47g/5mL/MSVOA F/SOIL
ALS Vial : 100 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
KG-PIT-2

Quant Time: Aug 03 13:51:20 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F073018S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 31 15:23:22 2018
Response via : Initial Calibration

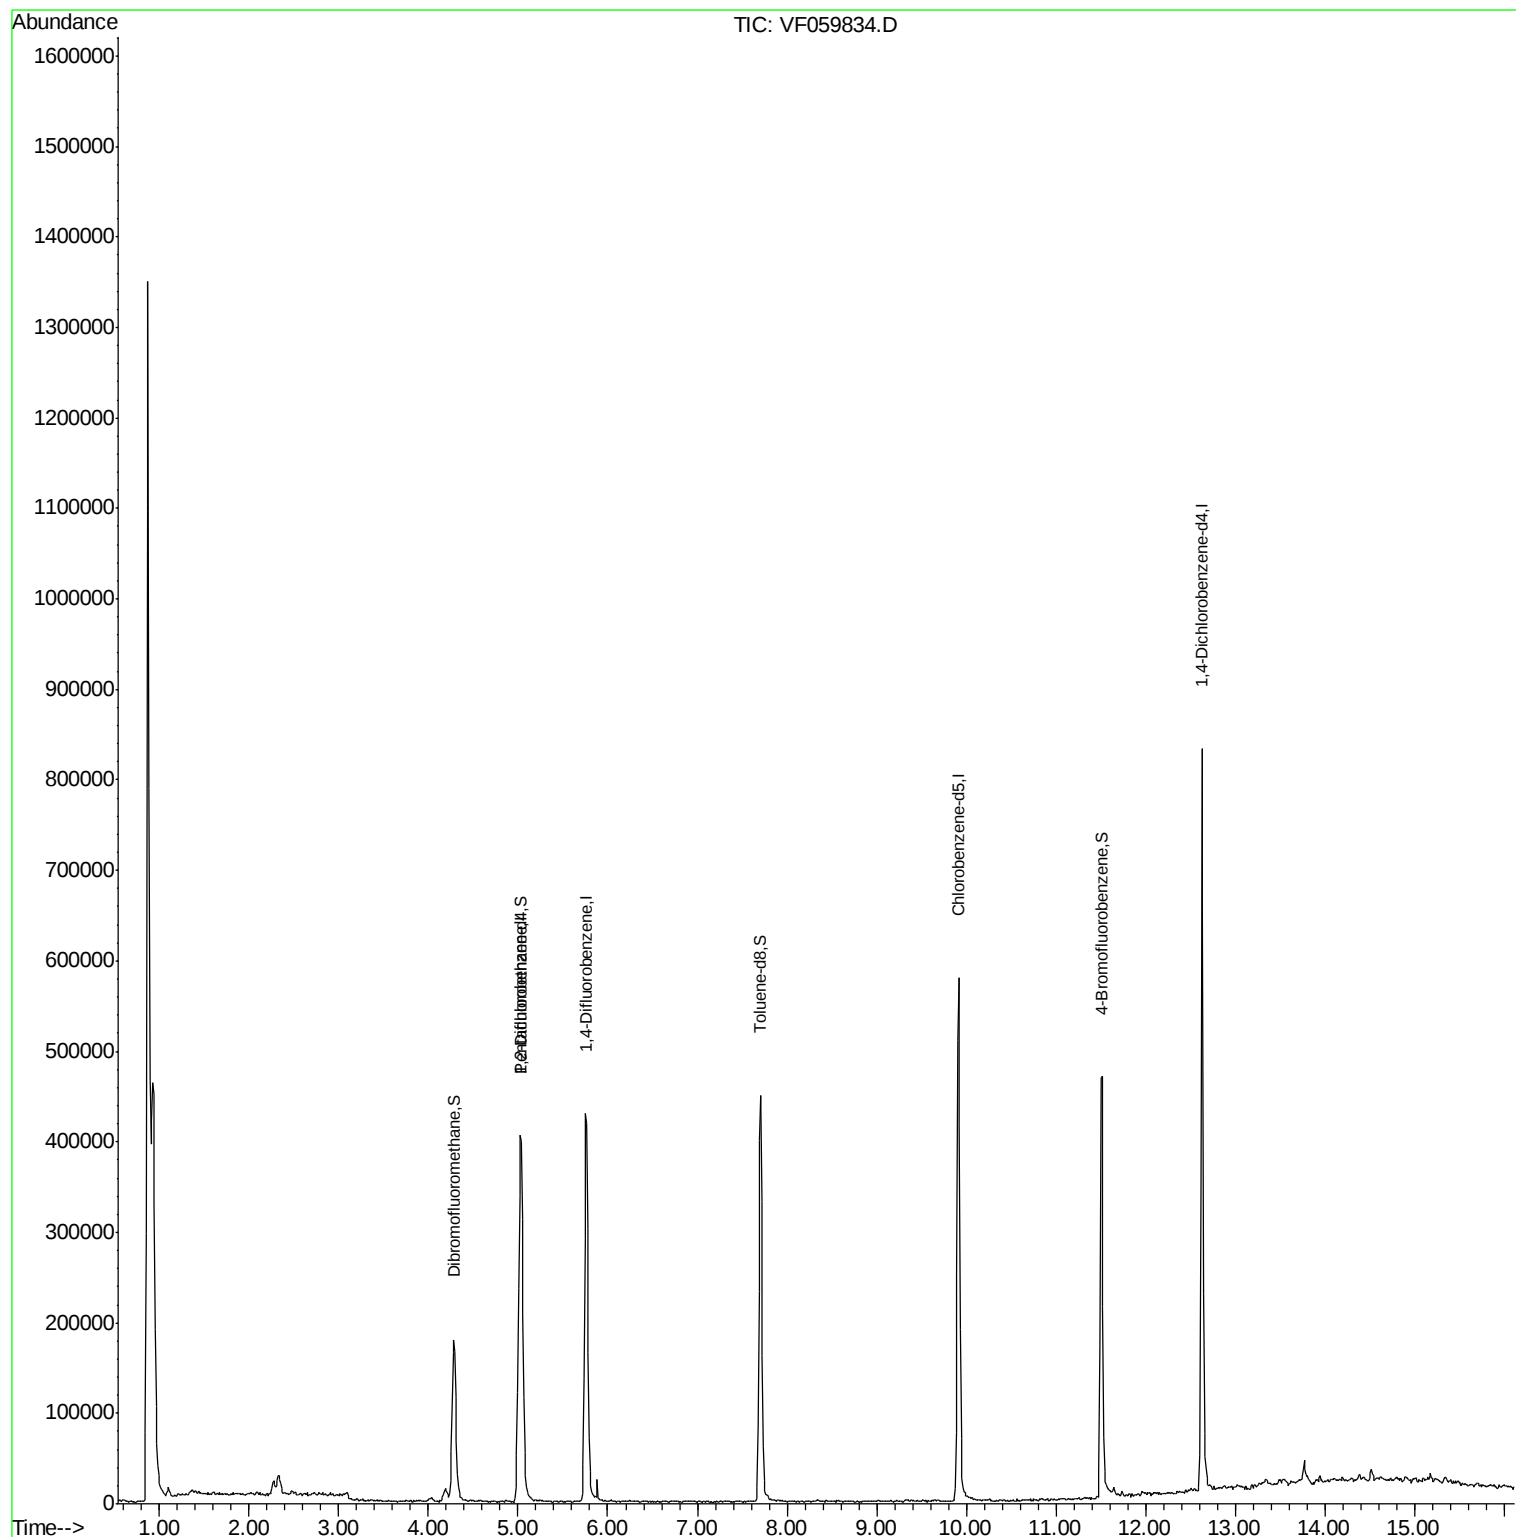

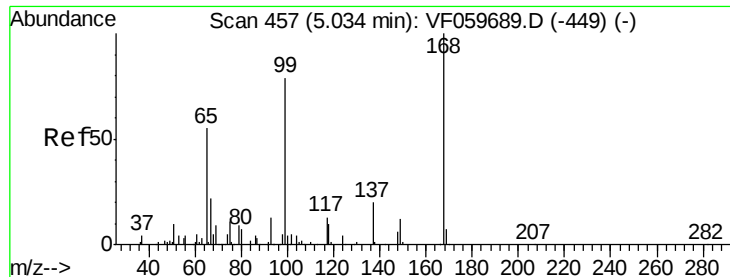

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.03 min Scan# 457

Delta R.T. 0.00 min

Lab File: VF059834.D

Acq: 3 Aug 2018 12:24

Instrument :

MSVOA_F

ClientSampleId :


KG-PIT-2

Tot Ion:168 Resp: 282102

Ion Ratio Lower Upper

168 100

99 71.4 63.3 94.9

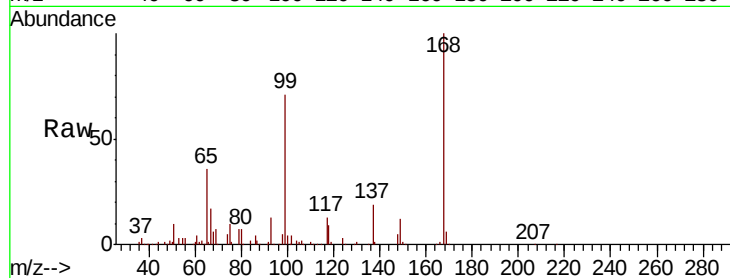

Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

5.03

100000

80000



60000

40000

20000

0

Time-->

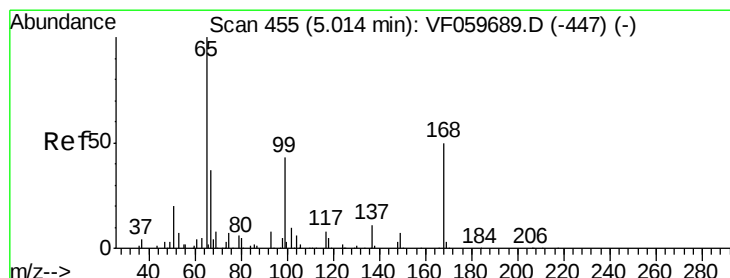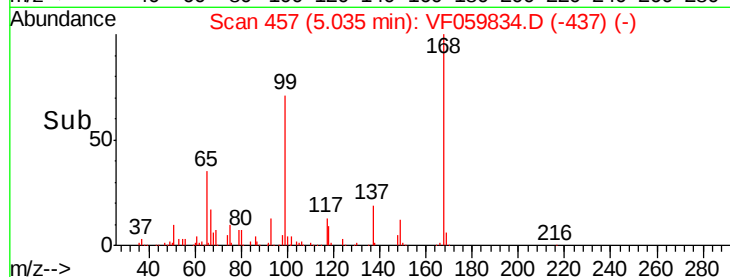

#33

1,2-Dichloroethane-d4

Concen: 37.39 ug/l

RT: 5.02 min Scan# 455

Delta R.T. 0.00 min

Lab File: VF059834.D


Acq: 3 Aug 2018 12:24

Tgt Ion: 65 Resp: 189555

Ion Ratio Lower Upper

65 100

67 46.2 0.0 84.6

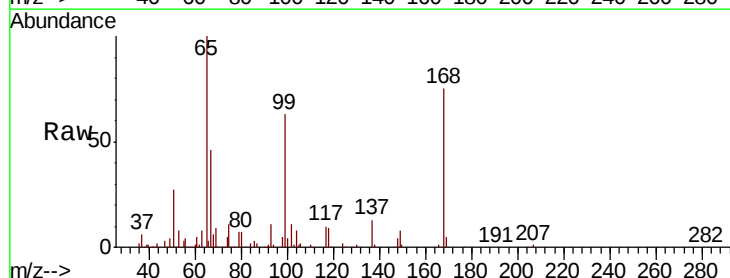

Abundance Ion 65.00 (64.70 to 65.70): VF0

Ion 67.00 (66.70 to 67.70): VF0

5.02


60000


40000

20000

0

Time-->

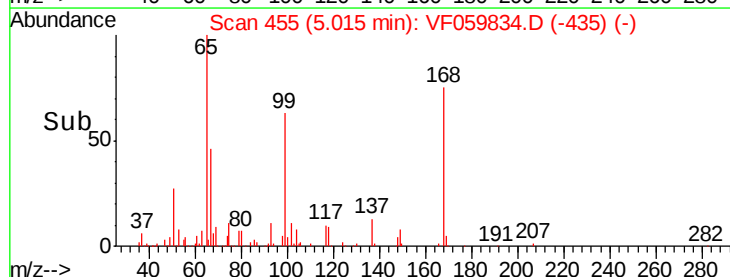

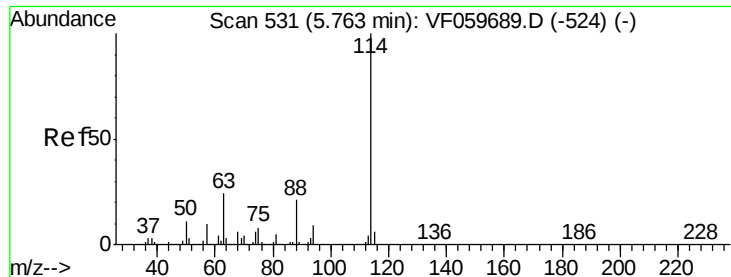

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 5.76 min Scan# 531

Delta R.T. 0.00 min

Lab File: VF059834.D

Acq: 3 Aug 2018 12:24

Instrument :

MSVOA_F

ClientSampleId :

KG-PIT-2


Tot Ion:114 Resp: 433602

Ion Ratio Lower Upper

114 100

63 21.5 0.0 47.4




88 20.6 0.0 41.2

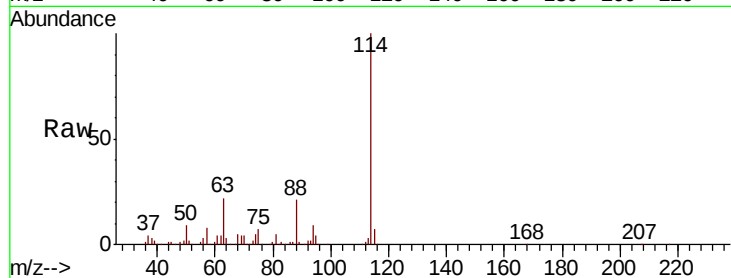

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VF0

Ion 88.00 (87.70 to 88.70): VF0

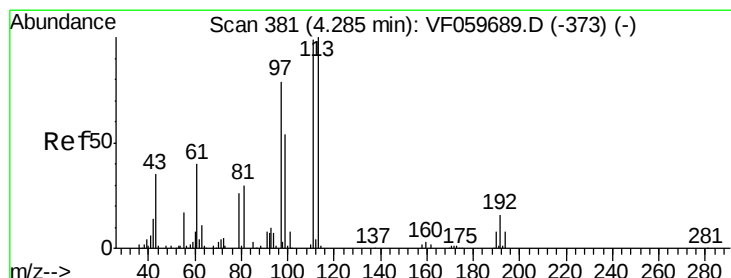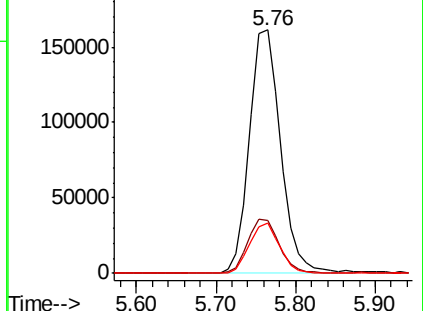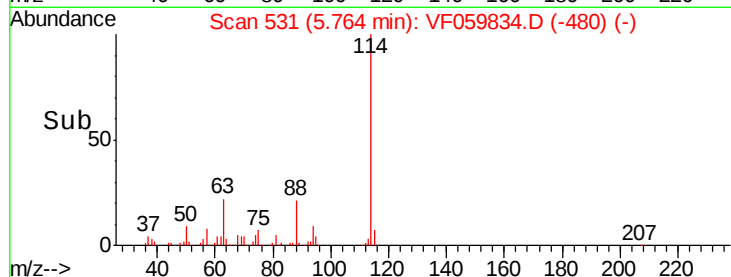

#35

Dibromofluoromethane

Concen: 36.97 ug/l

RT: 4.29 min Scan# 381

Delta R.T. 0.00 min

Lab File: VF059834.D

Acq: 3 Aug 2018 12:24


Tgt Ion:113 Resp: 166494

Ion Ratio Lower Upper

113 100

111 100.7 79.0 118.4



192 17.8 13.2 19.8

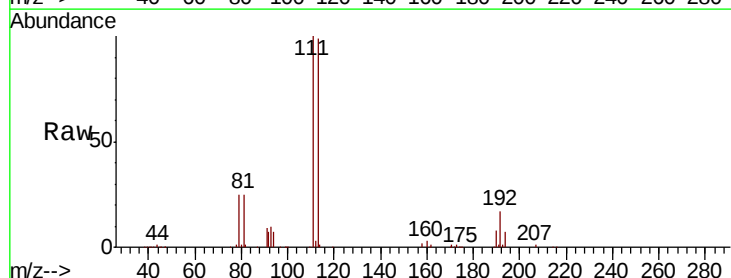


Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V



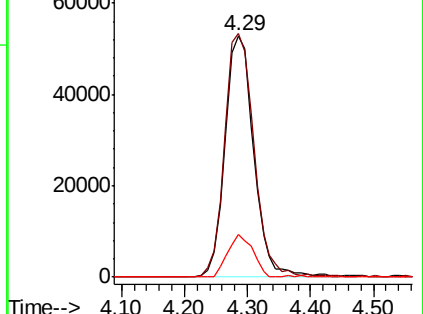
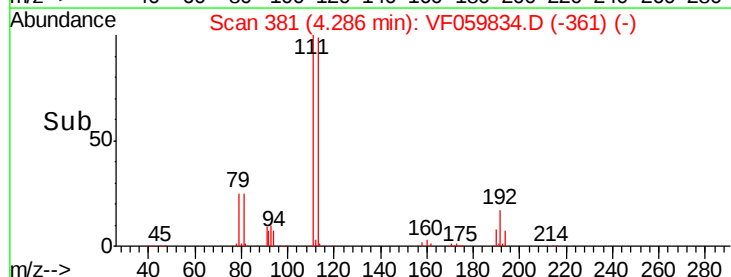


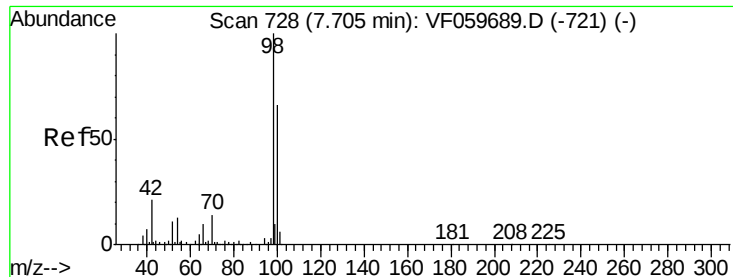

#50
Toluene-d8
Concen: 34.78 ug/l
RT: 7.71 min Scan# 728
Delta R.T. 0.00 min
Lab File: VF059834.D
Acq: 3 Aug 2018 12:24




Instrument :
MSVOA_F
ClientSampleId :
KG-PIT-2


Tot Ion: 98 Resp: 365276
Ion Ratio Lower Upper
98 100
100 67.7 52.8 79.2

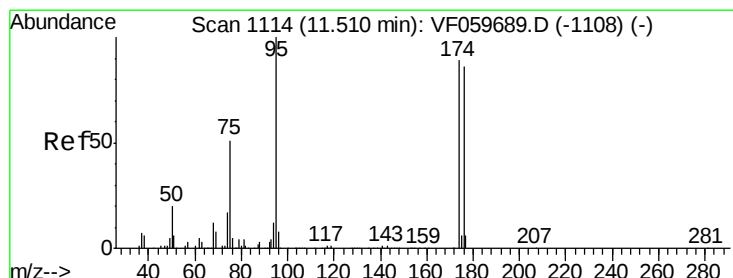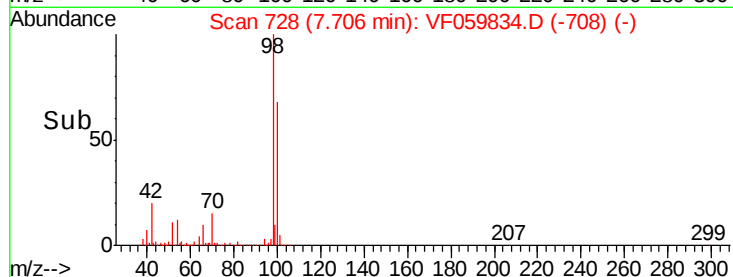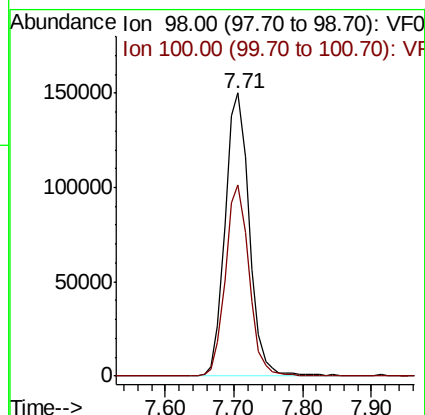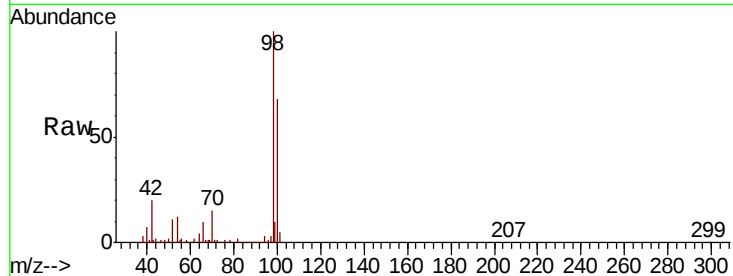

#62
4-Bromofluorobenzene
Concen: 29.89 ug/l
RT: 11.50 min Scan# 1113
Delta R.T. -0.01 min
Lab File: VF059834.D
Acq: 3 Aug 2018 12:24

Tgt Ion: 95 Resp: 173756
Ion Ratio Lower Upper
95 100
174 71.6 0.0 178.4
176 71.7 0.0 173.0

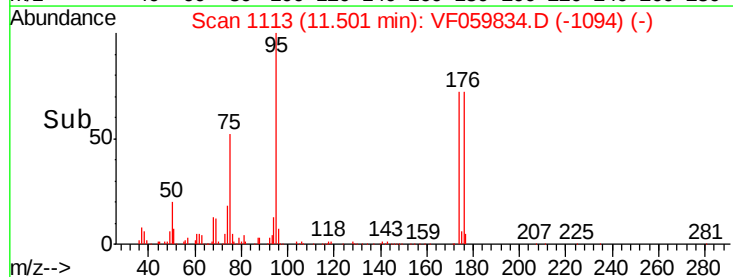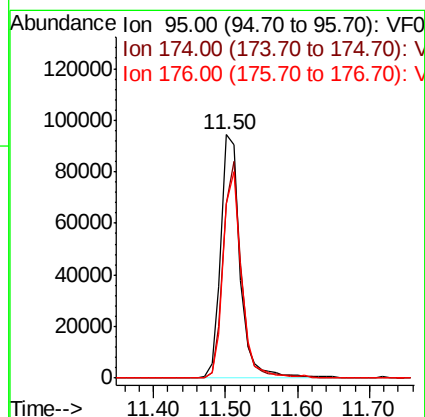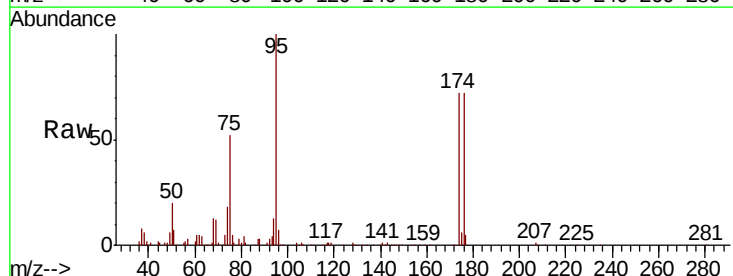


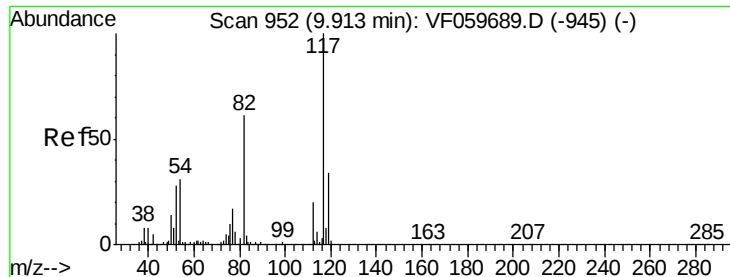

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.91 min Scan# 952
Delta R.T. 0.00 min
Lab File: VF059834.D
Acq: 3 Aug 2018 12:24

Instrument :
MSVOA_F
ClientSampleId :
KG-PIT-2

Tot Ion	Ratio	Lower	Upper
117	100		
82	58.5	49.0	73.4
119	31.6	27.3	40.9



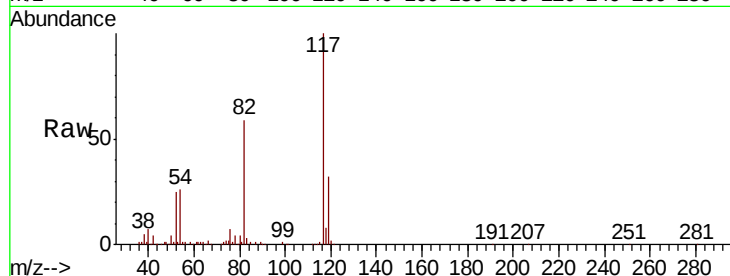


Abundance

Ion 117.00 (116.70 to 117.70): V


Ion 82.00 (81.70 to 82.70): VF0

Ion 119.00 (118.70 to 119.70): V

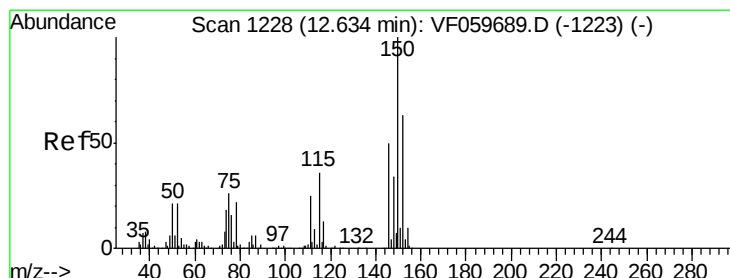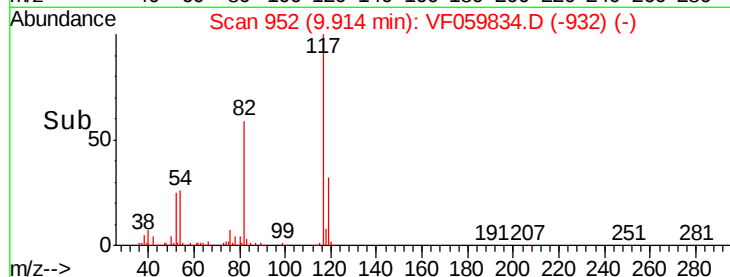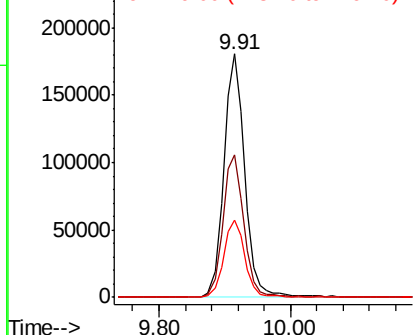

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.62 min Scan# 1227
Delta R.T. -0.01 min
Lab File: VF059834.D
Acq: 3 Aug 2018 12:24

Tgt Ion	Ratio	Lower	Upper
152	100		
115	61.4	28.2	84.6
150	154.9	0.0	316.2

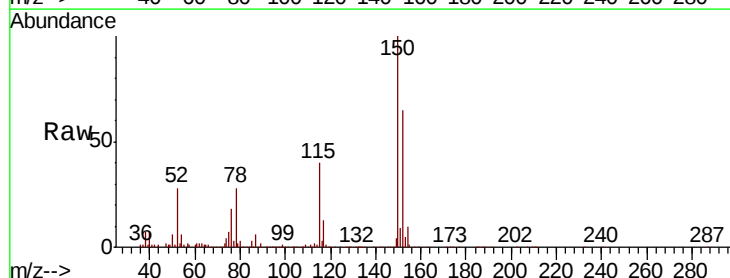

Abundance

Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

