


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF080218\
Data File : VF059795.D
Acq On : 2 Aug 2018 12:15
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F073018S.M
Title : SW846 8260
Last Update : Tue Jul 31 15:23:22 2018

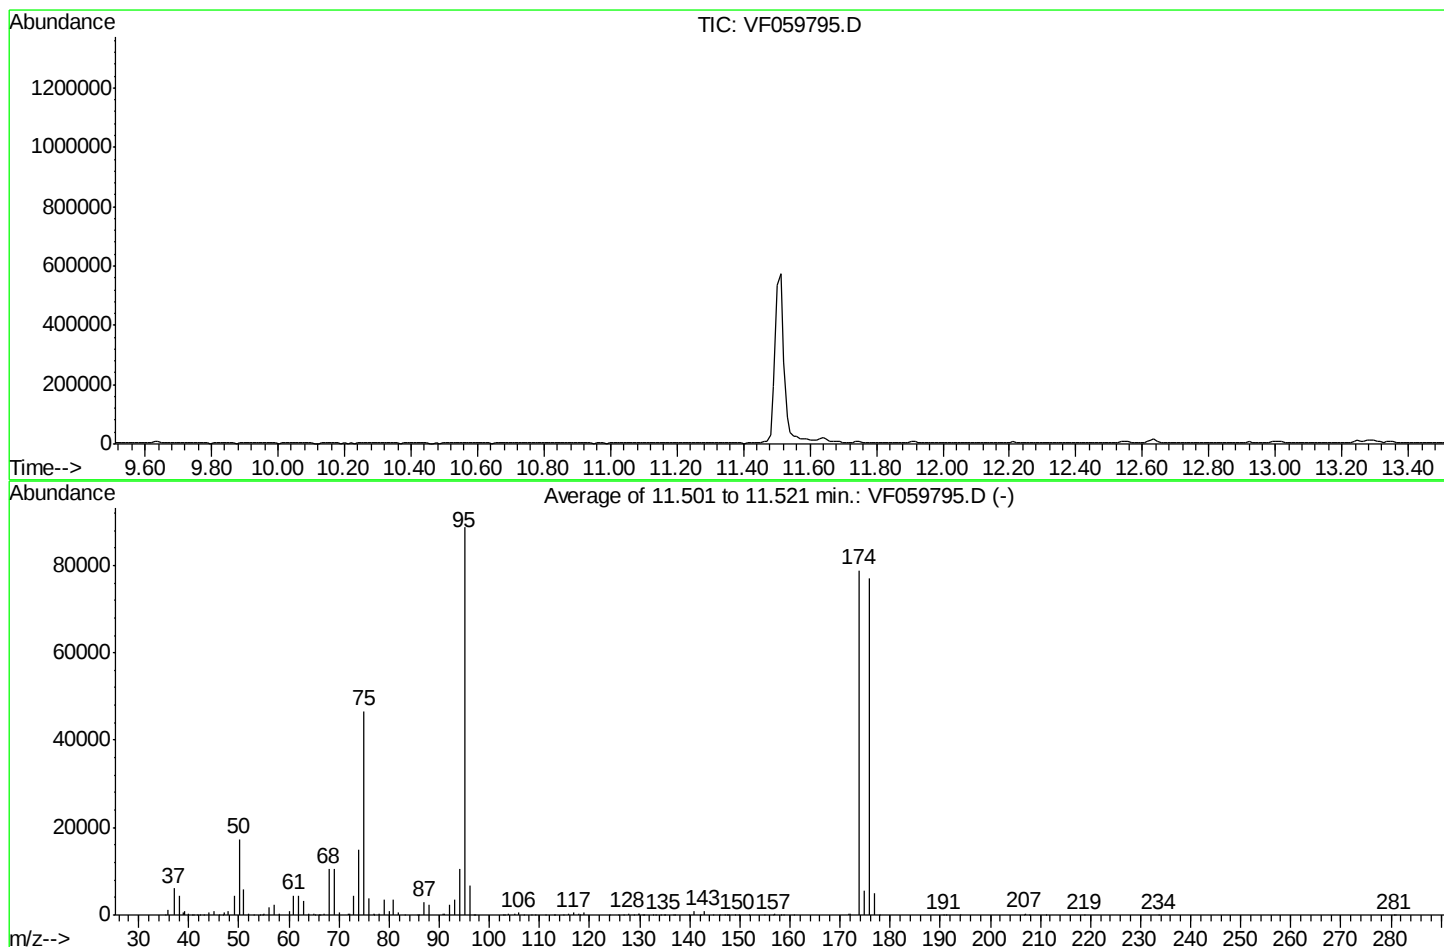

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	17434	PASS
75	95	30	60	52.6	46672	PASS
95	95	100	100	100.0	88709	PASS
96	95	5	9	7.5	6624	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.9	78826	PASS
175	174	5	9	7.0	5510	PASS
176	174	95	101	97.8	77114	PASS
177	176	5	9	6.6	5098	PASS