


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF080218\
 Data File : VF059820.D
 Acq On : 3 Aug 2018 1:11
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F073018S.M
 Title : SW846 8260
 Last Update : Tue Jul 31 15:23:22 2018

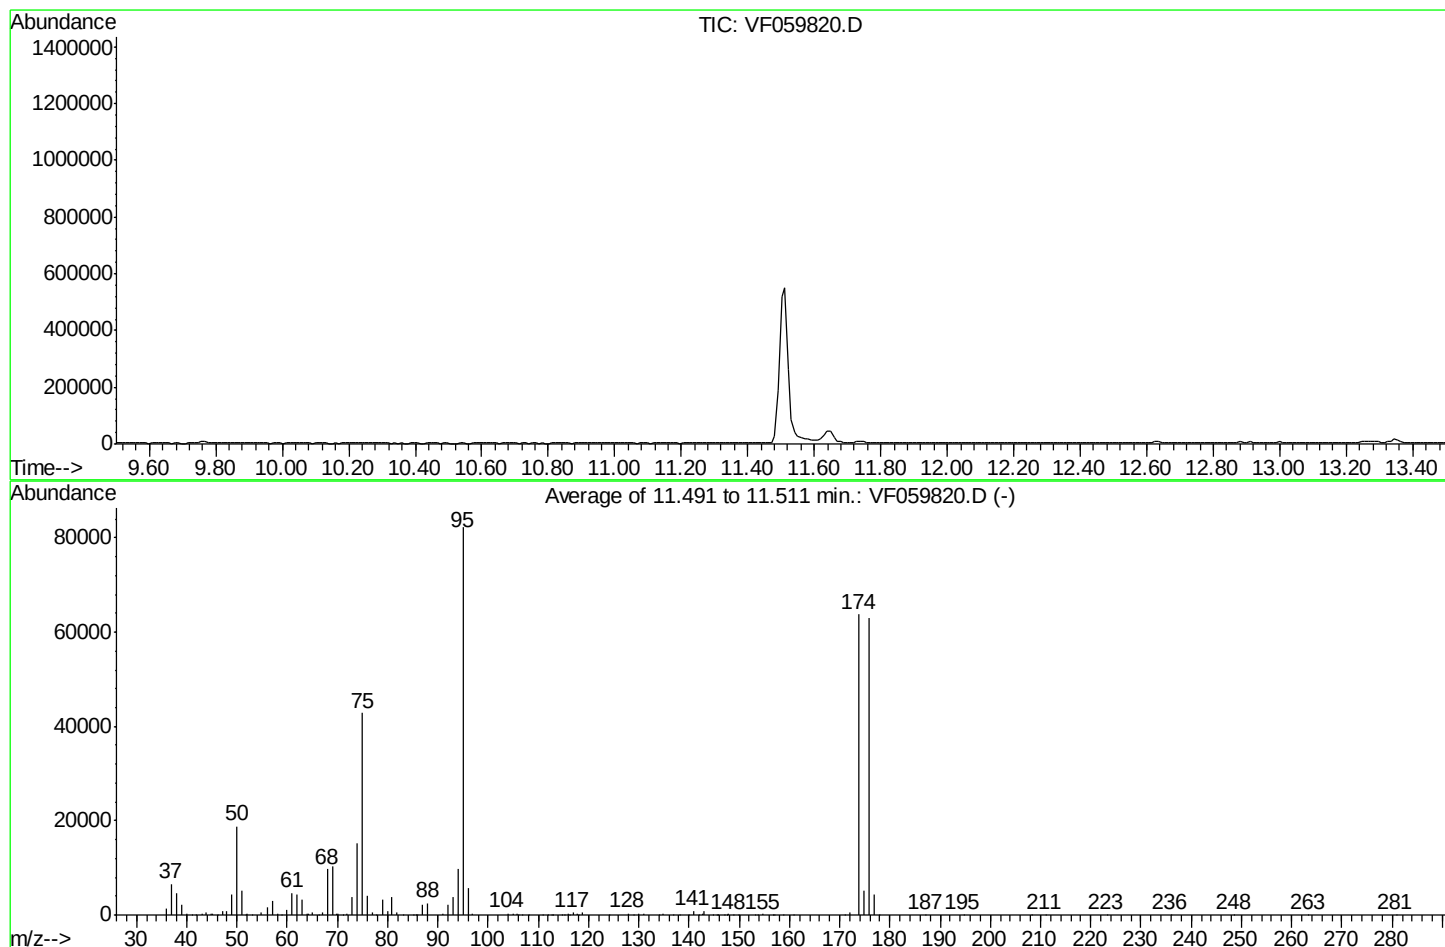

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	18756	PASS
75	95	30	60	52.1	42856	PASS
95	95	100	100	100.0	82232	PASS
96	95	5	9	7.0	5730	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.5	63690	PASS
175	174	5	9	7.9	5057	PASS
176	174	95	101	98.9	62968	PASS
177	176	5	9	6.7	4236	PASS