


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF080318\
 Data File : VF059836.D
 Acq On : 3 Aug 2018 13:32
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F073018S.M
 Title : SW846 8260
 Last Update : Tue Jul 31 15:23:22 2018

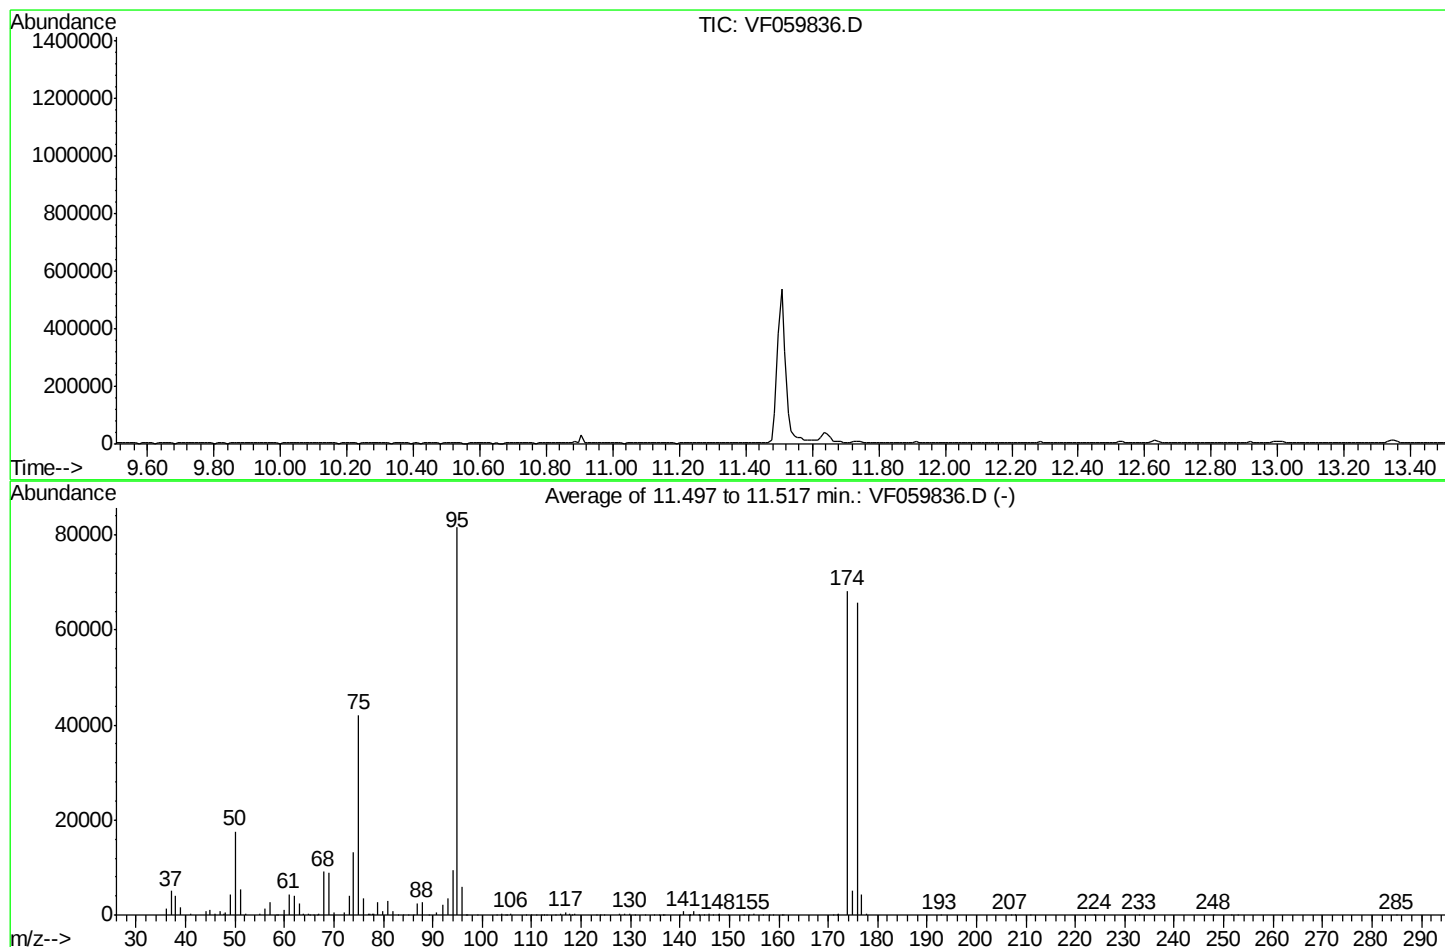

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	17623	PASS
75	95	30	60	51.6	42168	PASS
95	95	100	100	100.0	81642	PASS
96	95	5	9	7.1	5813	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.6	68216	PASS
175	174	5	9	7.3	5008	PASS
176	174	95	101	96.3	65690	PASS
177	176	5	9	6.5	4263	PASS