



Methylene Chloride

Response Ratio

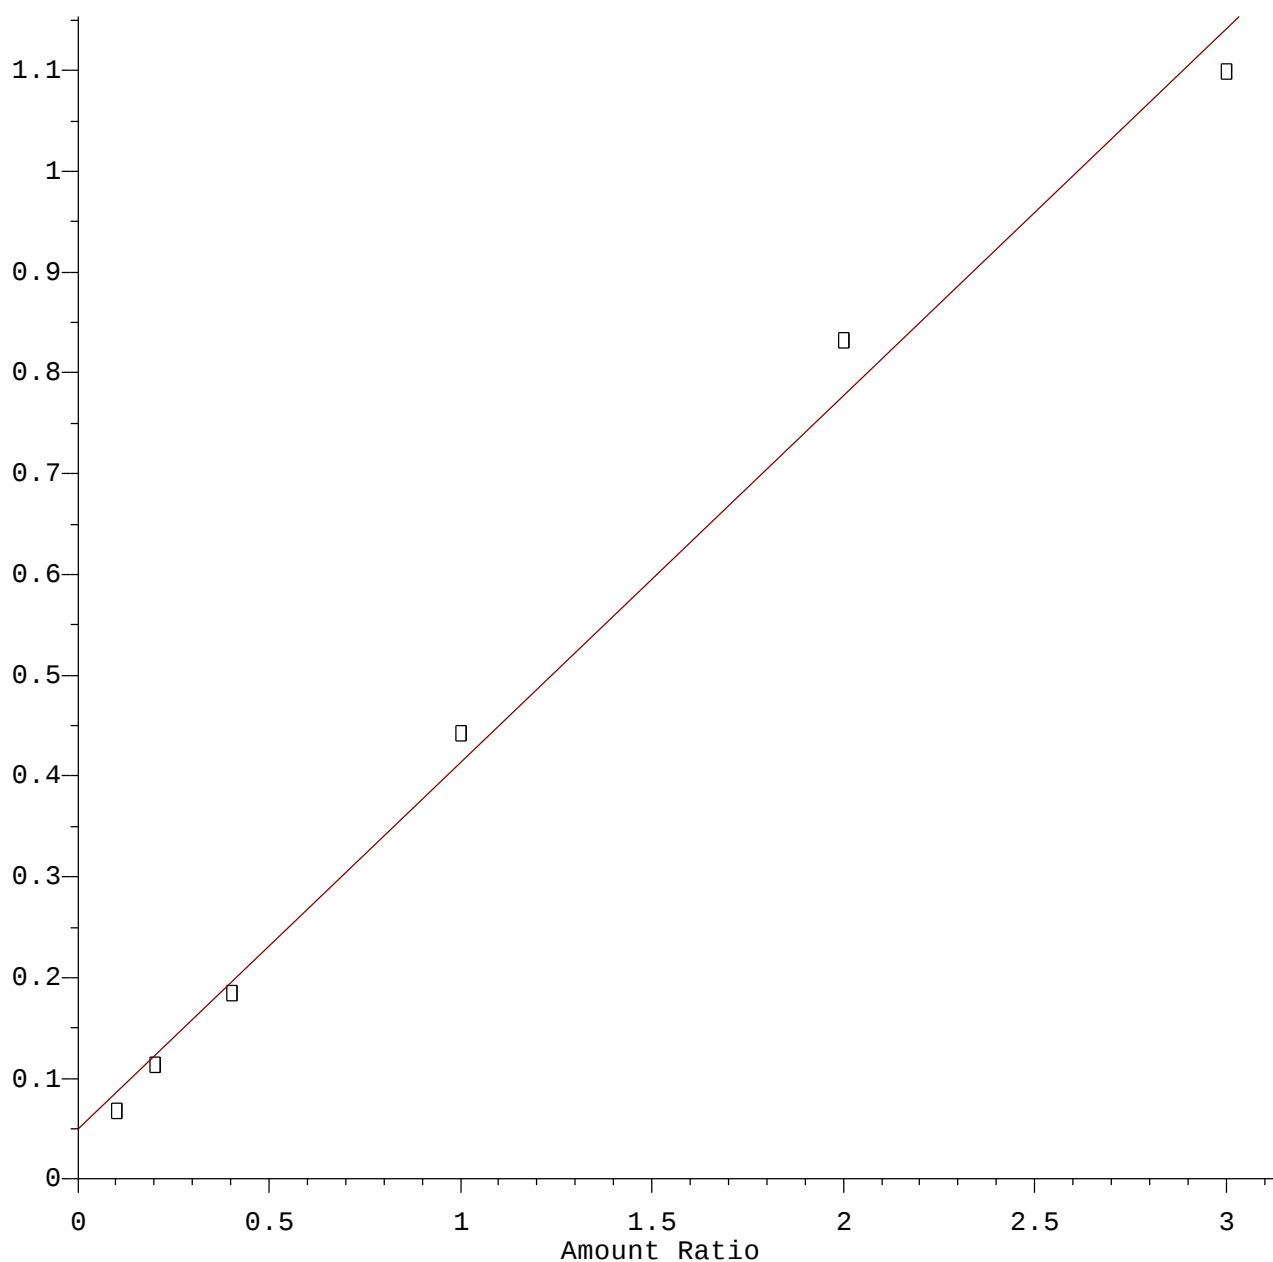


Resp Ratio = $3.64 \times 10^{-1} \times \text{Amt} + 4.99 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
Calibration Table Last Updated: Sat Aug 04 07:08:36 2018

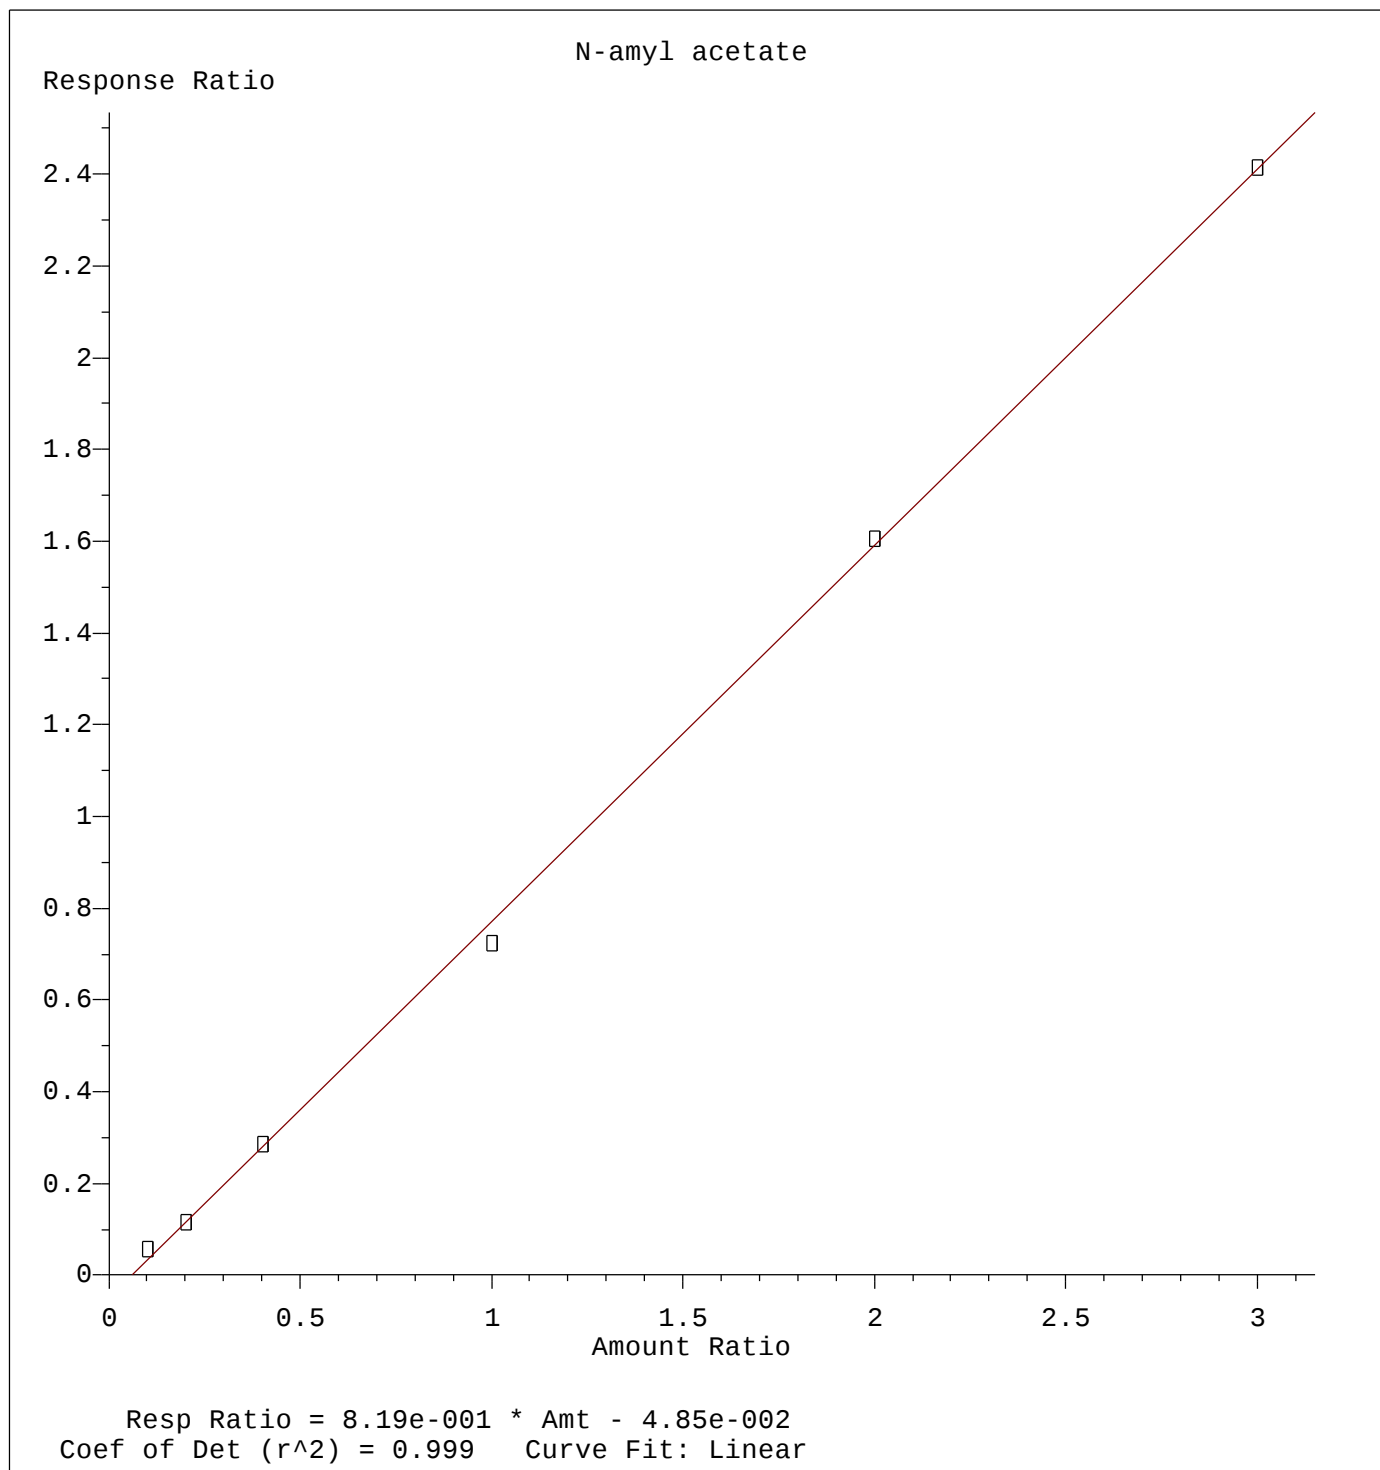


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
Calibration Table Last Updated: Sat Aug 04 07:08:36 2018

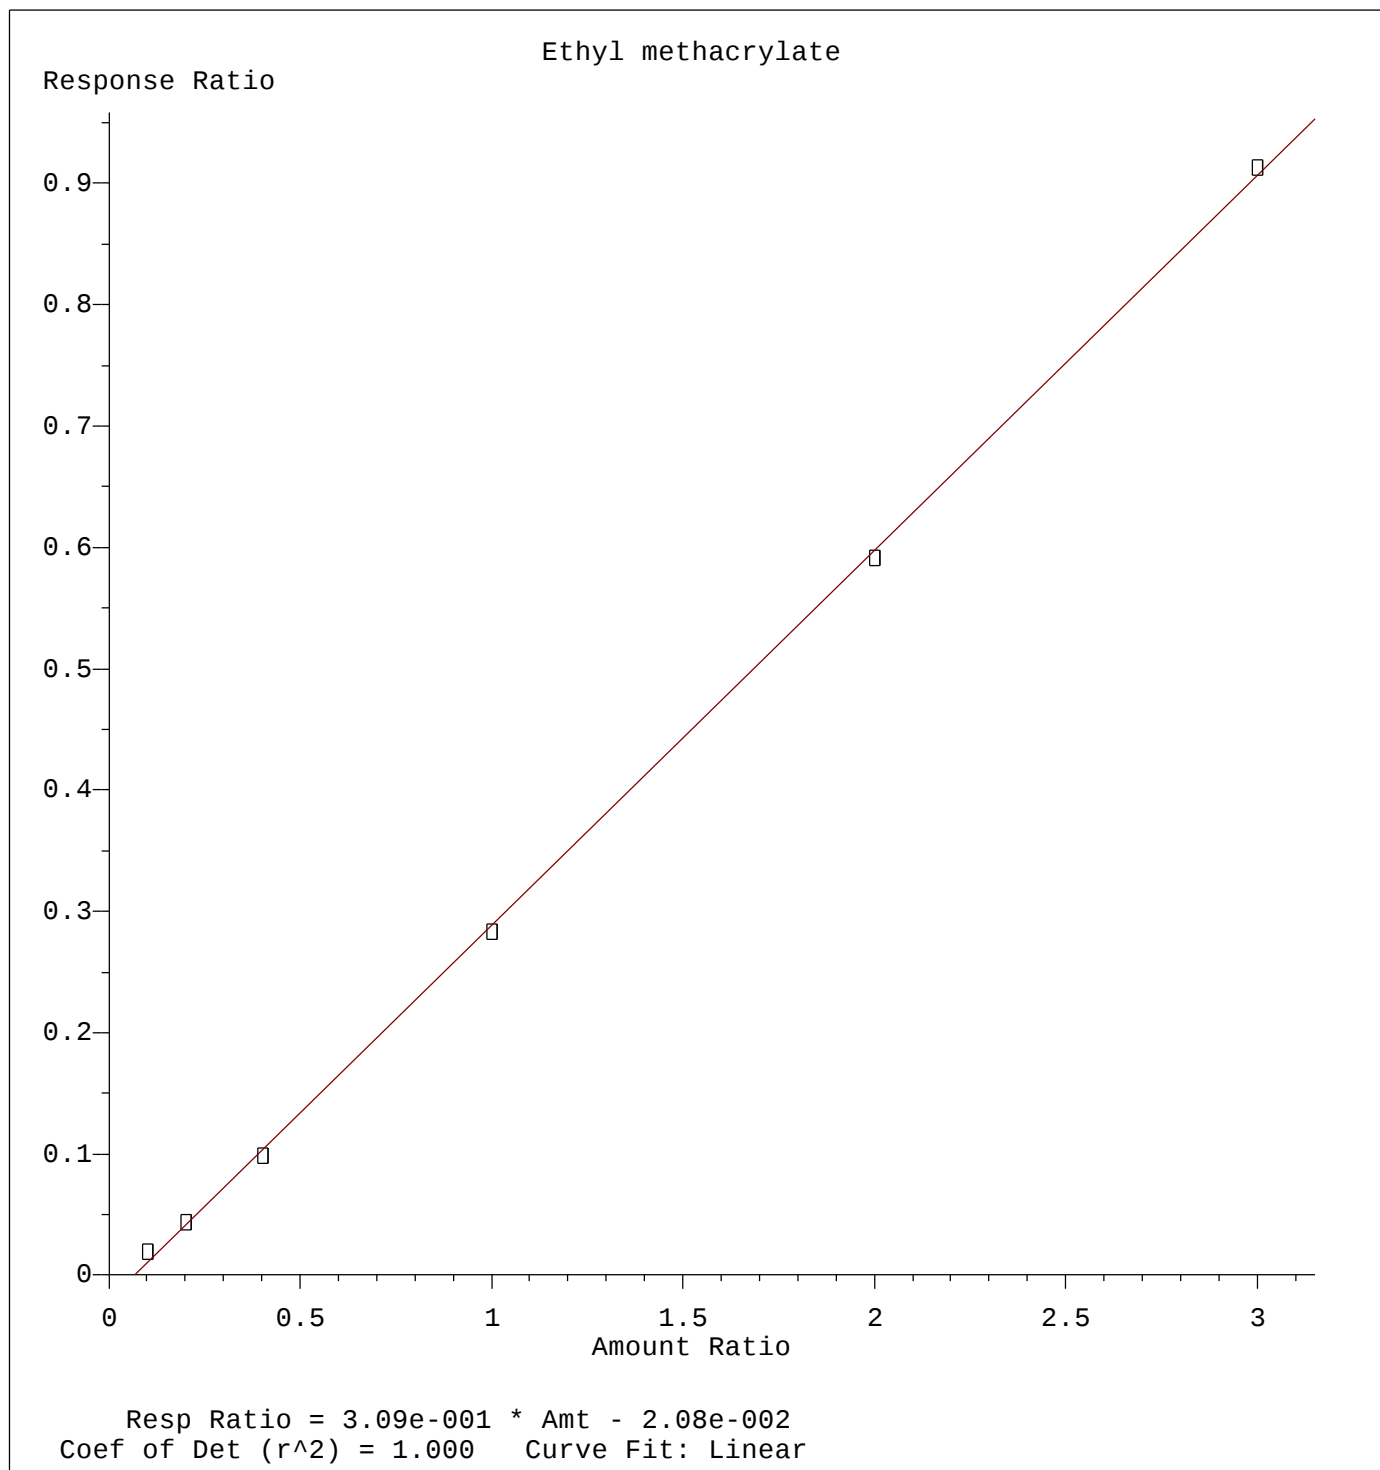

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
Calibration Table Last Updated: Sat Aug 04 07:08:36 2018

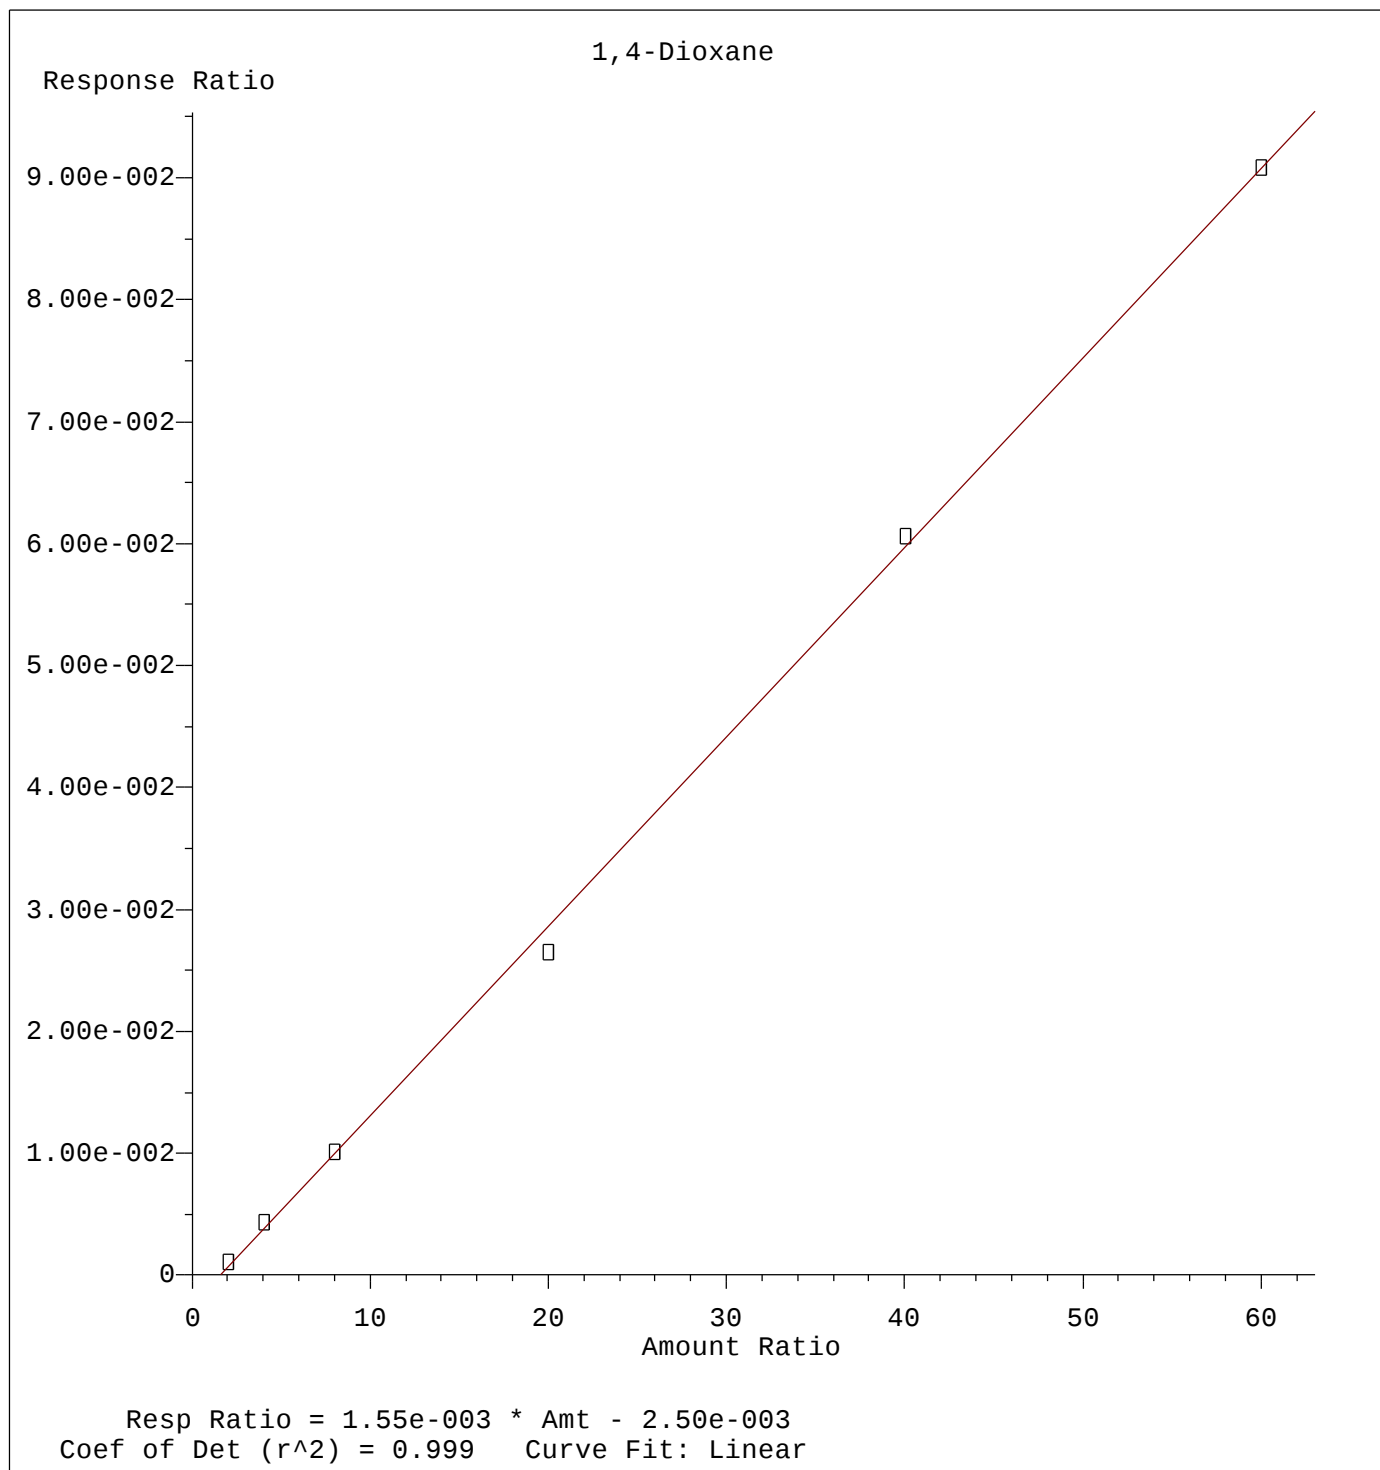

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
Calibration Table Last Updated: Sat Aug 04 07:08:36 2018

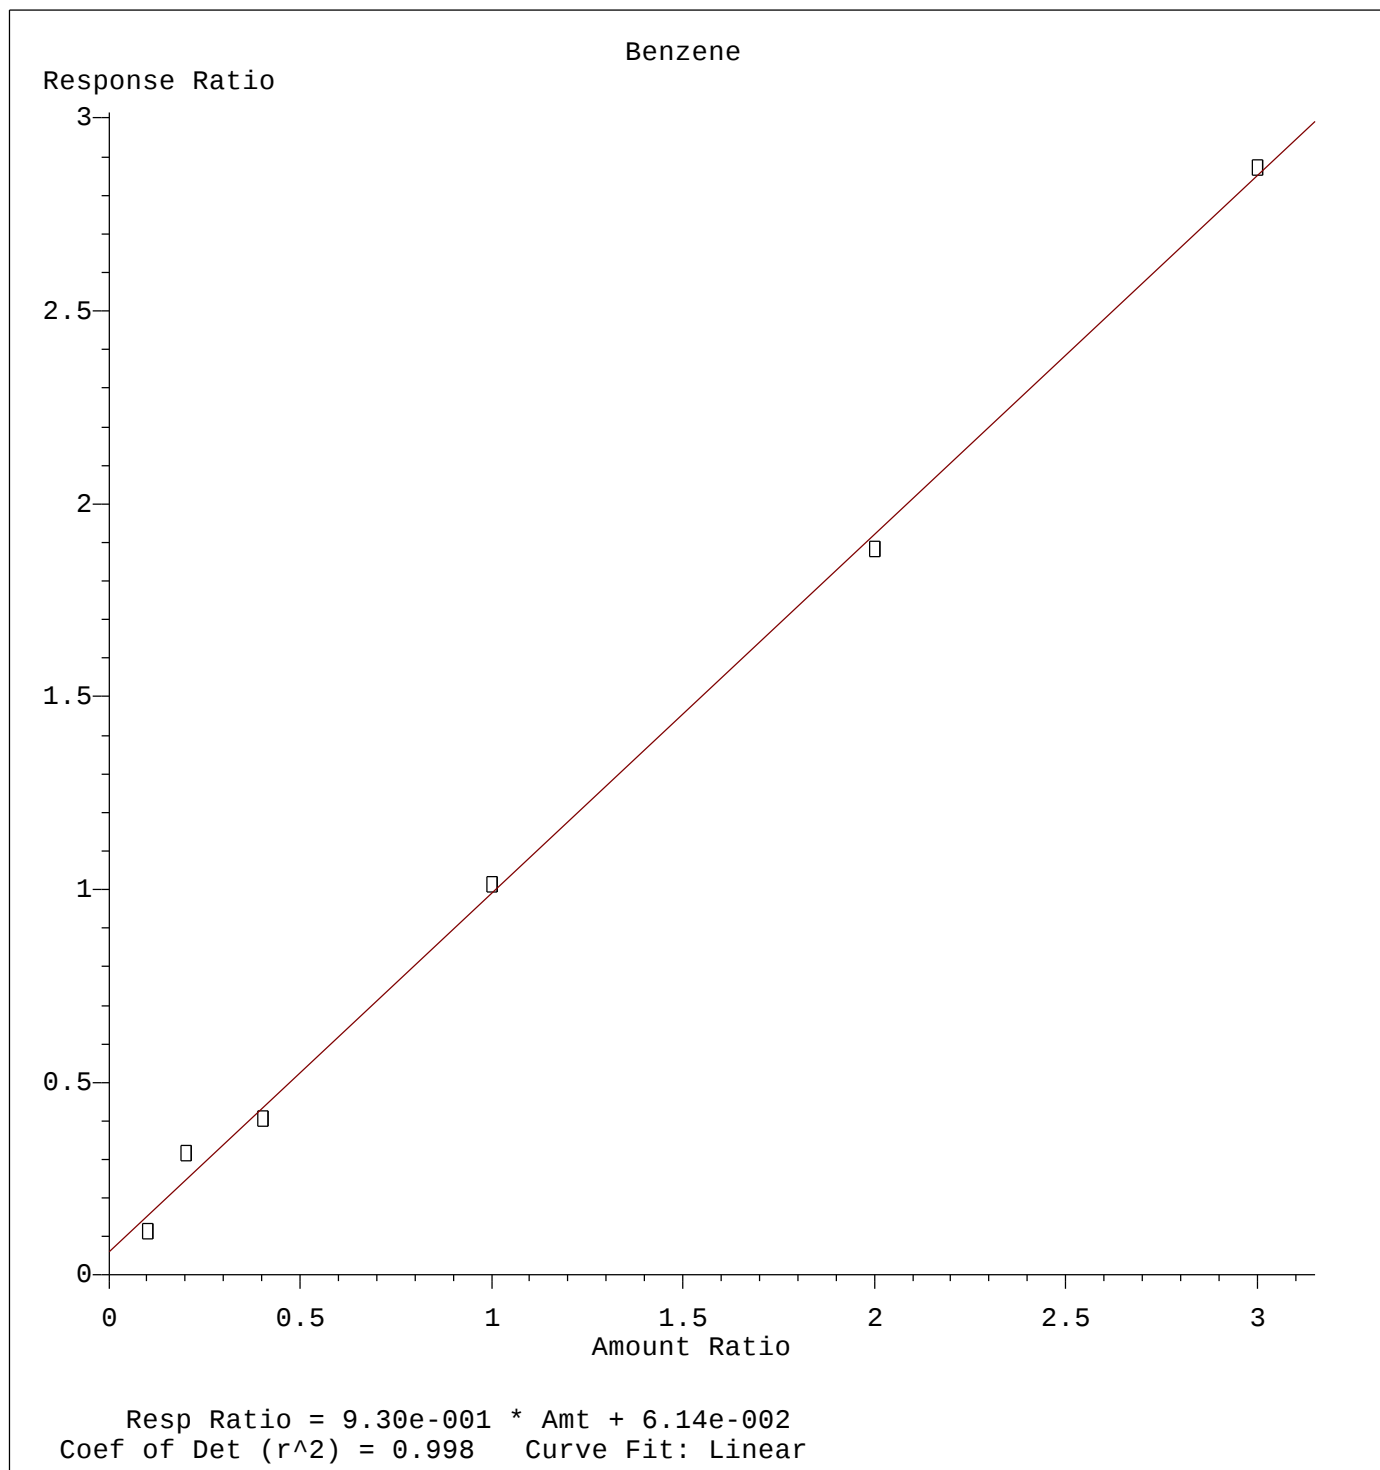

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
Calibration Table Last Updated: Sat Aug 04 07:08:36 2018