


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF080418\
 Data File : VF059861.D
 Acq On : 4 Aug 2018 1:58
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
 Title : SW846 8260
 Last Update : Sat Aug 04 07:08:36 2018

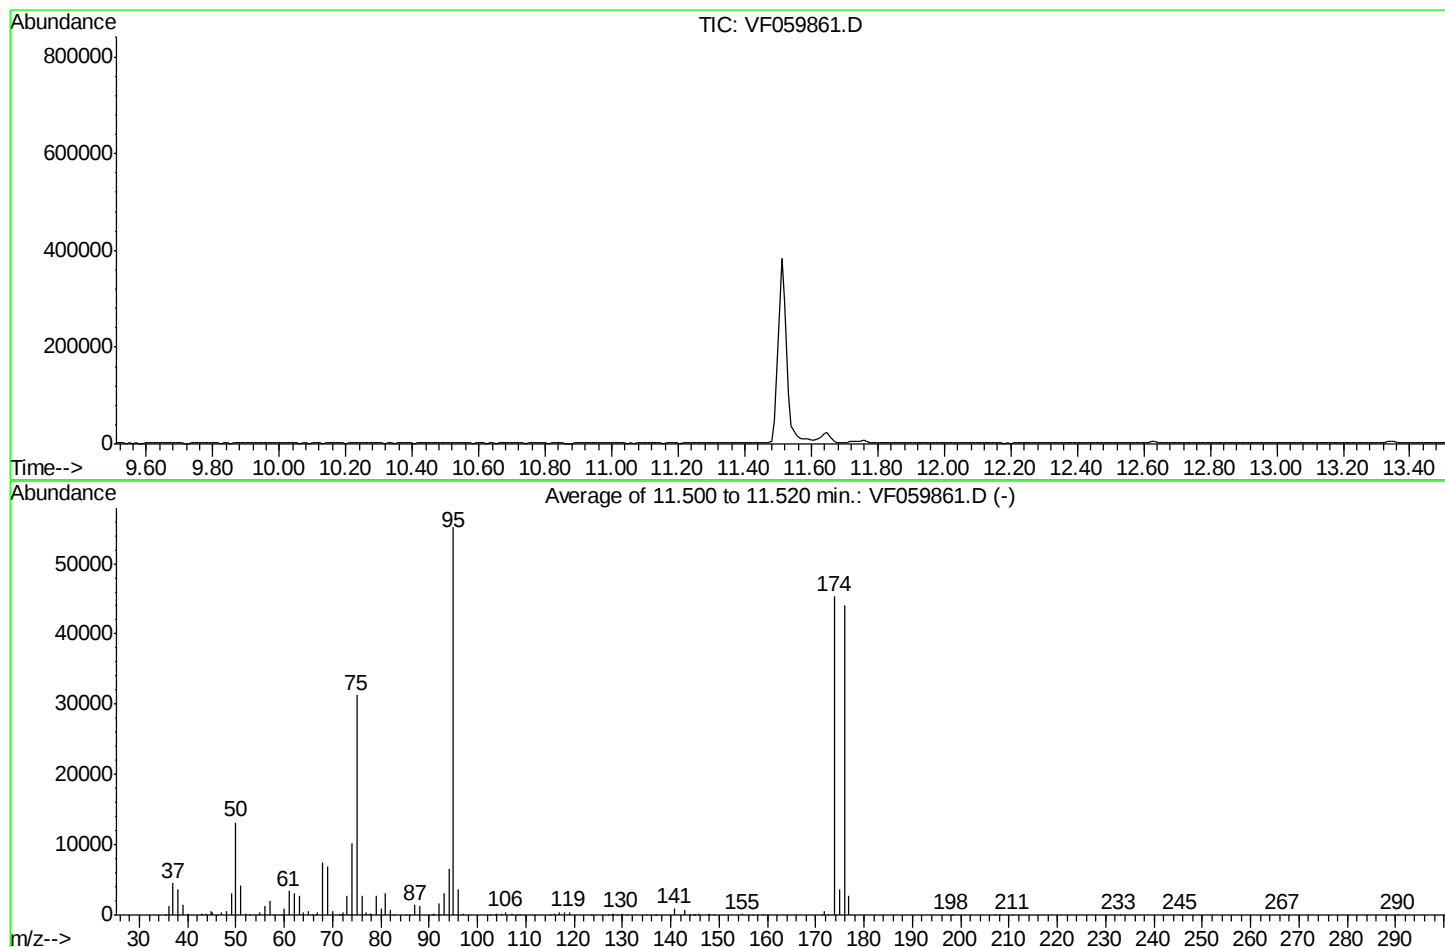

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1108

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	13197	PASS
75	95	30	60	56.7	31285	PASS
95	95	100	100	100.0	55170	PASS
96	95	5	9	6.7	3695	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.1	45306	PASS
175	174	5	9	8.1	3648	PASS
176	174	95	101	97.4	44120	PASS
177	176	5	9	6.2	2731	PASS