


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF080618\
 Data File : VF059882.D
 Acq On : 6 Aug 2018 17:11
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
 Title : SW846 8260
 Last Update : Sat Aug 04 07:08:36 2018

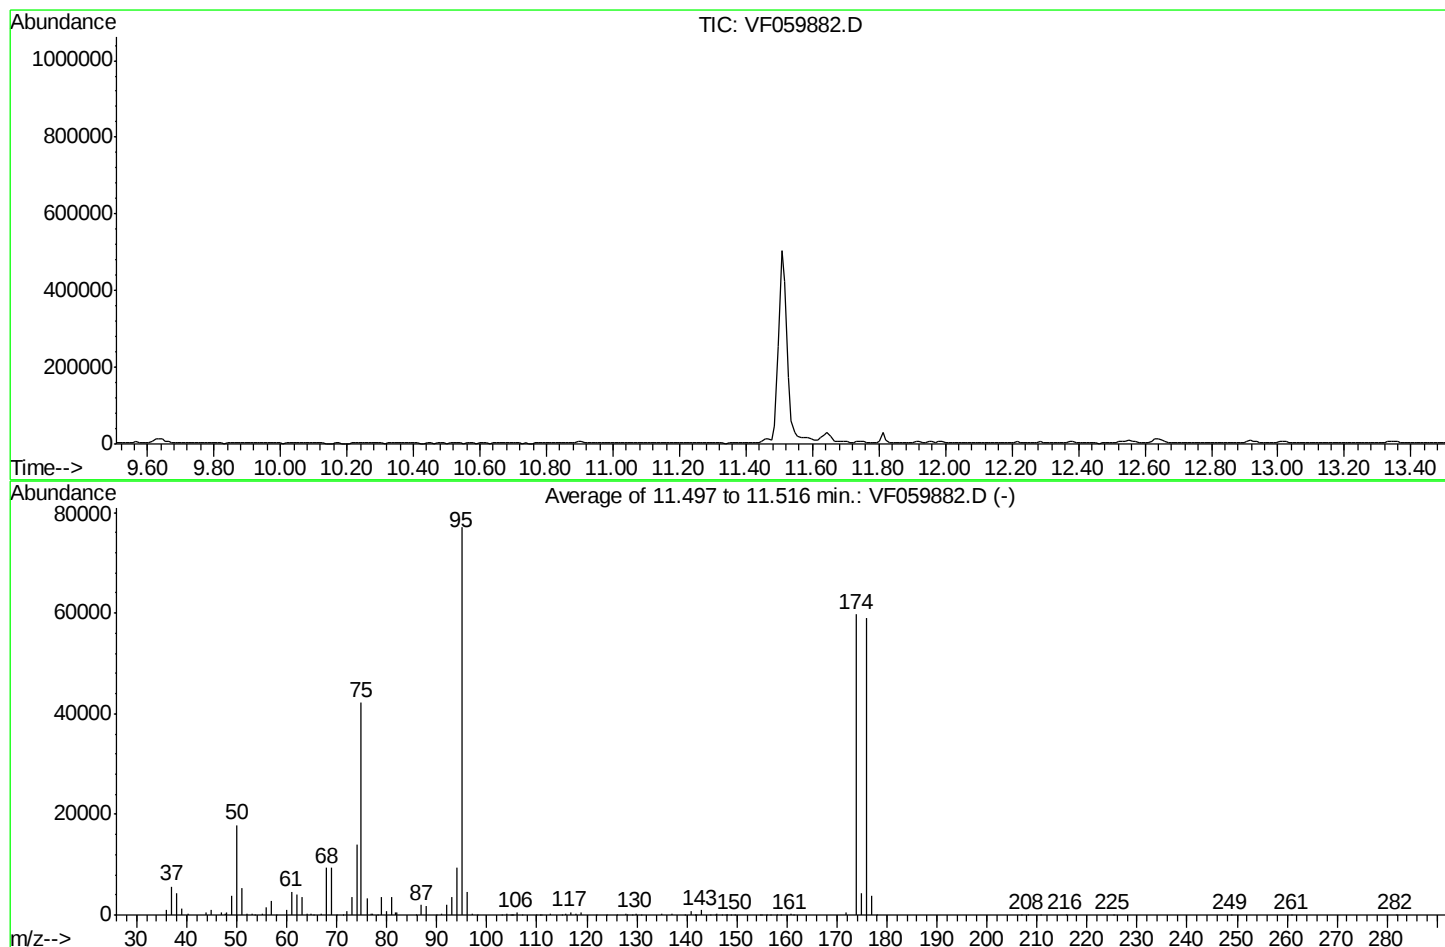

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	17818	PASS
75	95	30	60	54.8	42216	PASS
95	95	100	100	100.0	77050	PASS
96	95	5	9	6.0	4626	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.5	59701	PASS
175	174	5	9	7.2	4284	PASS
176	174	95	101	98.8	58962	PASS
177	176	5	9	6.7	3942	PASS