

Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF080718\
 Data File : VF059922.D
 Acq On : 7 Aug 2018 14:52
 Operator : VA/AP
 Sample : J4348-01RE
 Misc : 4.89g/5mL/MSVOA F/SOIL
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 72-11930RE

Quant Time: Aug 07 15:49:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 04 07:08:36 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.07	168	80	50.00	ug/l	0.03
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-5.77
63) Chlorobenzene-d5	10.07	117	59	50.00	ug/l	0.14
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.63

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.00	65	88	61.01	ug/l	-0.02
Spiked Amount			Recovery	=	122.02%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount			Recovery	=	0.00%	
50) Toluene-d8	7.71	98	108	0.00	ug/l	0.00
Spiked Amount			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	11.60	95	109	0.00	ug/l	0.09
Spiked Amount			Recovery	=	0.00%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.17	50	82	129.69	ug/l #	42
6) Chloroethane	1.39	64	106	260.55	ug/l #	41
8) Diethyl Ether	1.75	74	62	220.39	ug/l #	1
9) 1,1,2-Trichlorotrifluoroet	1.98	101	76	77.69	ug/l #	20
10) Methyl Iodide	1.93	142	76	50.57	ug/l #	1
11) Tert butyl alcohol	2.69	59	247	4245.74	ug/l #	74
12) 1,1-Dichloroethene	1.99	96	70	97.96	ug/l #	1
13) Acrolein	2.23	56	92	2638.80	ug/l #	9
14) Allyl chloride	2.20	41	86	72.18	ug/l #	1
15) Acrylonitrile	2.98	53	83	778.59	ug/l #	13
16) Acetone	2.36	43	72	270.42	ug/l #	70
17) Carbon Disulfide	1.87	76	88	46.13	ug/l #	70
18) Methyl Acetate	2.46	43	136	302.79	ug/l #	56
19) Methyl tert-butyl Ether	2.47	73	59	29.16	ug/l #	59
20) Methylene Chloride	2.30	84	77	125.40	ug/l #	1
21) trans-1,2-Dichloroethene	2.36	96	64	90.16	ug/l #	1
22) Diisopropyl ether	2.92	45	61	26.61	ug/l #	52
23) Vinyl Acetate	3.45	43	150	135.19	ug/l #	80
25) 2-Butanone	4.46	43	75	259.06	ug/l #	60
26) 2,2-Dichloropropane	3.74	77	158	162.60	ug/l #	66
27) cis-1,2-Dichloroethene	3.52	96	80	100.23	ug/l #	1
28) Bromochloromethane	3.75	49	67	113.67	ug/l #	6
29) Tetrahydrofuran	4.23	42	72	675.54	ug/l #	38
30) Chloroform	4.04	83	74	32.77	ug/l #	20
31) Cyclohexane	3.94	56	64	77.47	ug/l #	18
32) 1,1,1-Trichloroethane	4.34	97	73	40.41	ug/l #	22
69) o-Xylene	10.88	106	72	94.24	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF080718\
Data File : VF059922.D
Acq On : 7 Aug 2018 14:52
Operator : VA/AP
Sample : J4348-01RE
Misc : 4.89g/5mL/MSVOA F/SOIL
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
72-11930RE

Quant Time: Aug 07 15:49:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F080418S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 04 07:08:36 2018
Response via : Initial Calibration

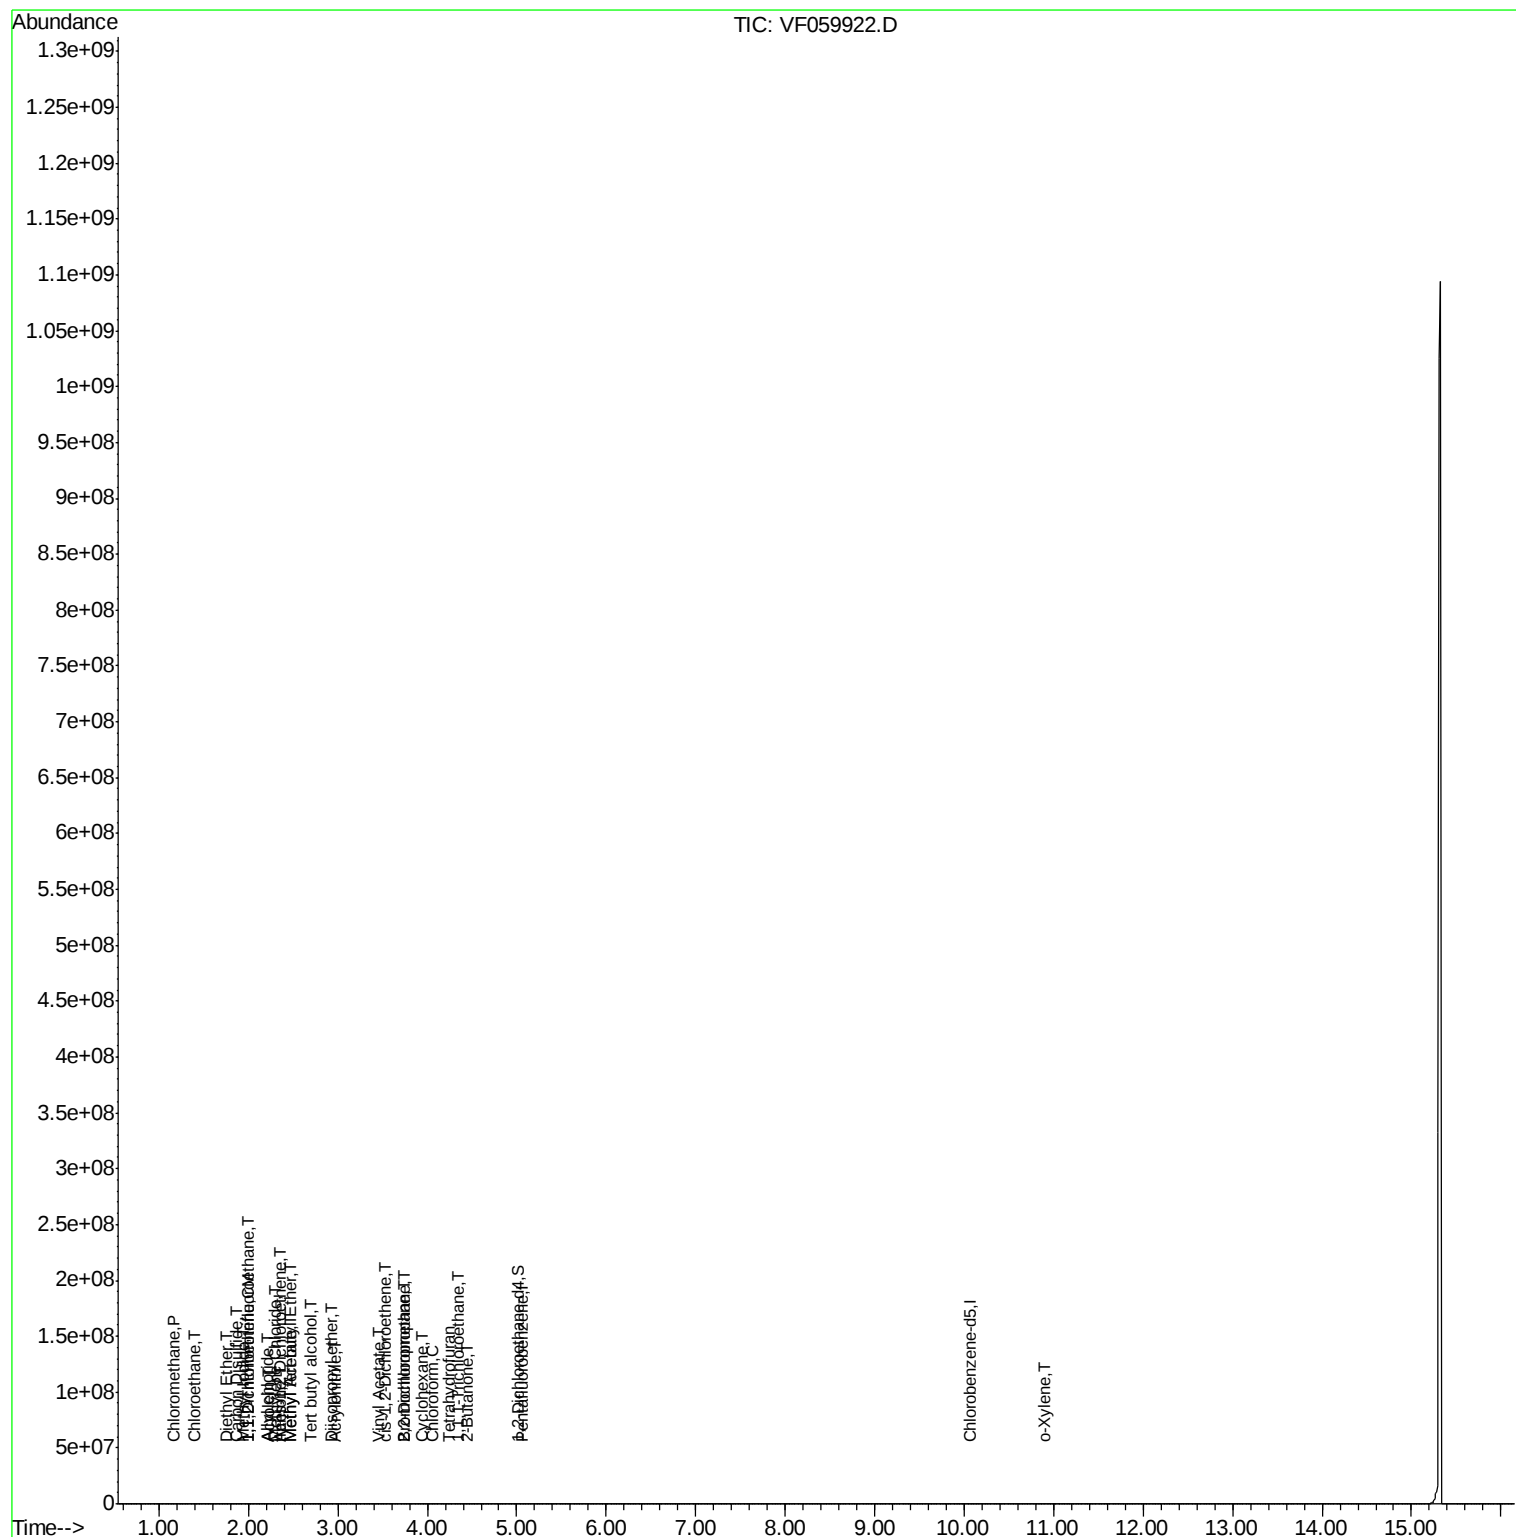



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.07 min Scan# 460

Delta R.T. 0.03 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampled :


72-11930RE

Tot Ion:168 Resp: 80

Ion Ratio Lower Upper

168 100

99 0.0 66.3 99.5#



Abundance Ion 168.00 (167.70 to 168.70): VF0

Ion 99.00 (98.70 to 99.70): VF0

5.07

150



100

50

0

Time-->

5.04 5.06 5.08 5.10



#3

Chloromethane

Concen: 129.69 ug/l

RT: 1.17 min Scan# 64

Delta R.T. 0.07 min

Lab File: VF059922.D


Acq: 7 Aug 2018 14:52

Tgt Ion: 50 Resp: 82

Ion Ratio Lower Upper

50 100

52 0.0 25.8 38.8#



Abundance Ion 50.00 (49.70 to 50.70): VF0

Ion 52.00 (51.70 to 52.70): VF0

1.17

150


100


50

0

Time-->

1.14 1.16 1.18





#6

Chloroethane

Concen: 260.55 ug/l

RT: 1.39 min Scan# 87

Delta R.T. -0.03 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampleId :


72-11930RE

Tot Ion: 64 Resp: 106




Ion Ratio Lower Upper

64 100

66 0.0 26.9 40.3#



Abundance Ion 64.00 (63.70 to 64.70): VF0

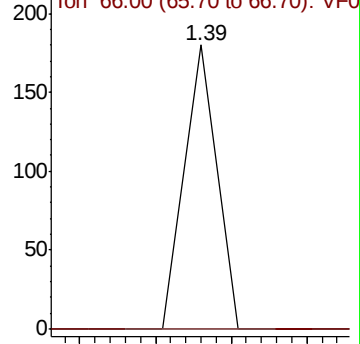

#8

Diethyl Ether

Concen: 220.39 ug/l

RT: 1.75 min Scan# 123

Delta R.T. 0.04 min

Lab File: VF059922.D


Acq: 7 Aug 2018 14:52

Tgt Ion: 74 Resp: 62



Ion Ratio Lower Upper


74 100

45 0.0 73.6 220.7#



Abundance Ion 74.00 (73.70 to 74.70): VF0

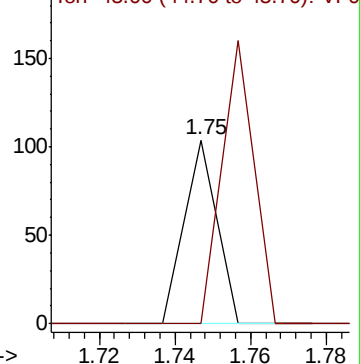



#9

1,1,2-Trichlorotrifluoroethane

Concen: 77.69 ug/l

RT: 1.98 min Scan# 147

Delta R.T. 0.07 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampleId :

72-11930RE


Tot Ion:101 Resp: 76

Ion Ratio Lower Upper

101 100

85 0.0 44.5 66.7#




151 0.0 53.8 80.8#



Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VF0

Ion 151.00 (150.70 to 151.70): V

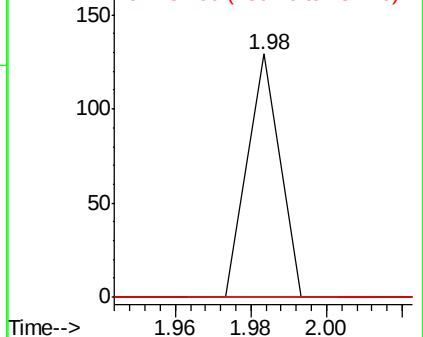

#10

Methyl Iodide

Concen: 50.57 ug/l

RT: 1.93 min Scan# 142

Delta R.T. -0.03 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52


Tgt Ion:142 Resp: 76

Ion Ratio Lower Upper

142 100

127 0.0 61.5 92.3#



141 100.0 13.0 19.4#




Abundance Ion 142.00 (141.70 to 142.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 141.00 (140.70 to 141.70): V

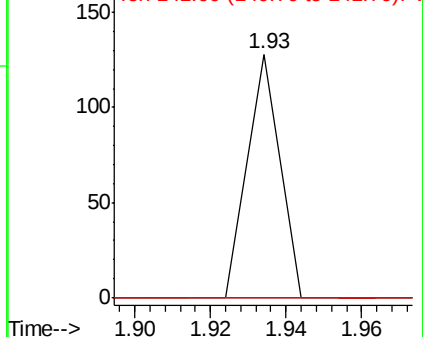







#11

Tert butyl alcohol
 Concen: 4245.74 ug/l
 RT: 2.69 min Scan# 219
 Delta R.T. 0.01 min
 Lab File: VF059922.D
 Acq: 7 Aug 2018 14:52

Instrument :
 MSVOA_F
 ClientSampleId :
 72-11930RE




Tot Ion: 59 Resp: 247
 Ion Ratio Lower Upper
 59 100
 57 0.0 7.6 11.4#

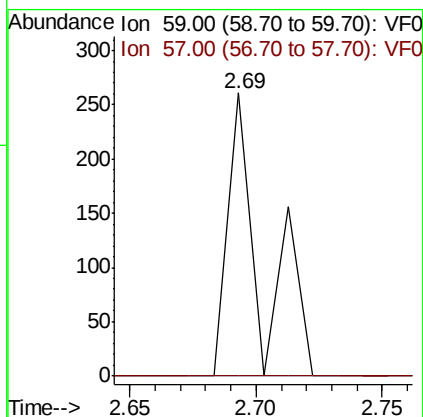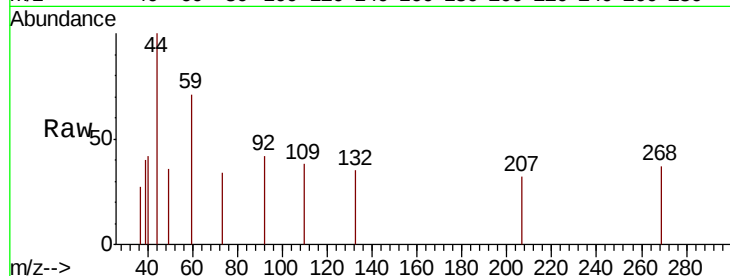


#12

1,1-Dichloroethene
 Concen: 97.96 ug/l
 RT: 1.99 min Scan# 148
 Delta R.T. 0.13 min
 Lab File: VF059922.D
 Acq: 7 Aug 2018 14:52

Tgt Ion: 96 Resp: 70
 Ion Ratio Lower Upper
 96 100
 61 0.0 230.2 345.2#
 98 0.0 52.7 79.1#

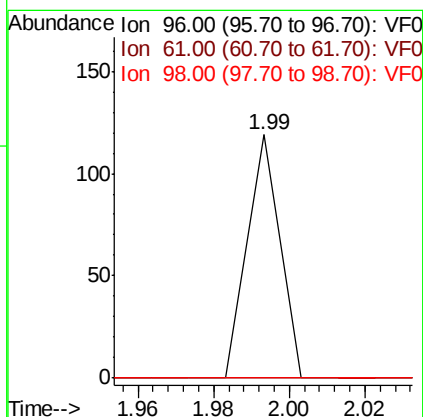



#13

Acrolein

Concen: 2638.80 ug/l

RT: 2.23 min Scan# 172

Delta R.T. 0.14 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampleId :





72-11930RE

Tot Ion: 56 Resp: 92

Ion Ratio Lower Upper

56 100

55 0.0 64.6 96.8#

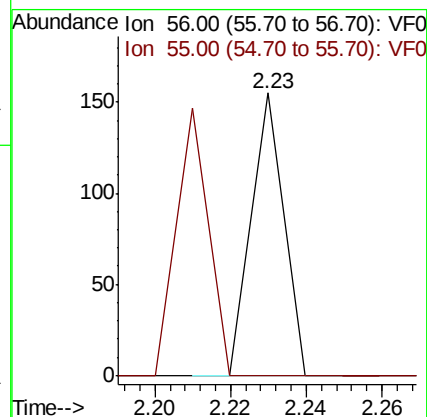

#14

Allyl chloride

Concen: 72.18 ug/l

RT: 2.20 min Scan# 169

Delta R.T. 0.02 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52




Tgt Ion: 41 Resp: 86


Ion Ratio Lower Upper

41 100

39 0.0 114.6 171.8#

76 0.0 21.0 31.4#

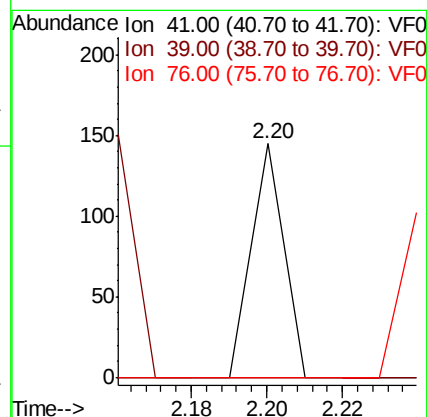

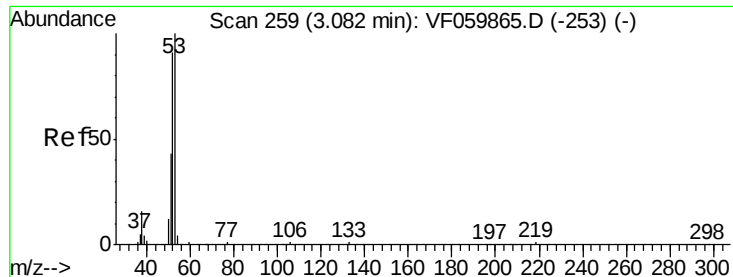

#15

Acrylonitrile

Concen: 778.59 ug/l

RT: 2.98 min Scan# 248

Delta R.T. -0.10 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampleId :

72-11930RE


Tot Ion: 53 Resp: 83

Ion Ratio Lower Upper

53 100

52 0.0 72.9 109.3#




51 0.0 34.5 51.7#

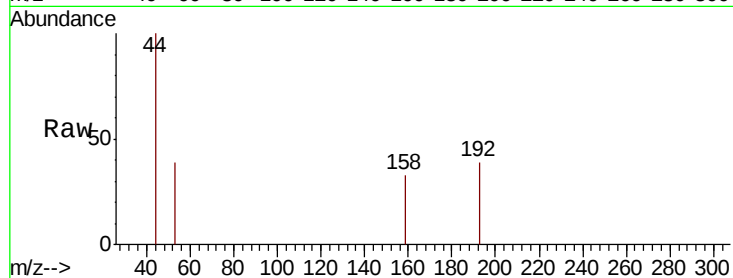

Abundance Ion 53.00 (52.70 to 53.70): VF0

Ion 52.00 (51.70 to 52.70): VF0

Ion 51.00 (50.70 to 51.70): VF0

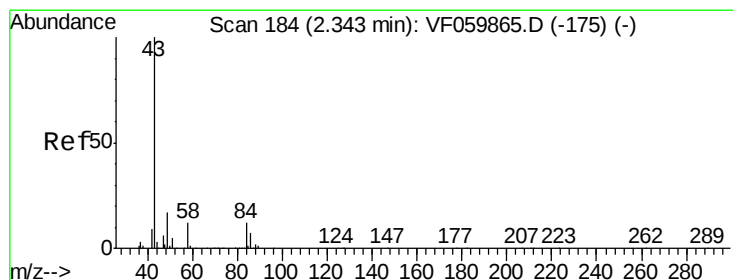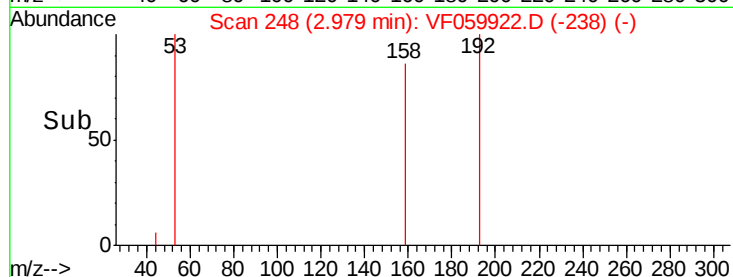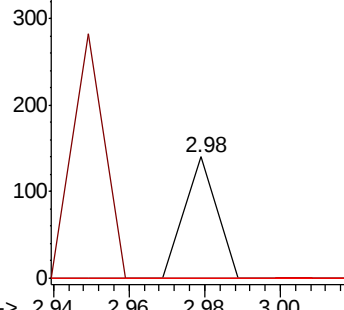

#16

Acetone

Concen: 270.42 ug/l

RT: 2.36 min Scan# 185

Delta R.T. 0.02 min

Lab File: VF059922.D


Acq: 7 Aug 2018 14:52

Tgt Ion: 43 Resp: 72

Ion Ratio Lower Upper



43 100


58 0.0 9.4 14.0#

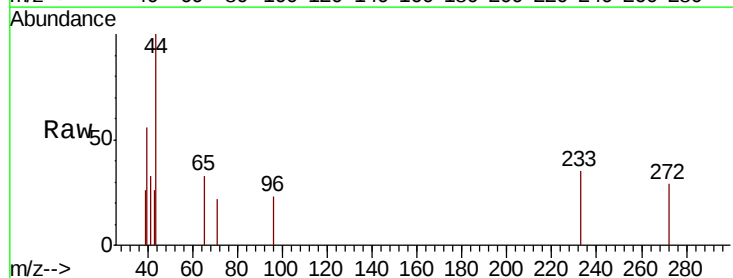

Abundance Ion 43.00 (42.70 to 43.70): VF0

Ion 58.00 (57.70 to 58.70): VF0



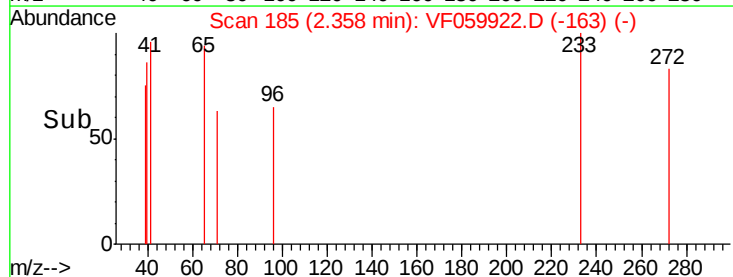
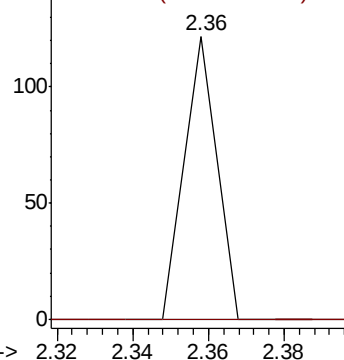


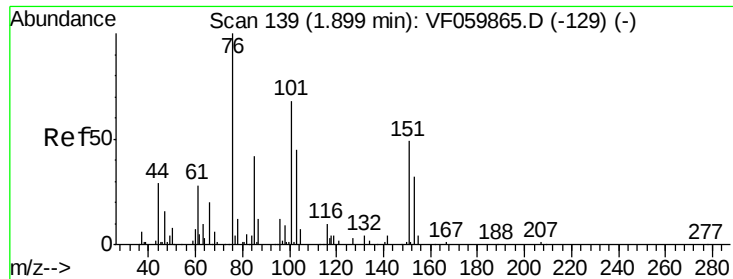

#17
Carbon Disulfide
Concen: 46.13 ug/l
RT: 1.87 min Scan# 136
Delta R.T. -0.02 min
Lab File: VF059922.D
Acq: 7 Aug 2018 14:52




Instrument :
MSVOA_F
ClientSampleId :
72-11930RE


Tot Ion: 76 Resp: 88
Ion Ratio Lower Upper
76 100
78 0.0 9.3 13.9#

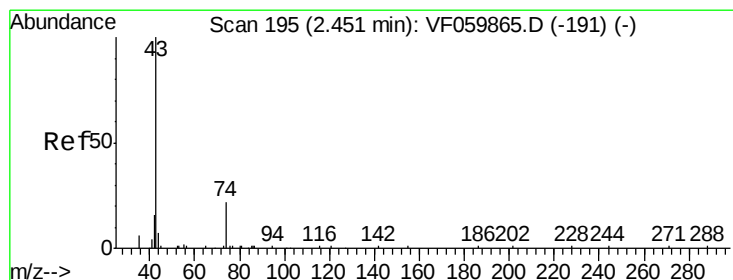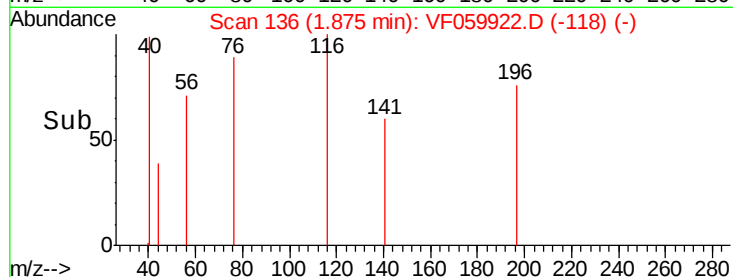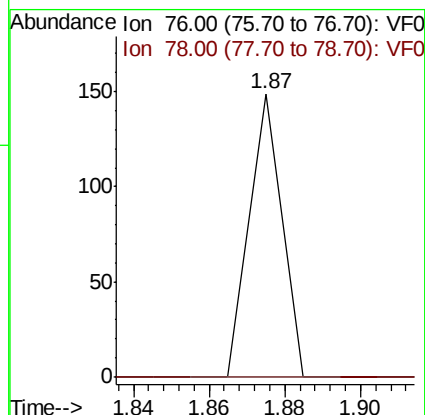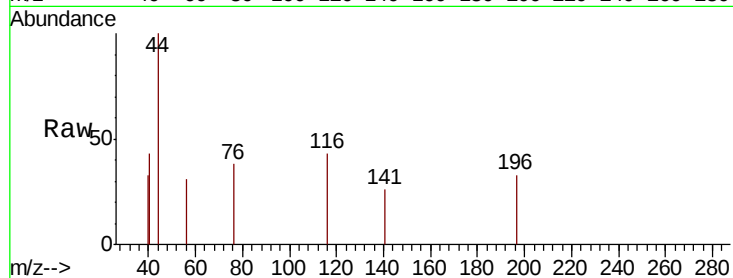

#18
Methyl Acetate
Concen: 302.79 ug/l
RT: 2.46 min Scan# 195
Delta R.T. 0.01 min
Lab File: VF059922.D
Acq: 7 Aug 2018 14:52

Tgt Ion: 43 Resp: 136
Ion Ratio Lower Upper
43 100
74 0.0 16.3 24.5#

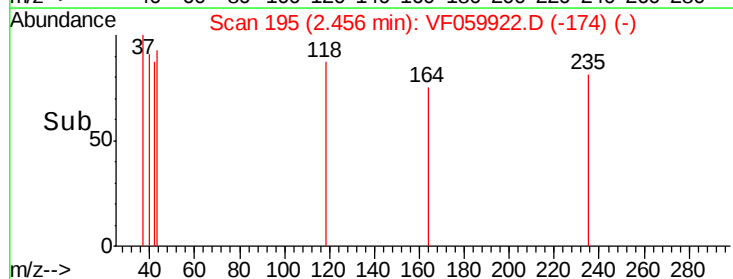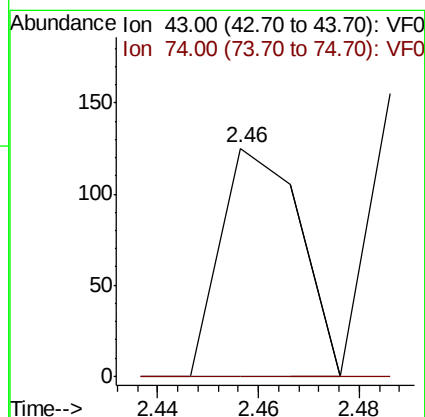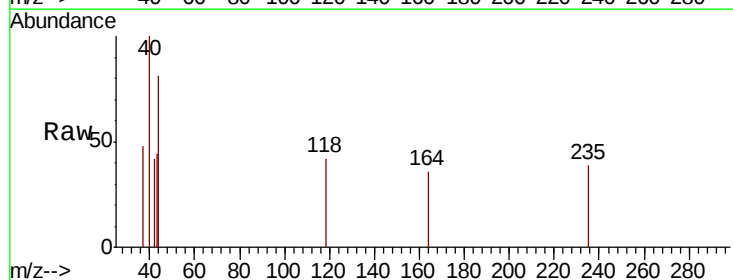







#19

Methyl tert-butyl Ether
 Concen: 29.16 ug/l
 RT: 2.47 min Scan# 196
 Delta R.T. -0.07 min
 Lab File: VF059922.D
 Acq: 7 Aug 2018 14:52

Instrument :
 MSVOA_F
 ClientSampleID :
 72-11930RE




Tot Ion: 73 Resp: 59
 Ion Ratio Lower Upper
 73 100
 57 0.0 14.3 21.5#

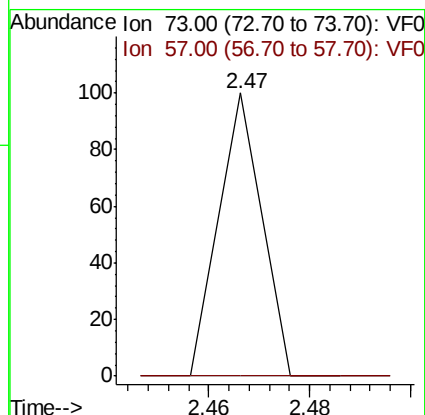


#20

Methylene Chloride
 Concen: 125.40 ug/l
 RT: 2.30 min Scan# 179
 Delta R.T. 0.02 min
 Lab File: VF059922.D
 Acq: 7 Aug 2018 14:52

Tgt Ion: 84 Resp: 77
 Ion Ratio Lower Upper
 84 100
 49 0.0 128.7 193.1#
 51 0.0 39.3 58.9#
 86 0.0 55.9 83.9#

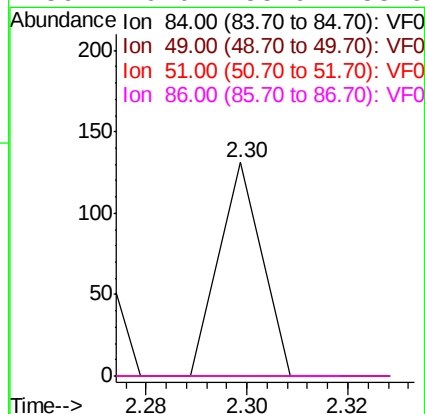



#21

trans-1,2-Dichloroethene

Concen: 90.16 ug/l

RT: 2.36 min Scan# 185

Delta R.T. -0.05 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampleId :

72-11930RE


Tot Ion: 96 Resp: 64

Ion Ratio Lower Upper




96 100

61 0.0 158.2 237.4#

98 0.0 52.0 78.0#

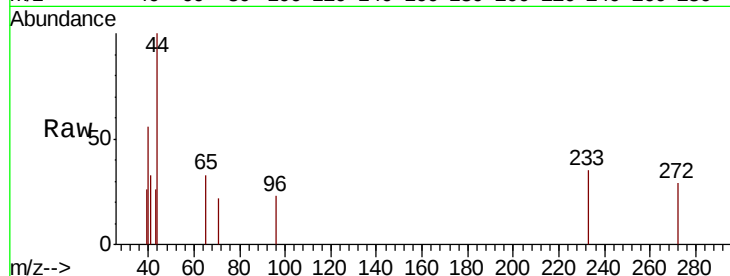

Abundance Ion 96.00 (95.70 to 96.70): VF0
Ion 61.00 (60.70 to 61.70): VF0
Ion 98.00 (97.70 to 98.70): VF0

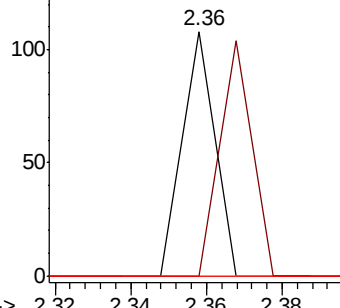

#22

Diisopropyl ether

Concen: 26.61 ug/l

RT: 2.92 min Scan# 242

Delta R.T. -0.00 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Tgt Ion: 45 Resp: 61


Ion Ratio Lower Upper

45 100



43 106.8 52.1 78.1#


87 0.0 13.8 20.8#

59 0.0 7.5 11.3#



Abundance Ion 45.00 (44.70 to 45.70): VF0
Ion 43.00 (42.70 to 43.70): VF0
Ion 87.00 (86.70 to 87.70): VF0
Ion 59.00 (58.70 to 59.70): VF0




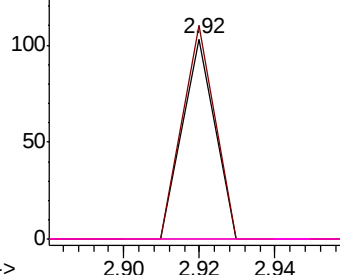




#23
 Vinyl Acetate
 Concen: 135.19 ug/l
 RT: 3.45 min Scan# 296
 Delta R.T. 0.11 min
 Lab File: VF059922.D
 Acq: 7 Aug 2018 14:52




Instrument :
 MSVOA_F
 ClientSampleId :
 72-11930RE


Tot Ion: 43 Resp: 150
 Ion Ratio Lower Upper
 43 100
 86 0.0 5.6 8.4#

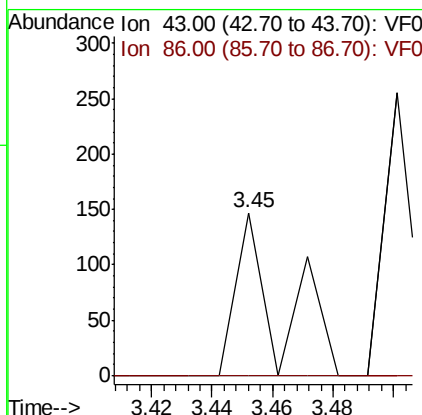

#25
 2-Butanone
 Concen: 259.06 ug/l
 RT: 4.46 min Scan# 398
 Delta R.T. -0.05 min
 Lab File: VF059922.D
 Acq: 7 Aug 2018 14:52

Tgt Ion: 43 Resp: 75
 Ion Ratio Lower Upper
 43 100
 72 0.0 13.9 20.9#

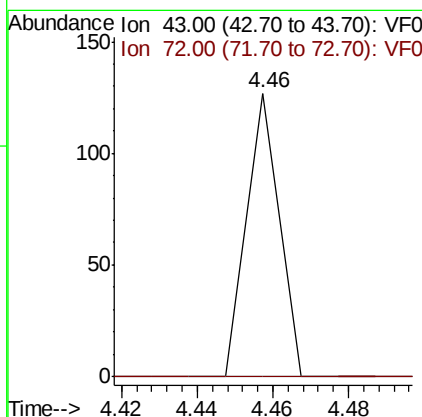



#26

2,2-Dichloropropane

Concen: 162.60 ug/l

RT: 3.74 min Scan# 325

Delta R.T. -0.03 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampleId :





72-11930RE

Tot Ion: 77 Resp: 158

Ion Ratio Lower Upper

77 100

97 0.0 6.8 20.3#

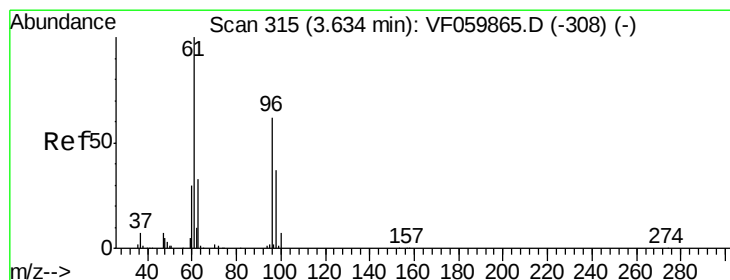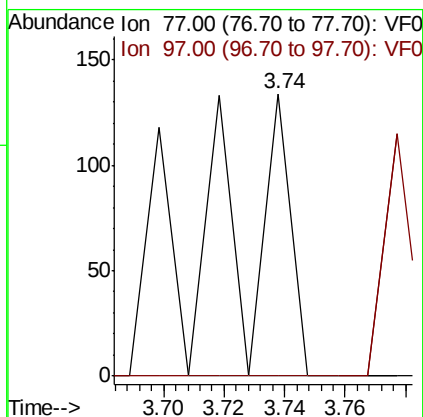

#27

cis-1,2-Dichloroethene

Concen: 100.23 ug/l

RT: 3.52 min Scan# 303

Delta R.T. -0.11 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52




Tgt Ion: 96 Resp: 80


Ion Ratio Lower Upper

96 100

61 0.0 0.0 320.8

98 0.0 0.0 117.6

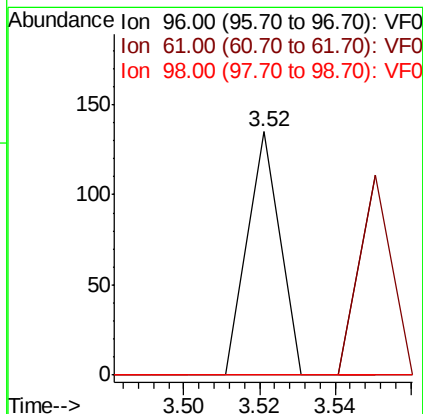



#28

Bromochloromethane

Concen: 113.67 ug/l

RT: 3.75 min Scan# 326

Delta R.T. -0.14 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampled :

72-11930RE


Tot Ion: 49 Resp: 67

Ion Ratio Lower Upper

49 100

129 0.0 0.0 4.6




130 0.0 73.8 110.8#

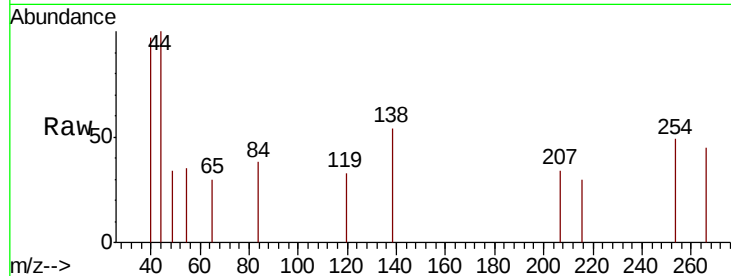

Abundance Ion 49.00 (48.70 to 49.70): VF0

Ion 129.00 (128.70 to 129.70): V

Ion 130.00 (129.70 to 130.70): V

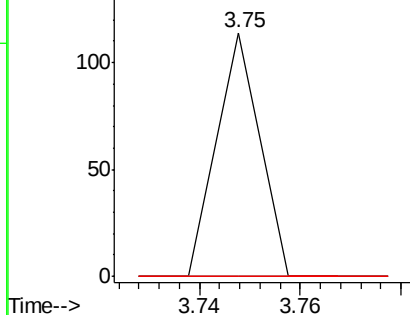

#29

Tetrahydrofuran

Concen: 675.54 ug/l

RT: 4.23 min Scan# 375

Delta R.T. -0.02 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52


Tgt Ion: 42 Resp: 72

Ion Ratio Lower Upper

42 100

72 0.0 29.3 43.9#



71 0.0 30.0 45.0#




Abundance Ion 42.00 (41.70 to 42.70): VF0

Ion 72.00 (71.70 to 72.70): VF0

Ion 71.00 (70.70 to 71.70): VF0




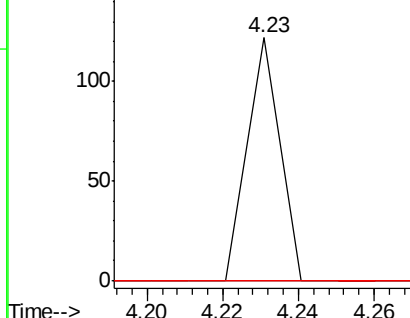




#30
Chloroform
Concen: 32.77 ug/l
RT: 4.04 min Scan# 356
Delta R.T. 0.01 min
Lab File: VF059922.D
Acq: 7 Aug 2018 14:52




Instrument :
MSVOA_F
ClientSampled :
72-11930RE


Tot Ion: 83 Resp: 74
Ion Ratio Lower Upper
83 100
85 0.0 49.3 73.9#

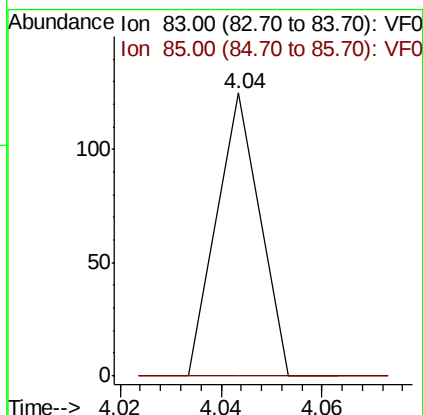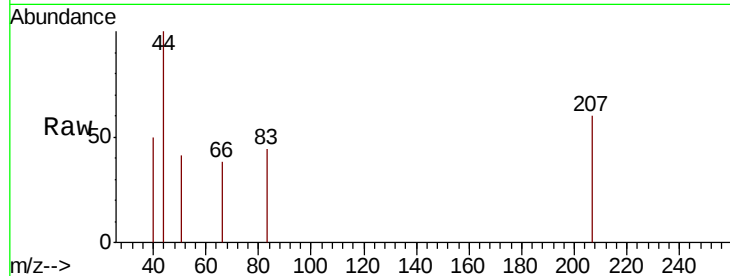

#31
Cyclohexane
Concen: 77.47 ug/l
RT: 3.94 min Scan# 345
Delta R.T. 0.07 min
Lab File: VF059922.D
Acq: 7 Aug 2018 14:52

Tgt Ion: 56 Resp: 64
Ion Ratio Lower Upper
56 100
69 0.0 26.7 40.1#
84 0.0 65.9 98.9#

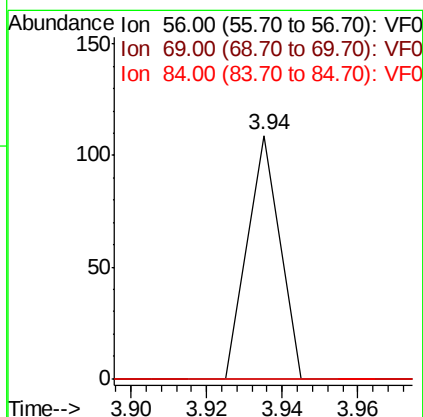



#32

1,1,1-Trichloroethane

Concen: 40.41 ug/l

RT: 4.34 min Scan# 386

Delta R.T. 0.06 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampleId :

72-11930RE





Tot Ion: 97 Resp: 73

Ion Ratio Lower Upper

97 100

99 0.0 51.4 77.2#

61 0.0 40.8 61.2#

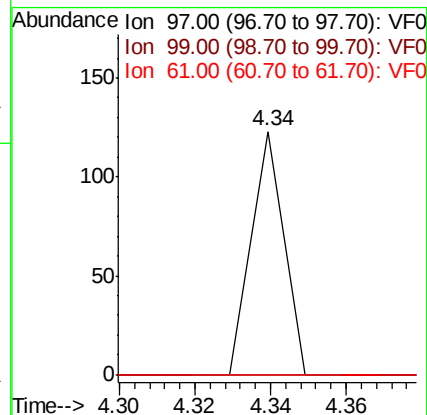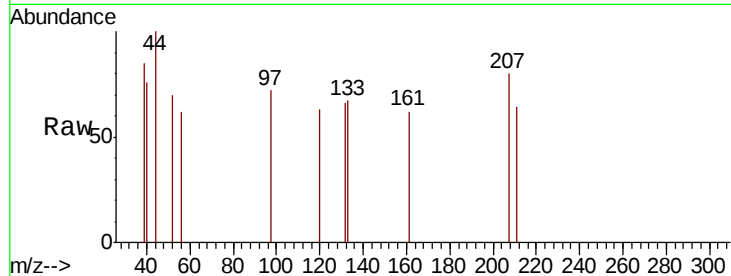

#33

1,2-Dichloroethane-d4

Concen: 61.01 ug/l

RT: 5.00 min Scan# 453

Delta R.T. -0.02 min

Lab File: VF059922.D




Acq: 7 Aug 2018 14:52


Tgt Ion: 65 Resp: 88

Ion Ratio Lower Upper

65 100

67 0.0 0.0 77.2

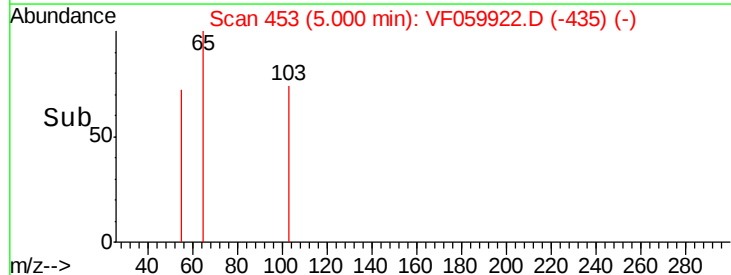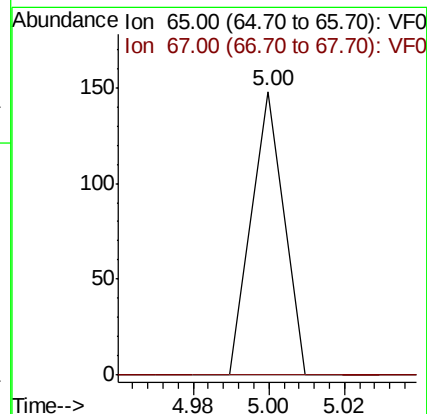

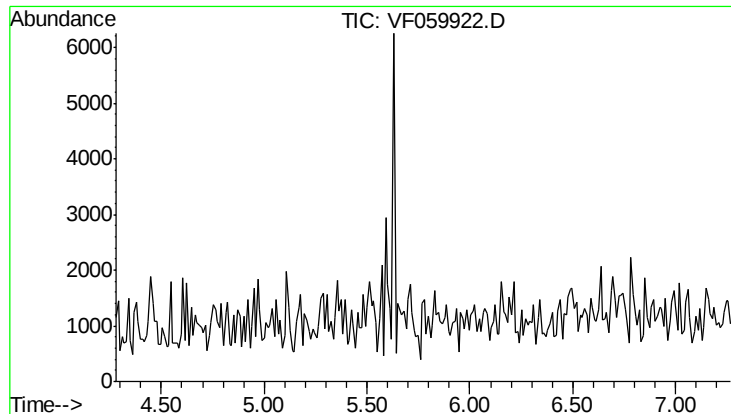

#34

1,4-Difluorobenzene

Concen: 0.00 ug/l

Expected RT: 5.77 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52

Instrument :

MSVOA_F

ClientSampleId :

72-11930RE



Tot Ion: 114

Sig Exp Ratio

114 100

63 24.0

88 19.7

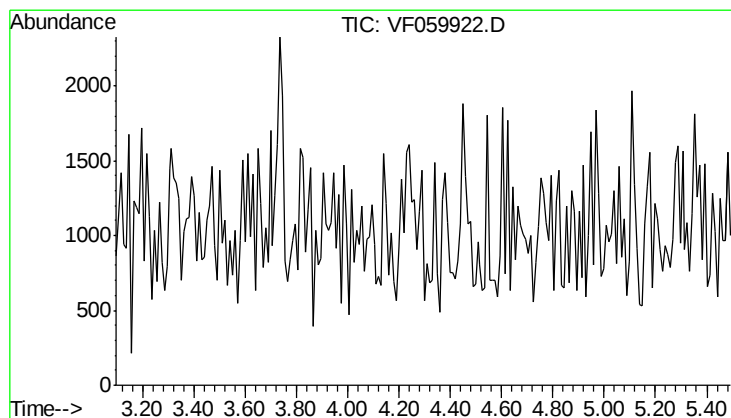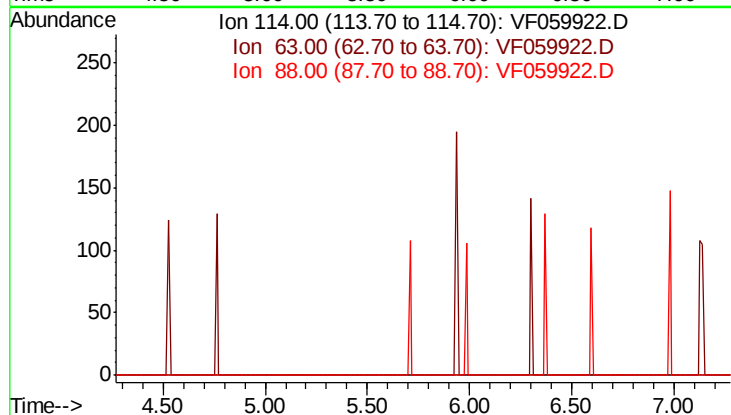

#35

Dibromofluoromethane

Concen: 0.00 ug/l

Expected RT: 4.29 min

Lab File: VF059922.D

Acq: 7 Aug 2018 14:52


Tgt Ion: 113


Sig Exp Ratio

113 100

111 102.3

192 15.5




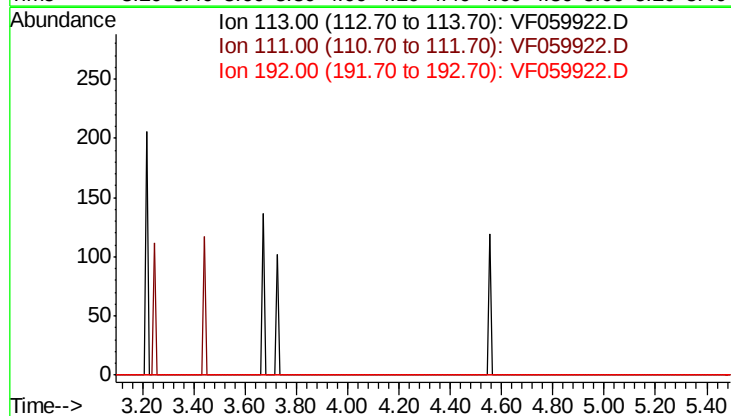




#50
Toluene-d8
Concen: 0.00 ug/l
RT: 7.71 min Scan# 728
Delta R.T. -0.00 min
Lab File: VF059922.D
Acq: 7 Aug 2018 14:52




Instrument :
MSVOA_F
ClientSampleId :
72-11930RE


Tot Ion: 98 Resp: 108
Ion Ratio Lower Upper
98 100
100 0.0 55.0 82.6#

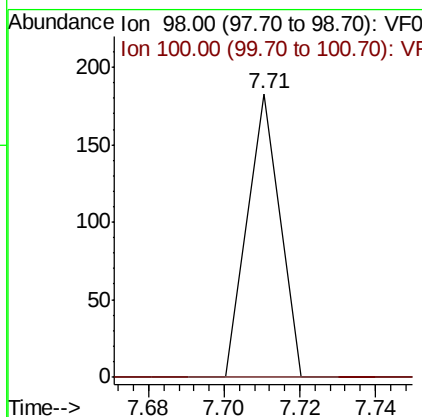

#62
4-Bromofluorobenzene
Concen: 0.00 ug/l
RT: 11.60 min Scan# 1123
Delta R.T. 0.09 min
Lab File: VF059922.D
Acq: 7 Aug 2018 14:52

Tgt Ion: 95 Resp: 109
Ion Ratio Lower Upper
95 100
174 0.0 0.0 151.6
176 0.0 0.0 149.8

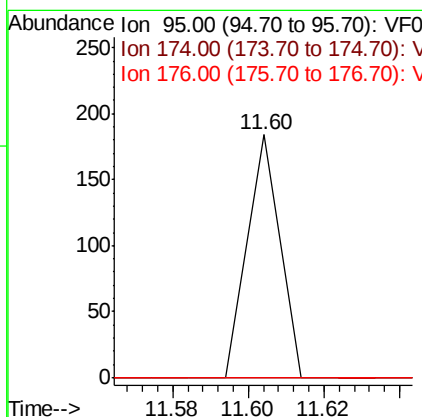







#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.07 min Scan# 967
Delta R.T. 0.14 min
Lab File: VF059922.D
Acq: 7 Aug 2018 14:52

Instrument :
MSVOA_F
ClientSampleId :
72-11930RE

Tot Ion:117 Resp: 59
Ion Ratio Lower Upper
117 100
82 0.0 51.3 76.9#
119 0.0 26.4 39.6#

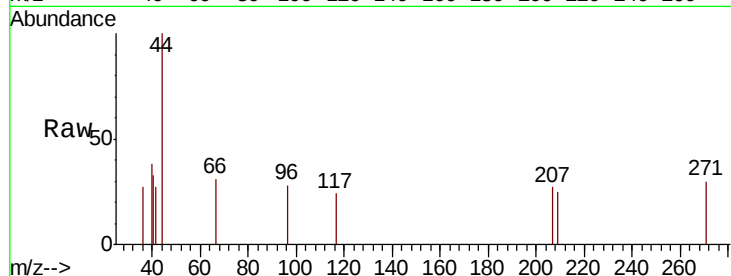


Abundance Ion 117.00 (116.70 to 117.70): V
Ion 82.00 (81.70 to 82.70): VF0
Ion 119.00 (118.70 to 119.70): V


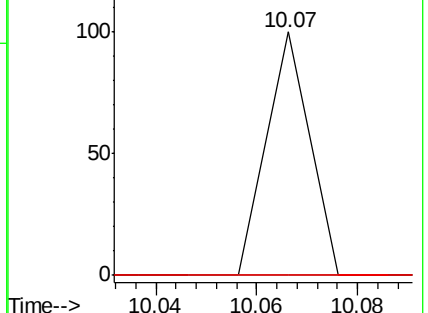



#69
o-Xylene
Concen: 94.24 ug/l
RT: 10.88 min Scan# 1050
Delta R.T. 0.05 min
Lab File: VF059922.D
Acq: 7 Aug 2018 14:52

Tgt Ion:106 Resp: 72
Ion Ratio Lower Upper
106 100
91 0.0 125.4 376.2#



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VF0

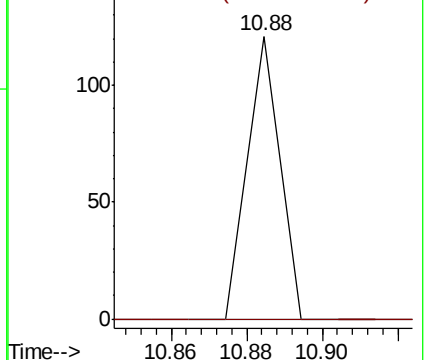

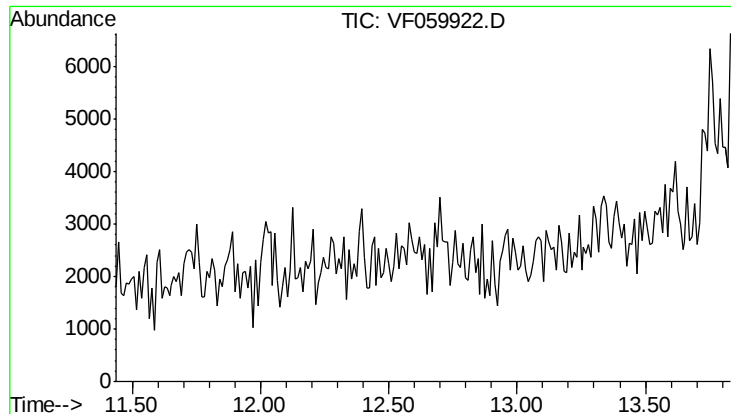

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.00 ug/l
 Expected RT: 12.63 min
 Lab File: VF059922.D
 Acq: 7 Aug 2018 14:52

Instrument :
 MSVOA_F
 ClientSampleId :
 72-11930RE

Tot Ion: 152
 Sig Exp Ratio
 152 100
 115 59.6
 150 157.8

