


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF080718\  
 Data File : VF059905.D  
 Acq On : 7 Aug 2018 5:47  
 Operator : VA/AP  
 Sample : BFB  
 Misc : 5.00µ/5mL/MSVOA F/SOIL  
 ALS Vial : 29 Sample Multiplier: 1

Instrument :  
 MSVOA\_F  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F080418S.M  
 Title : SW846 8260  
 Last Update : Sat Aug 04 07:08:36 2018

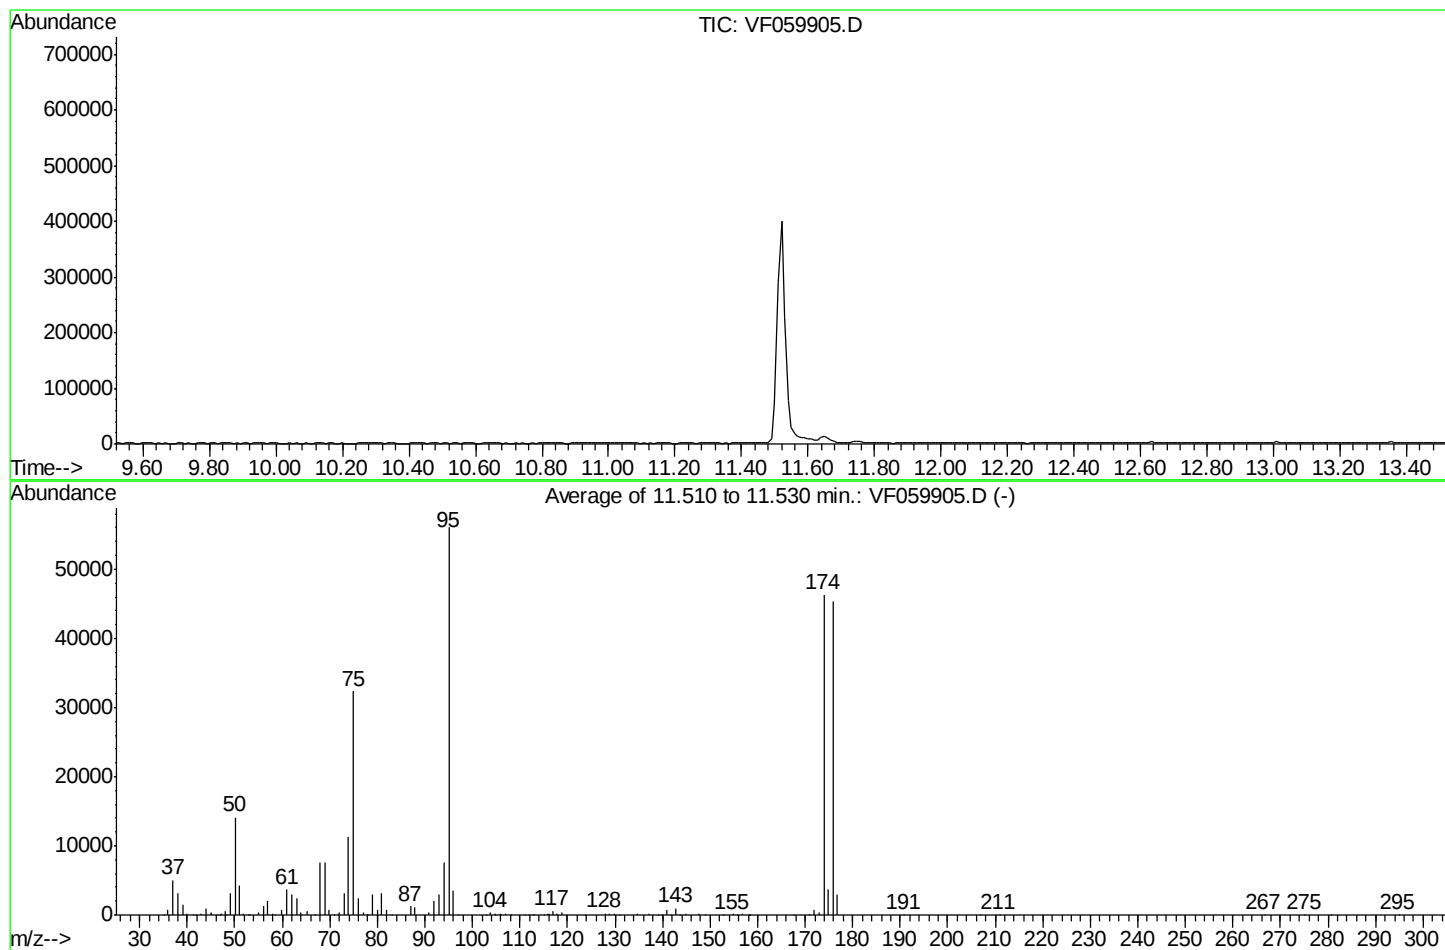

AutoFind: Scans 1114, 1115, 1116; Background Corrected with Scan 1108

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 25.1      | 14070   | PASS             |
| 75          | 95           | 30           | 60           | 57.8      | 32381   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 56058   | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 3542    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 446     | PASS             |
| 174         | 95           | 50           | 100          | 82.6      | 46296   | PASS             |
| 175         | 174          | 5            | 9            | 7.9       | 3670    | PASS             |
| 176         | 174          | 95           | 101          | 97.9      | 45333   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 2974    | PASS             |