


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF081418\  
Data File : VF059951.D  
Acq On : 14 Aug 2018 17:37  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µ/5mL/MSVOA F/SOIL  
ALS Vial : 29 Sample Multiplier: 1

Instrument :  
MSVOA\_F  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F081418S.M  
Title : SW846 8260  
Last Update : Wed Aug 15 09:20:23 2018

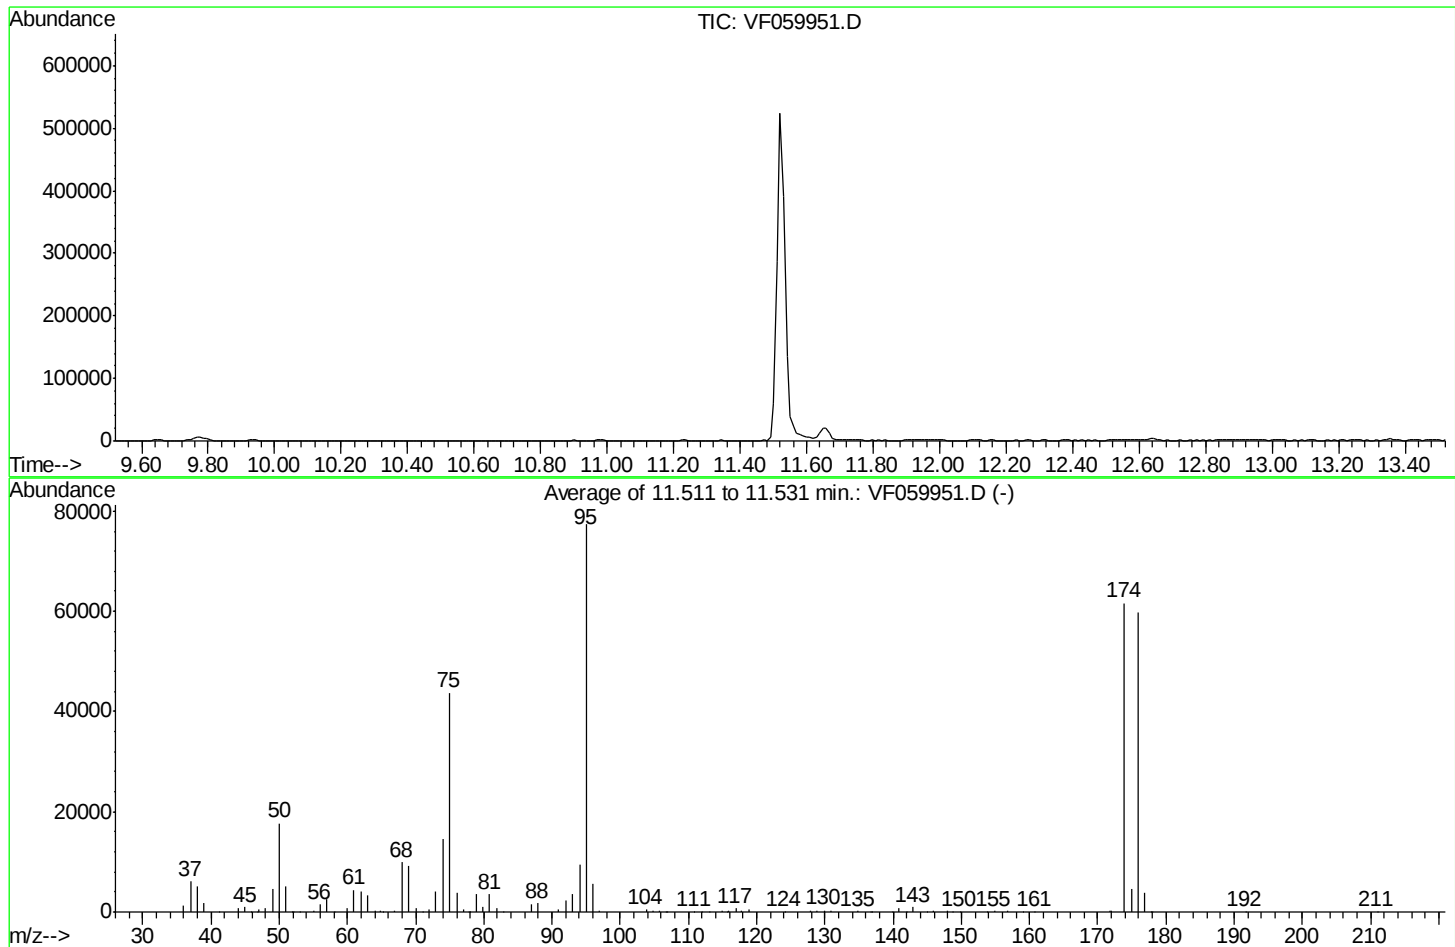

AutoFind: Scans 1114, 1115, 1116; Background Corrected with Scan 1109

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.9      | 17709   | PASS             |
| 75          | 95           | 30           | 60           | 56.6      | 43770   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 77365   | PASS             |
| 96          | 95           | 5            | 9            | 7.3       | 5665    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 79.7      | 61682   | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 4629    | PASS             |
| 176         | 174          | 95           | 101          | 96.8      | 59688   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 3958    | PASS             |