


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF081618\
Data File : VF059967.D
Acq On : 16 Aug 2018 18:18
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081618S.M
Title : SW846 8260
Last Update : Fri Aug 17 05:35:49 2018

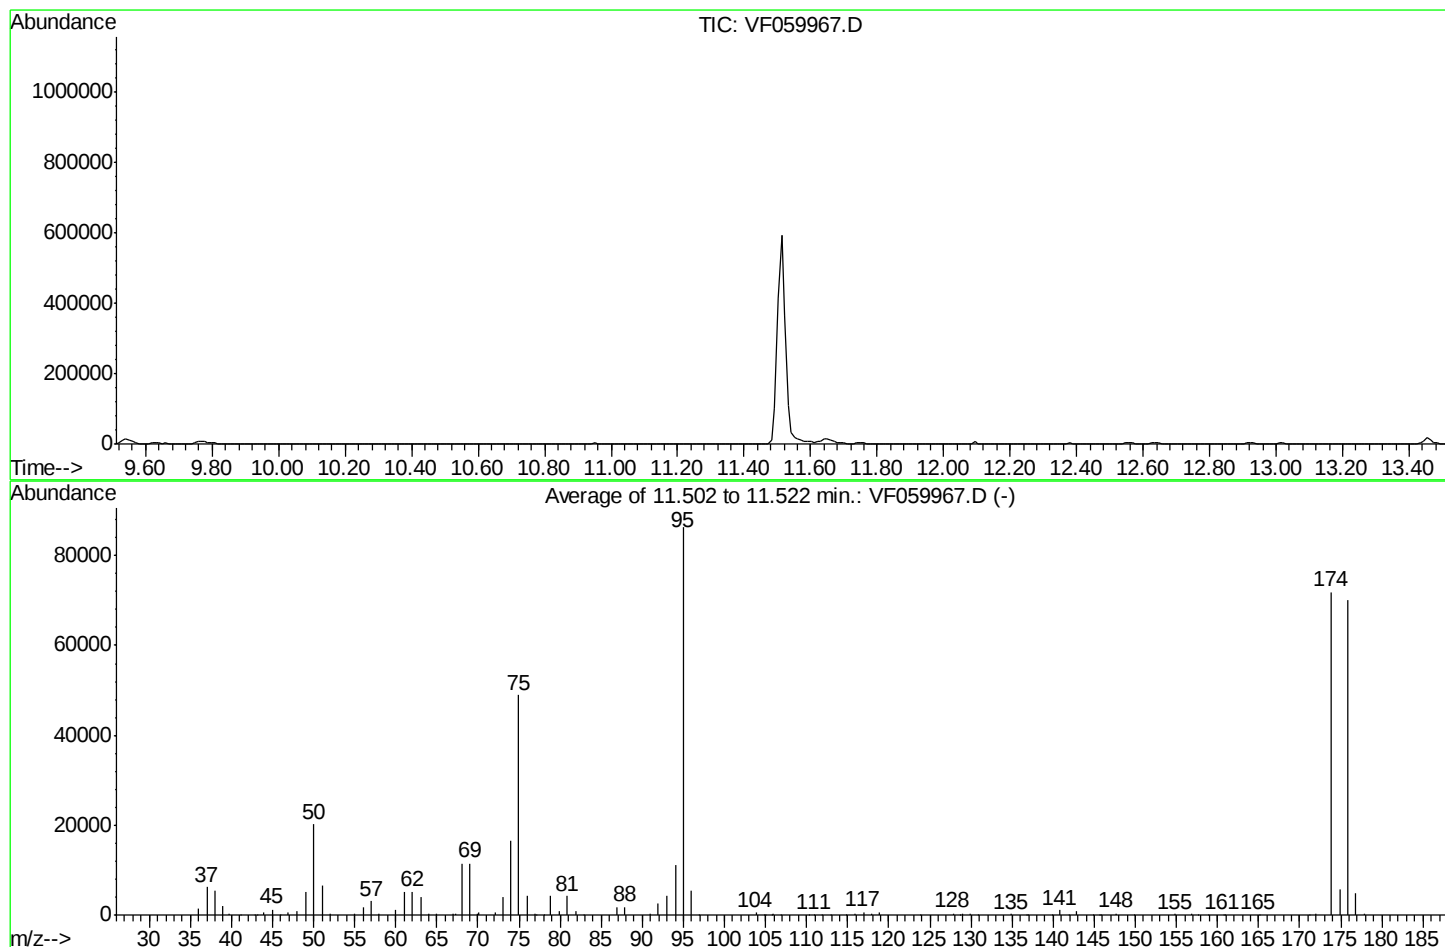

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	20211	PASS
75	95	30	60	56.8	49008	PASS
95	95	100	100	100.0	86309	PASS
96	95	5	9	6.3	5476	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.2	71850	PASS
175	174	5	9	8.0	5732	PASS
176	174	95	101	97.6	70128	PASS
177	176	5	9	6.8	4741	PASS