




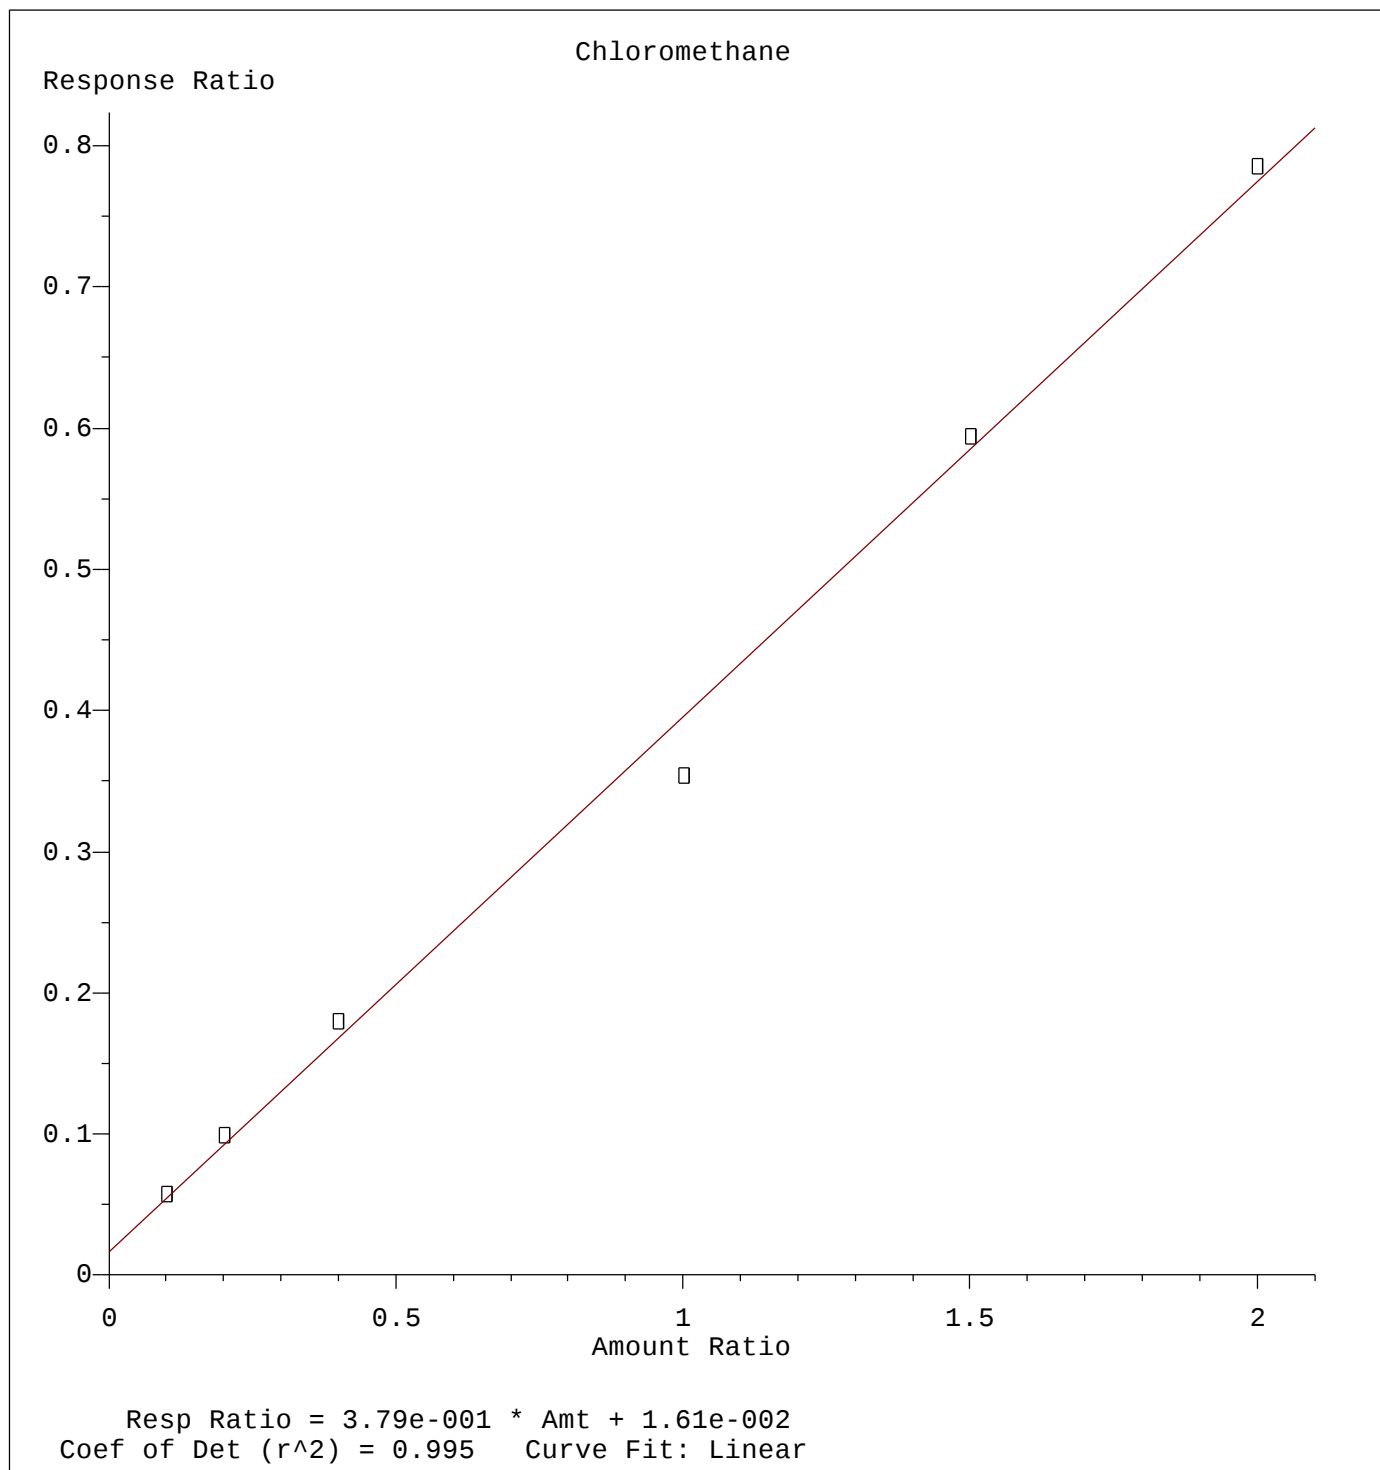

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Calibration Table Last Updated: Mon Aug 20 17:04:52 2018

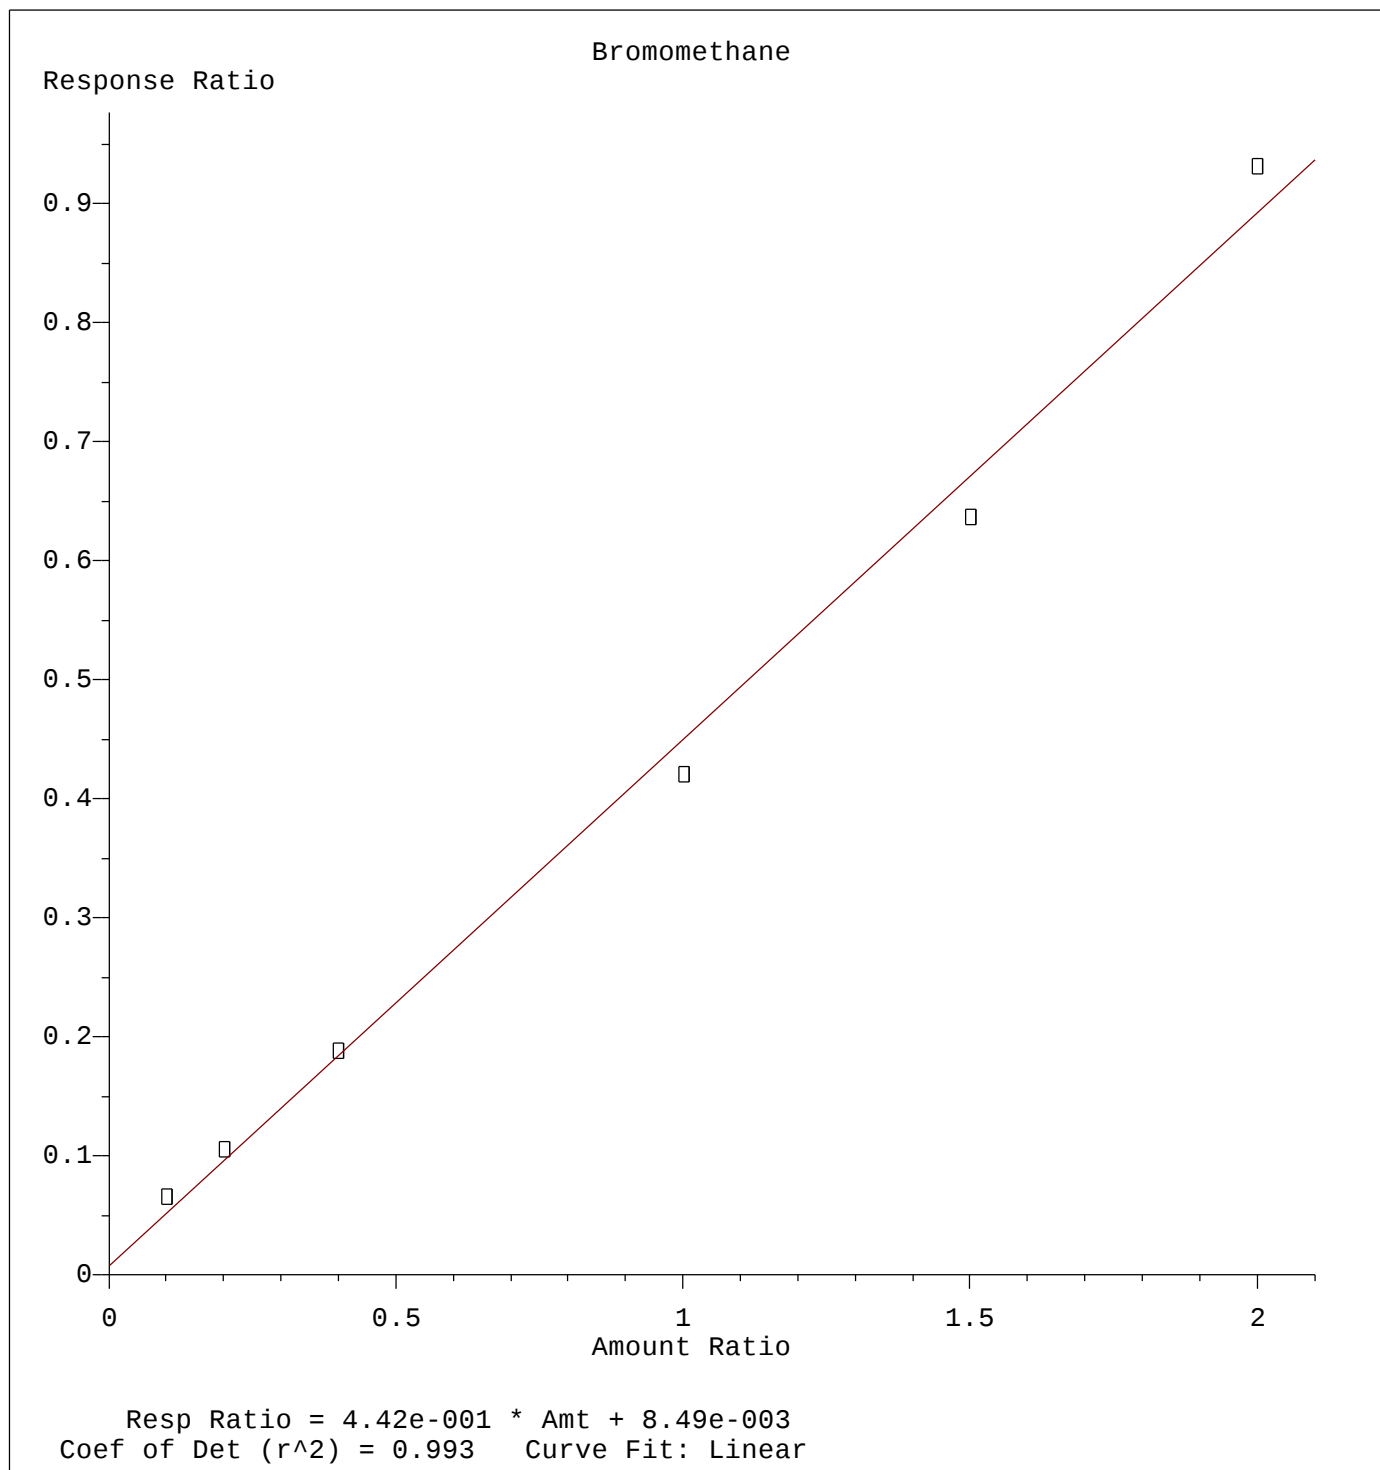


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Calibration Table Last Updated: Mon Aug 20 17:04:52 2018

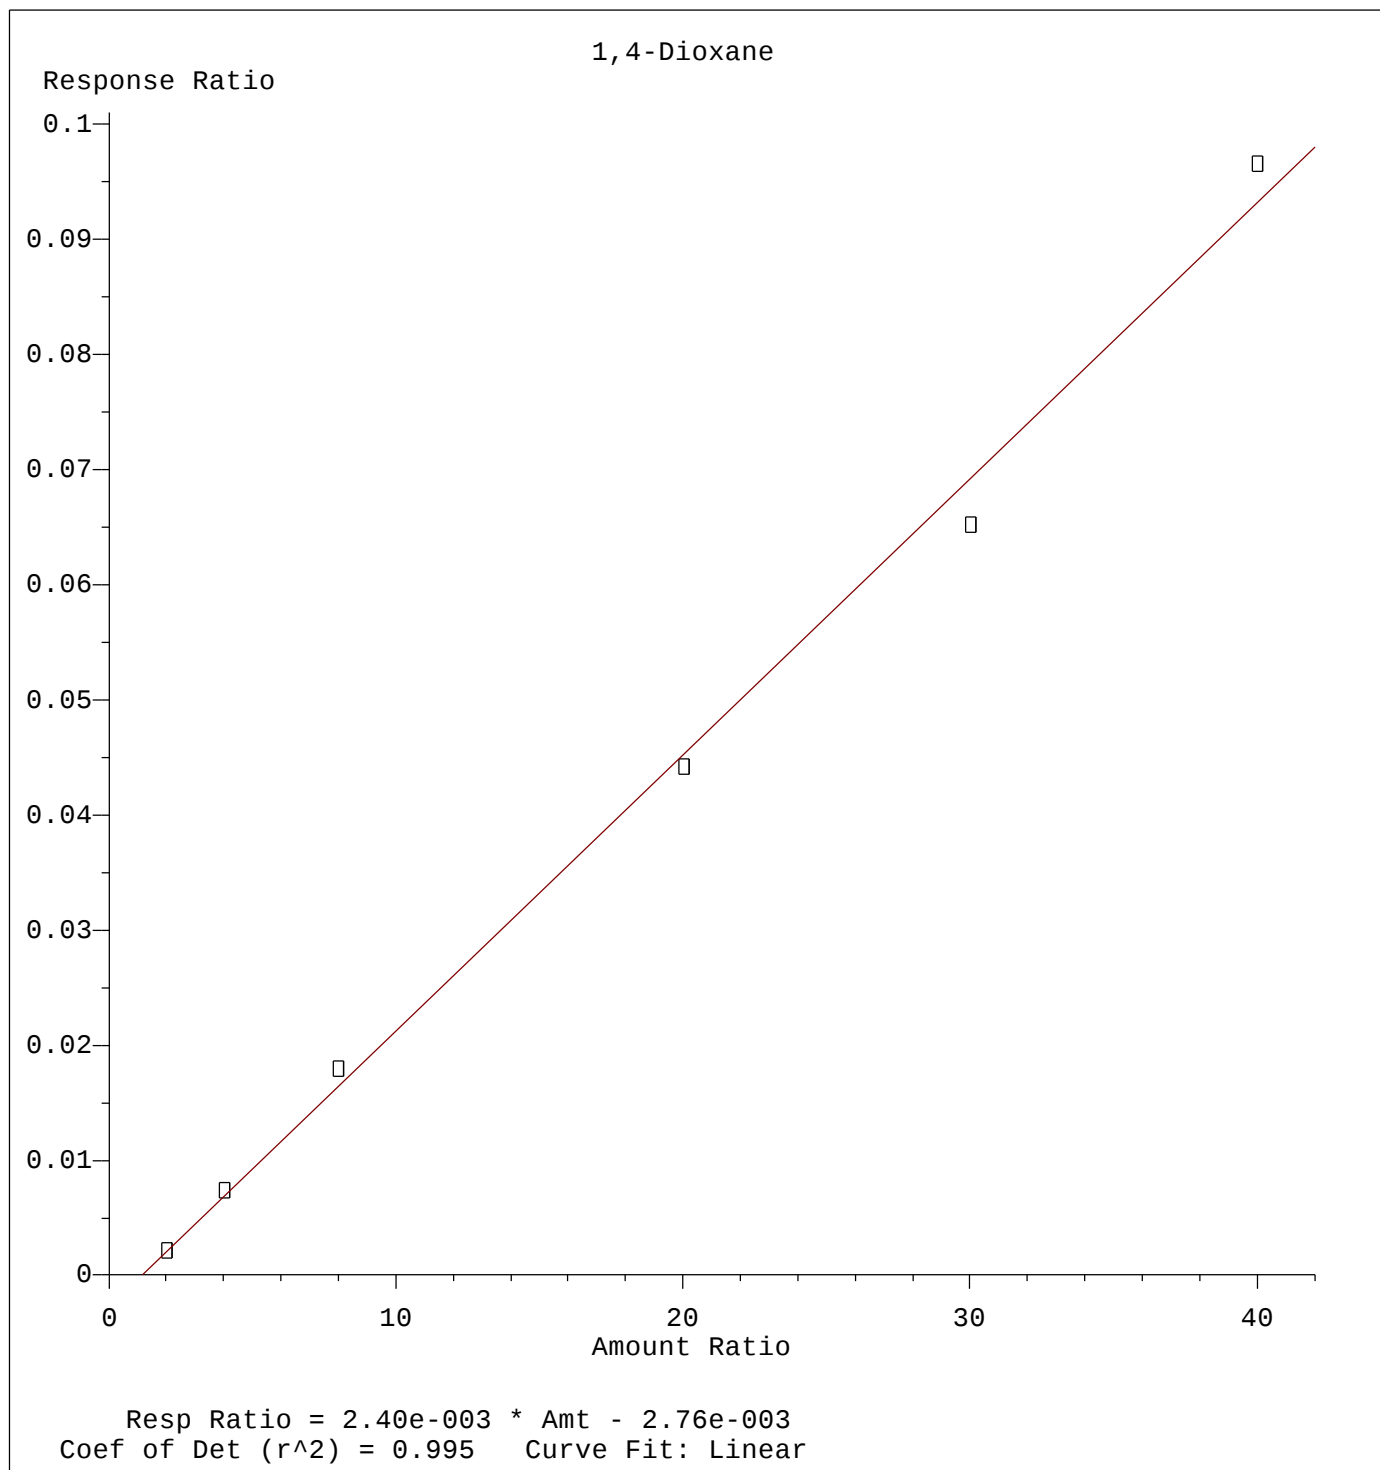

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Calibration Table Last Updated: Mon Aug 20 17:04:52 2018


Methylene Chloride

Response Ratio

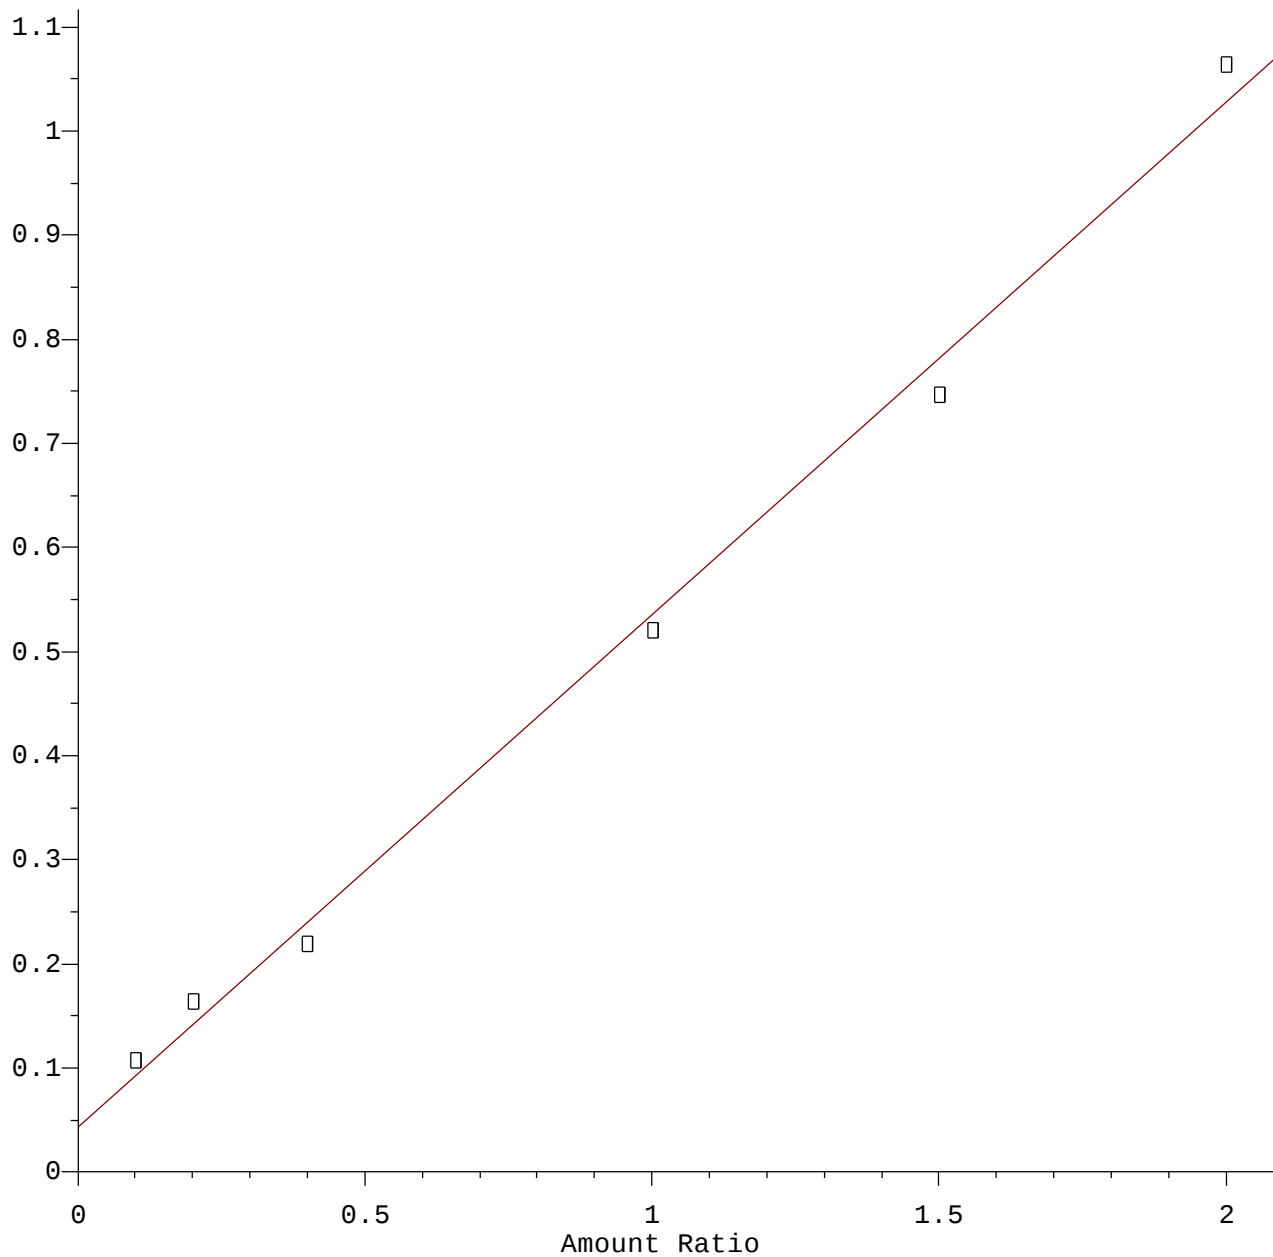


Resp Ratio = $4.92 \times 10^{-1} \times \text{Amt} + 4.35 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Calibration Table Last Updated: Mon Aug 20 17:04:52 2018

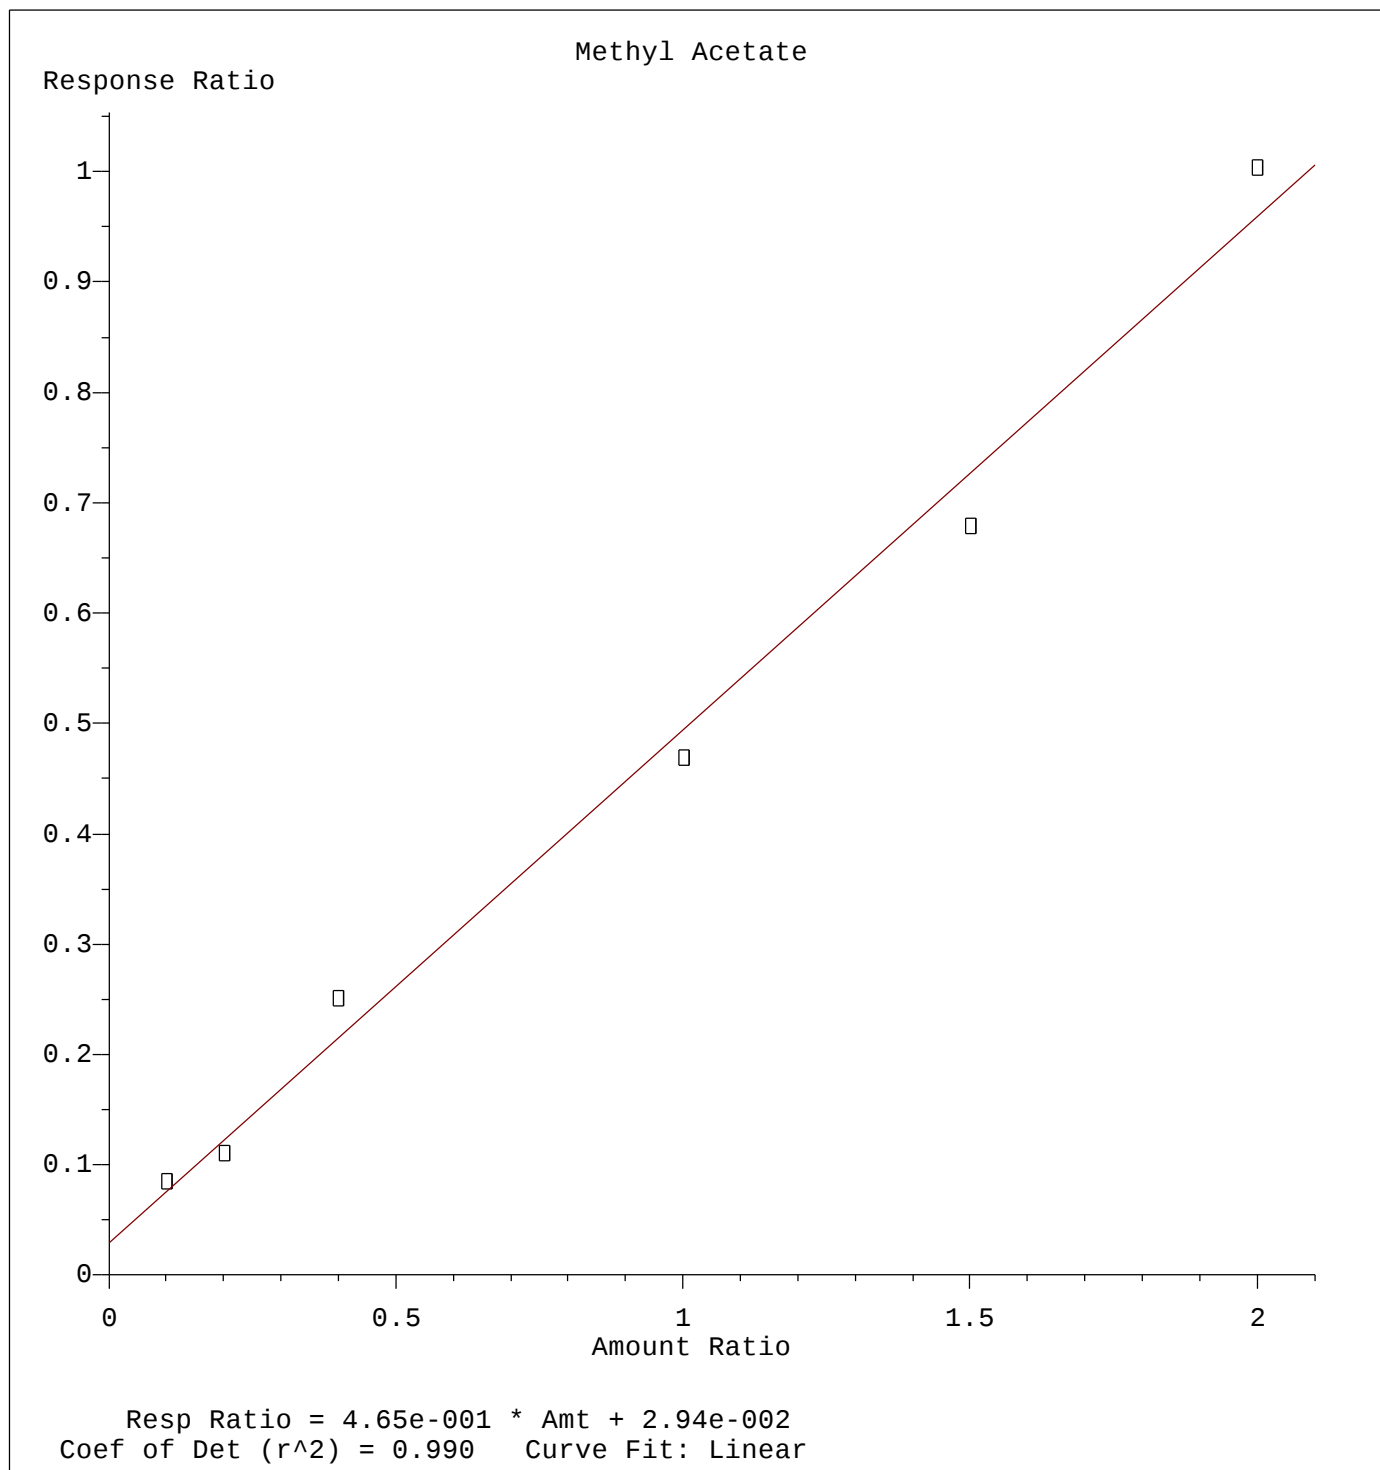

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Calibration Table Last Updated: Mon Aug 20 17:04:52 2018

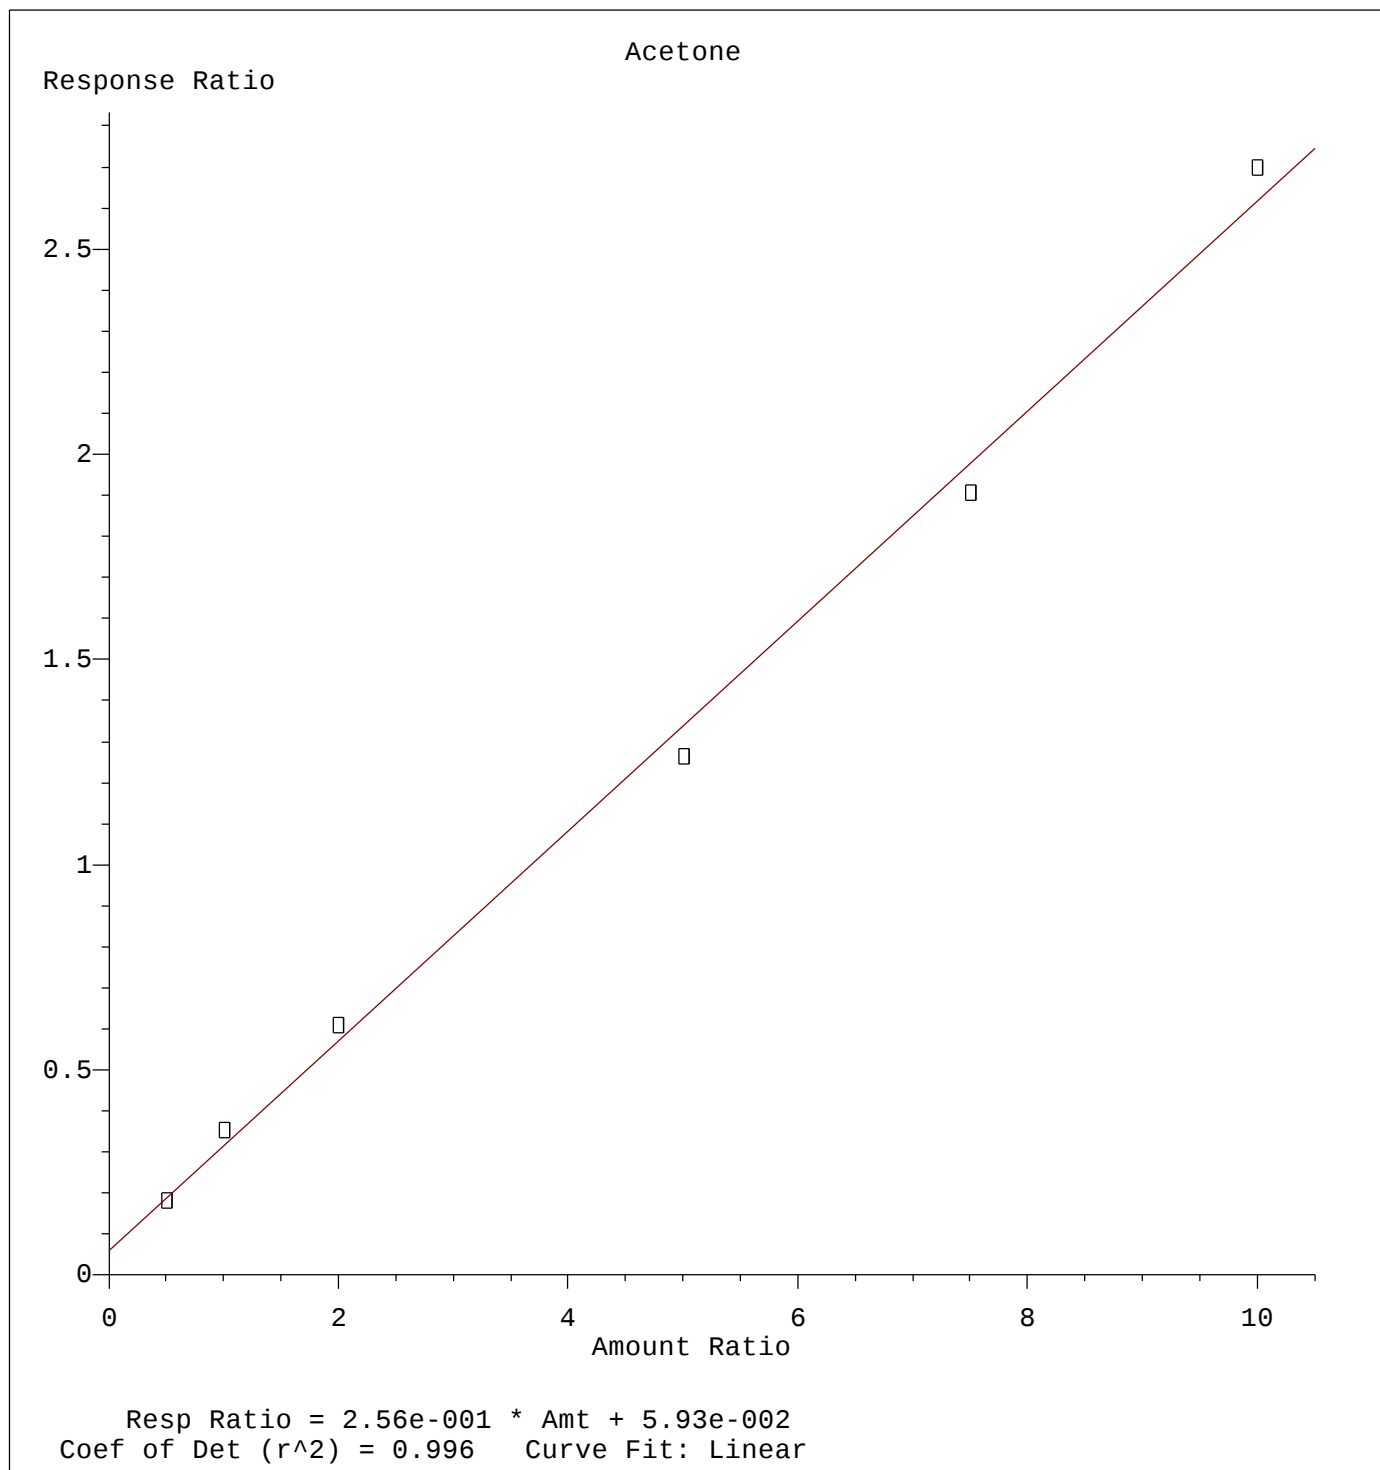

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Calibration Table Last Updated: Mon Aug 20 17:04:52 2018

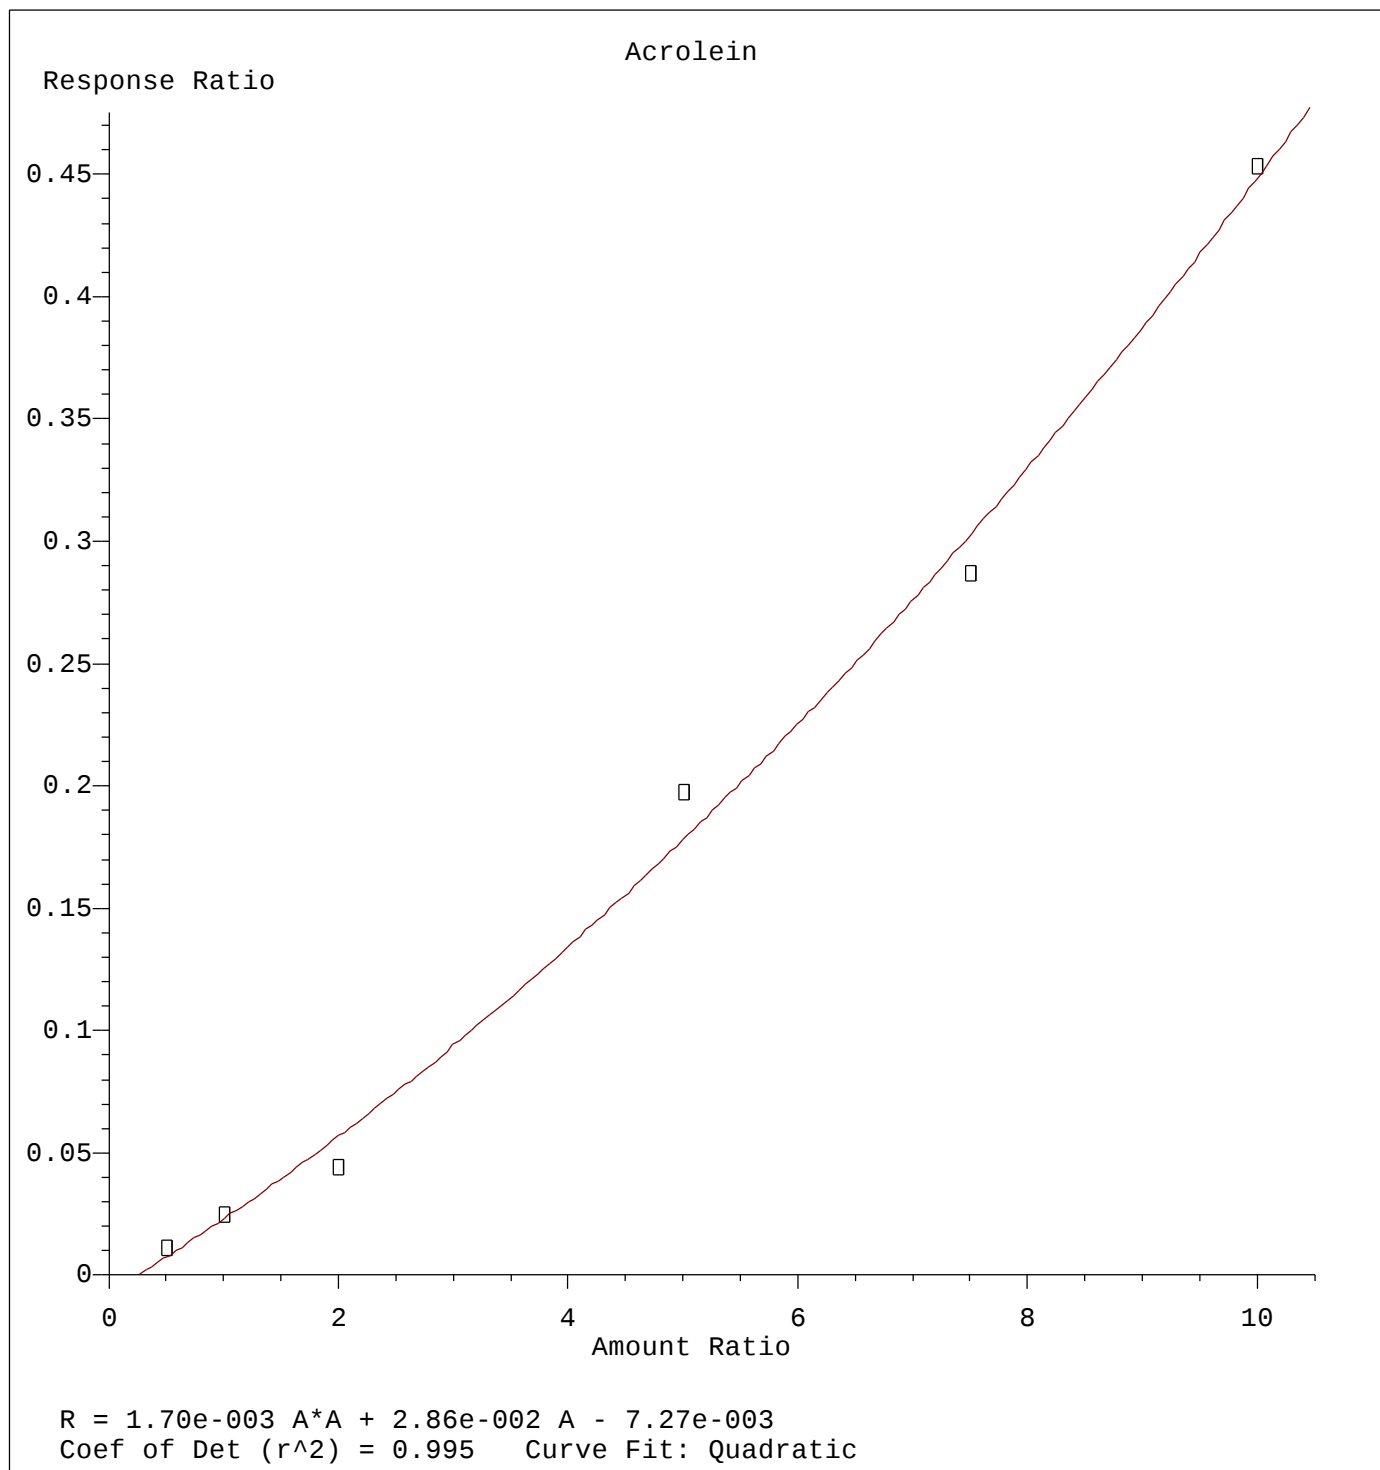

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Calibration Table Last Updated: Mon Aug 20 17:04:52 2018