


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF081718\
Data File : VF059976.D
Acq On : 17 Aug 2018 15:51
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Title : SW846 8260
Last Update : Sat Aug 18 01:11:02 2018

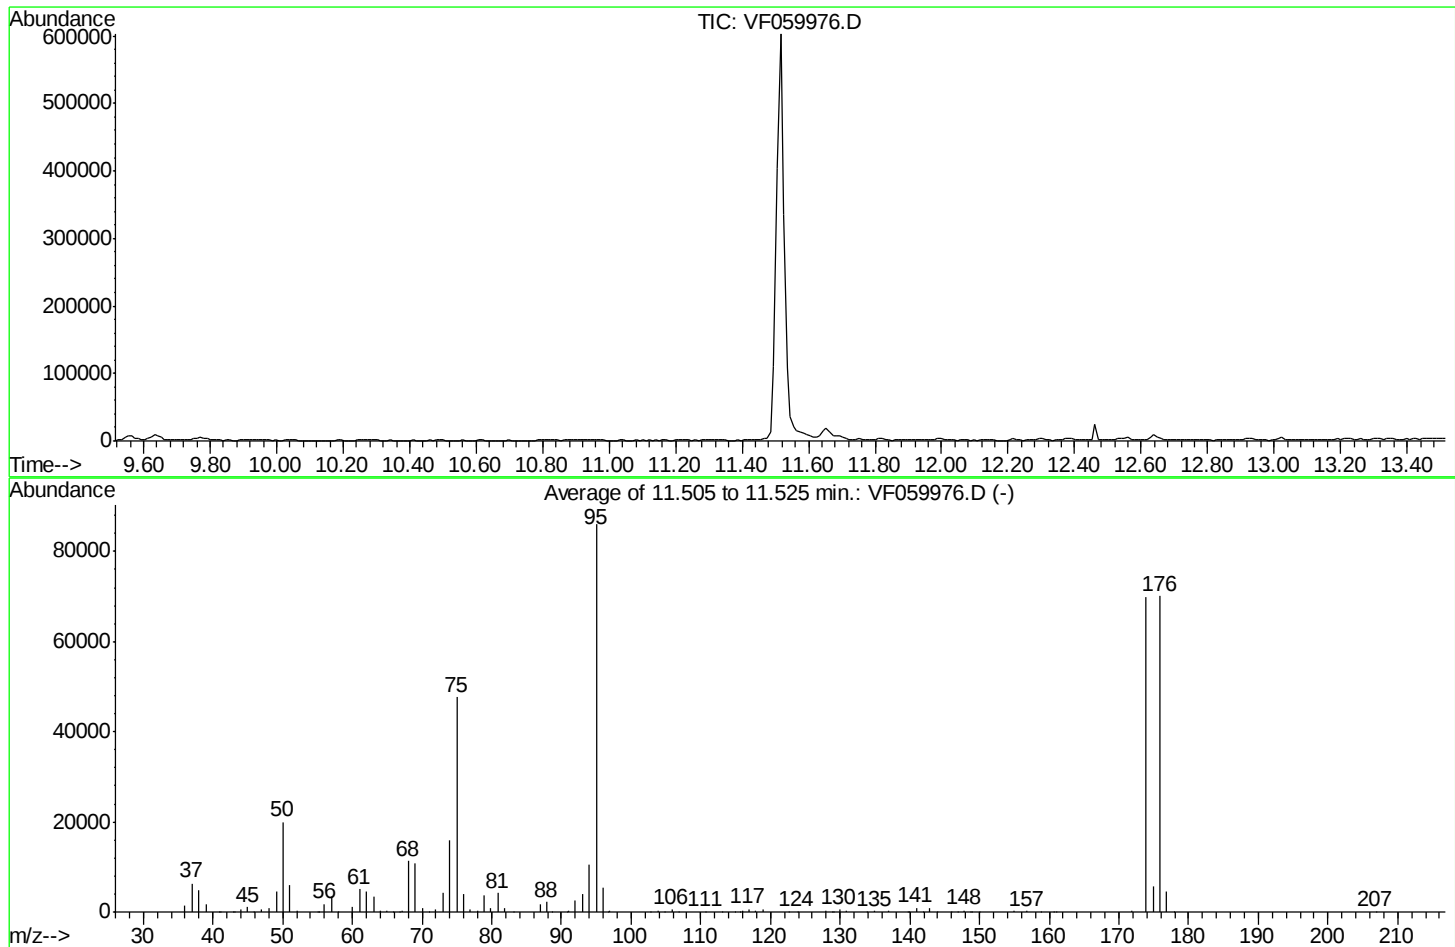

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	19958	PASS
75	95	30	60	55.3	47602	PASS
95	95	100	100	100.0	86021	PASS
96	95	5	9	6.1	5280	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.3	69968	PASS
175	174	5	9	8.1	5675	PASS
176	174	95	101	100.2	70128	PASS
177	176	5	9	6.4	4466	PASS