


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF082018\
Data File : VF059999.D
Acq On : 20 Aug 2018 12:43
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F081718S.M
Title : SW846 8260
Last Update : Sat Aug 18 01:11:02 2018

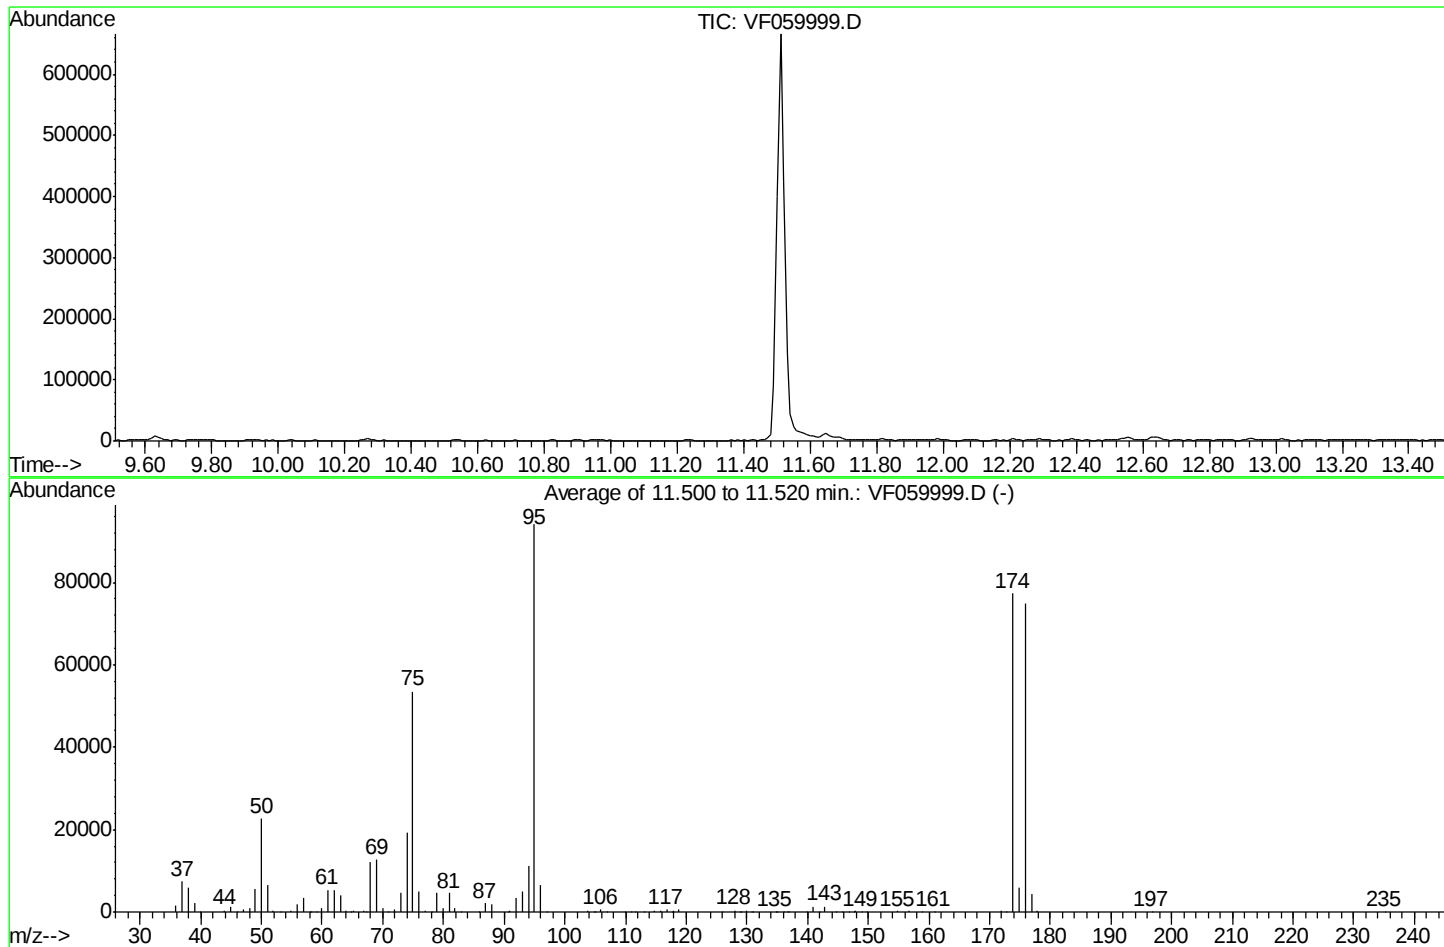

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1108

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	22642	PASS
75	95	30	60	56.8	53448	PASS
95	95	100	100	100.0	94088	PASS
96	95	5	9	6.8	6421	PASS
173	174	0.00	2	0.2	117	PASS
174	95	50	100	82.2	77304	PASS
175	174	5	9	7.7	5956	PASS
176	174	95	101	96.9	74920	PASS
177	176	5	9	5.9	4428	PASS