


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF082718\
Data File : VF060119.D
Acq On : 27 Aug 2018 9:54
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F082118S.M
Title : SW846 8260
Last Update : Wed Aug 22 04:43:43 2018

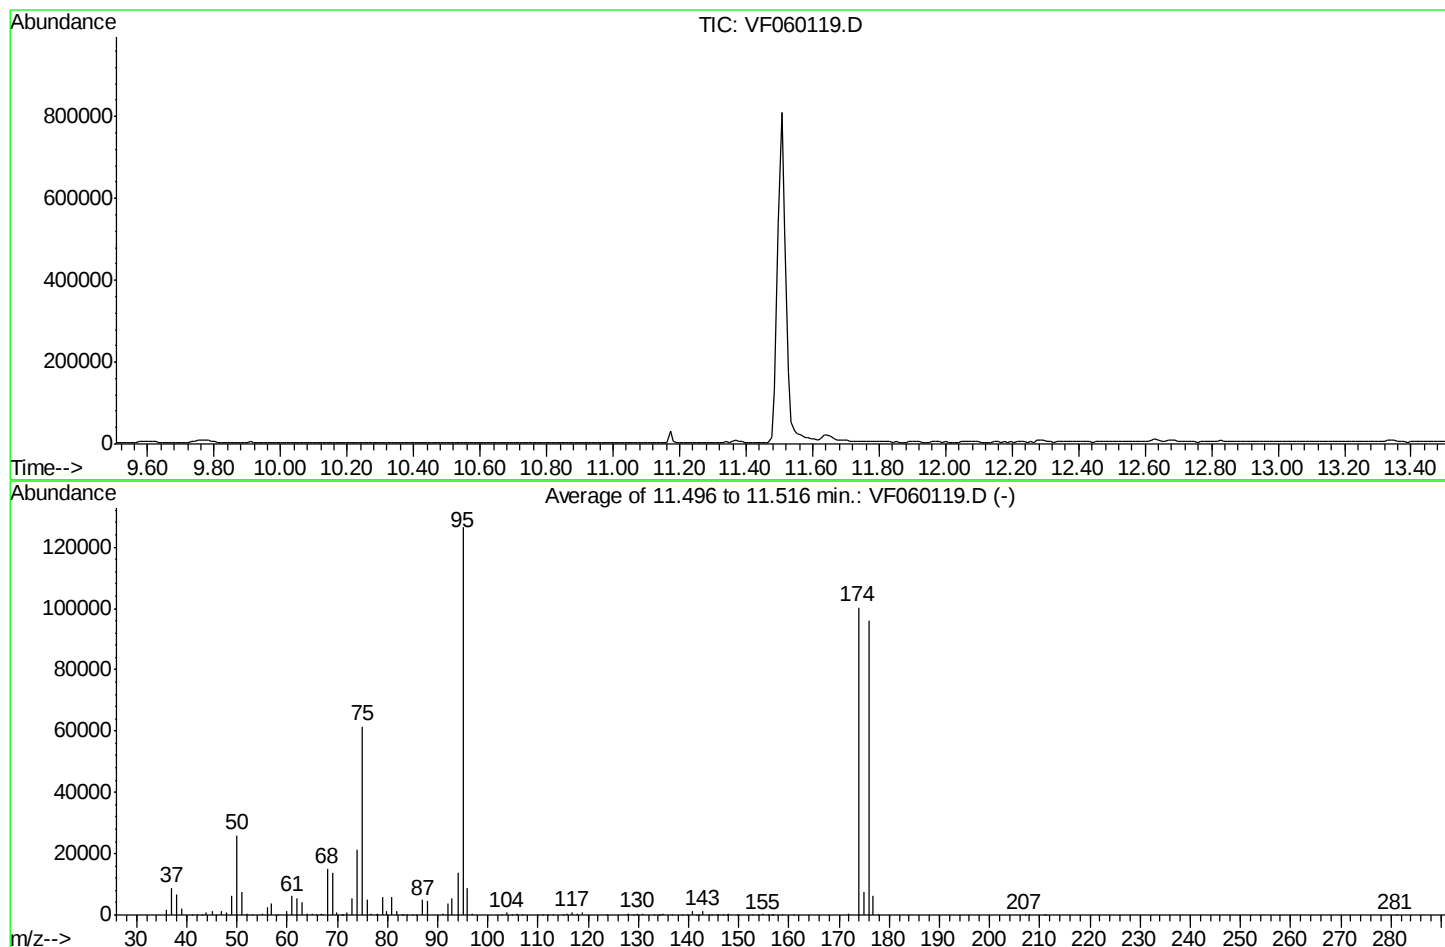

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1106

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	25898	PASS
75	95	30	60	48.6	61490	PASS
95	95	100	100	100.0	126464	PASS
96	95	5	9	6.9	8729	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.3	100312	PASS
175	174	5	9	7.4	7373	PASS
176	174	95	101	95.8	96064	PASS
177	176	5	9	6.7	6390	PASS