



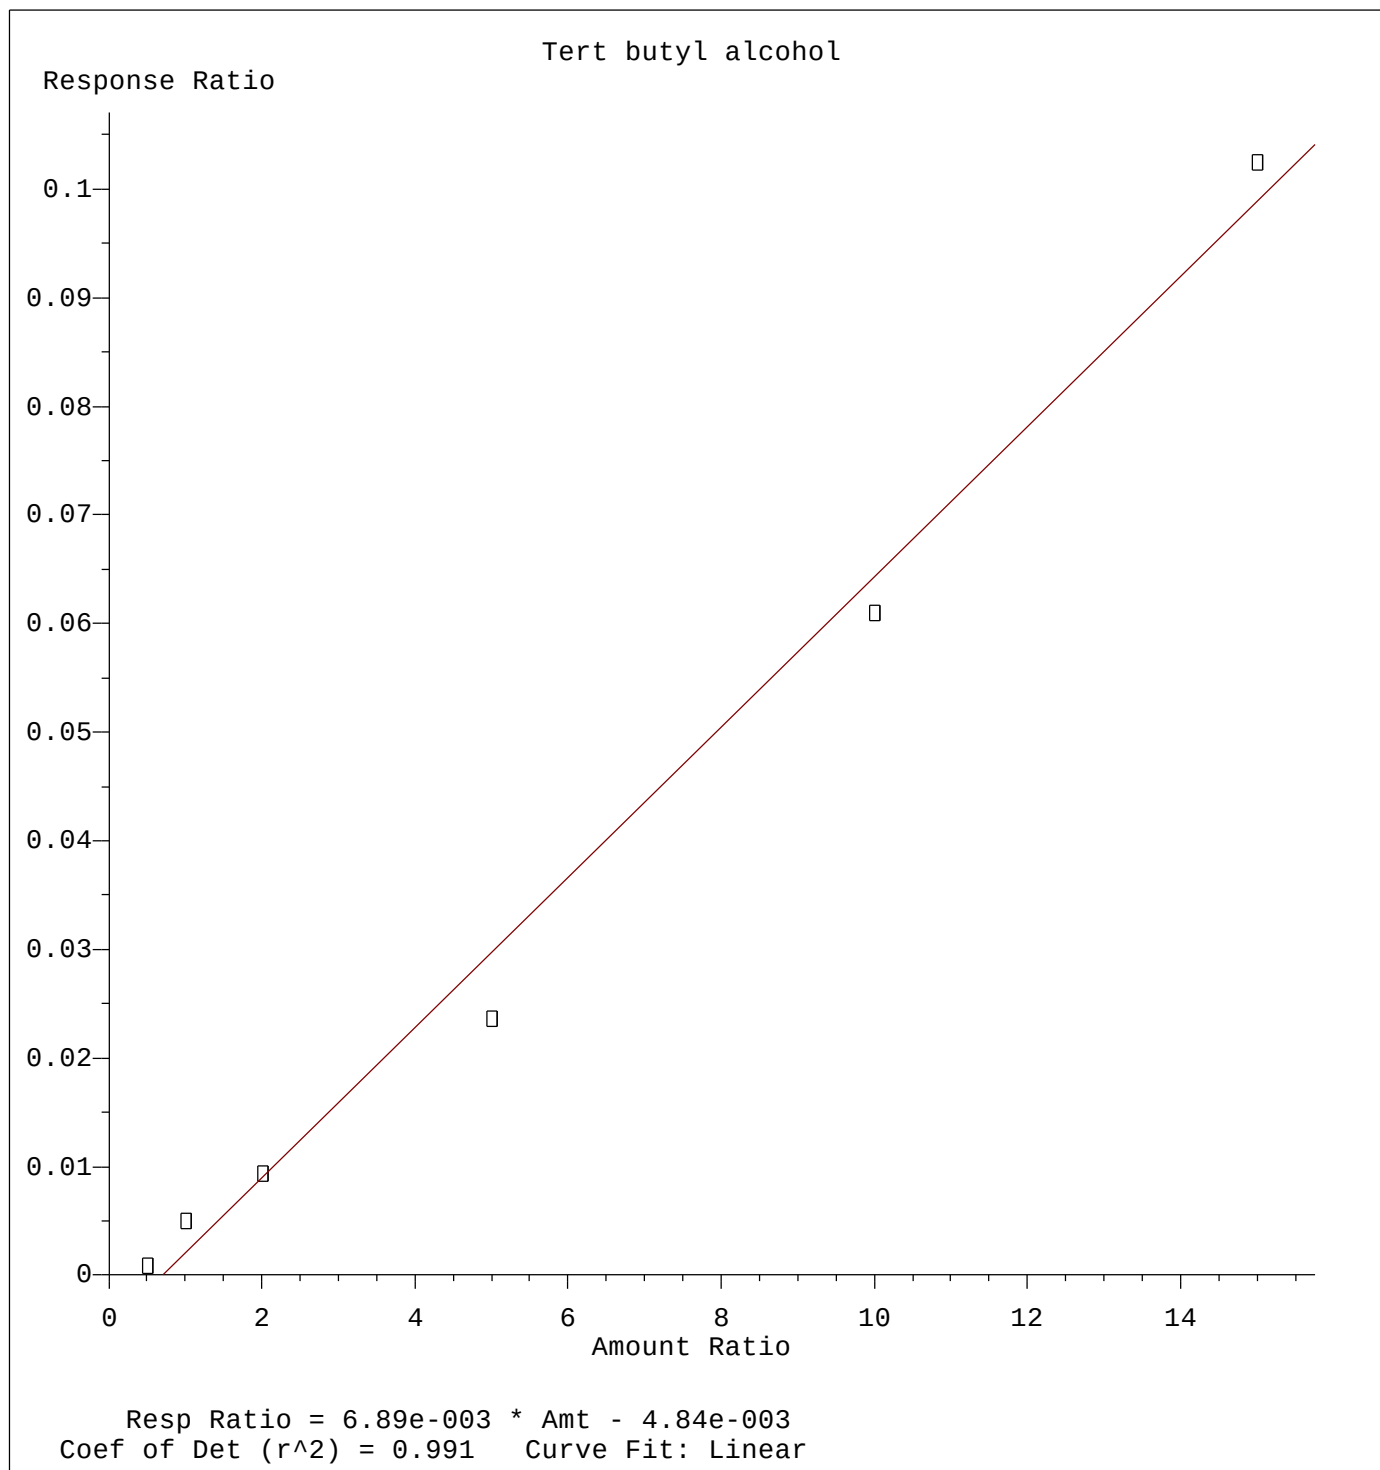

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018


# 1,2,3-Trichlorobenzene

Response Ratio

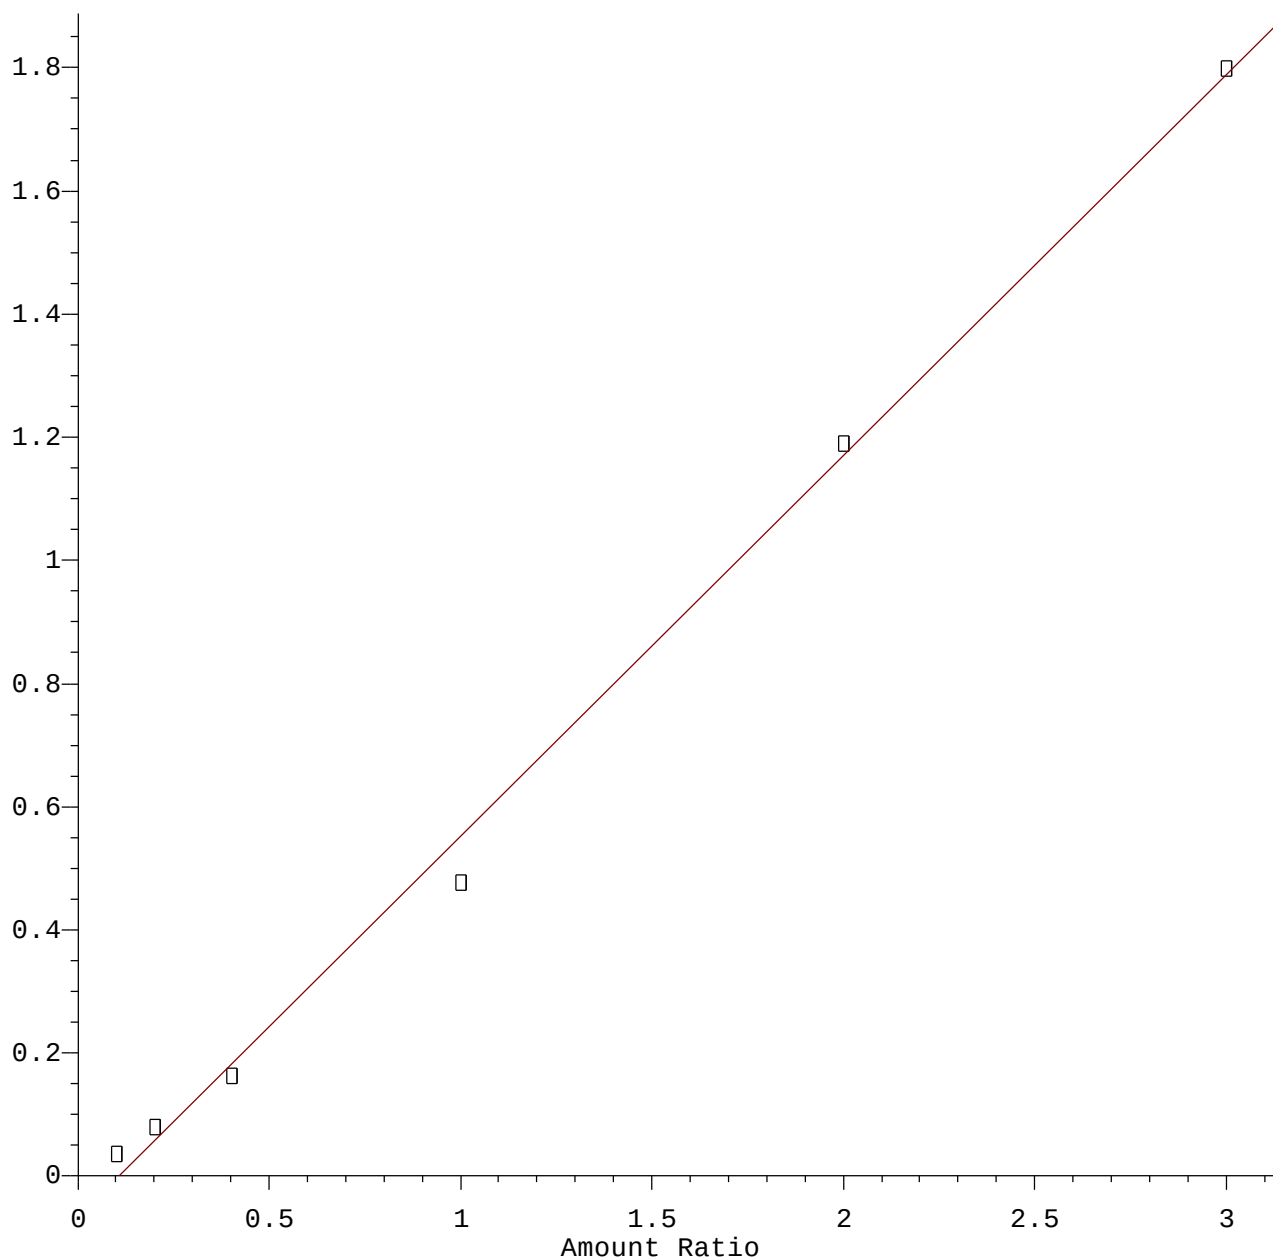

Resp Ratio =  $6.18 \times 10^{-1} \times \text{Amt} - 6.64 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.997    Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

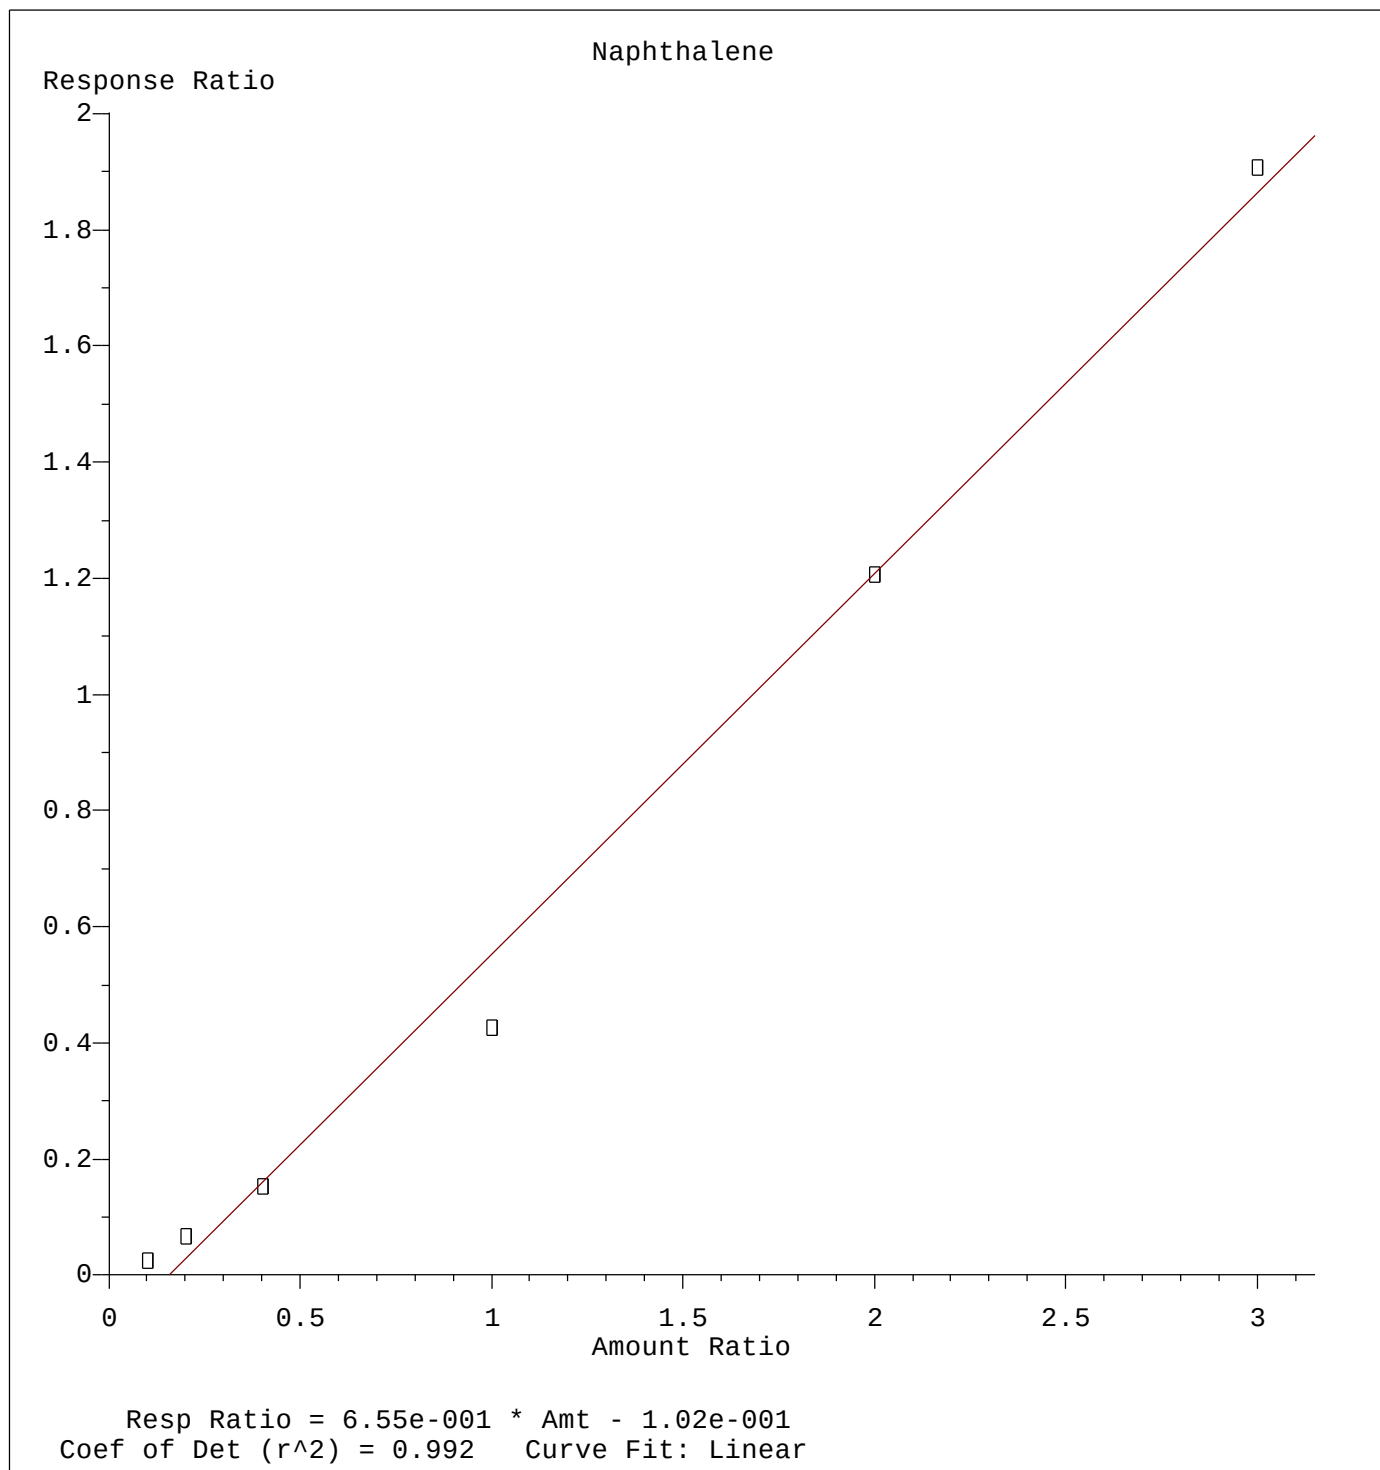

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018


# 1,2,4-Trichlorobenzene

Response Ratio

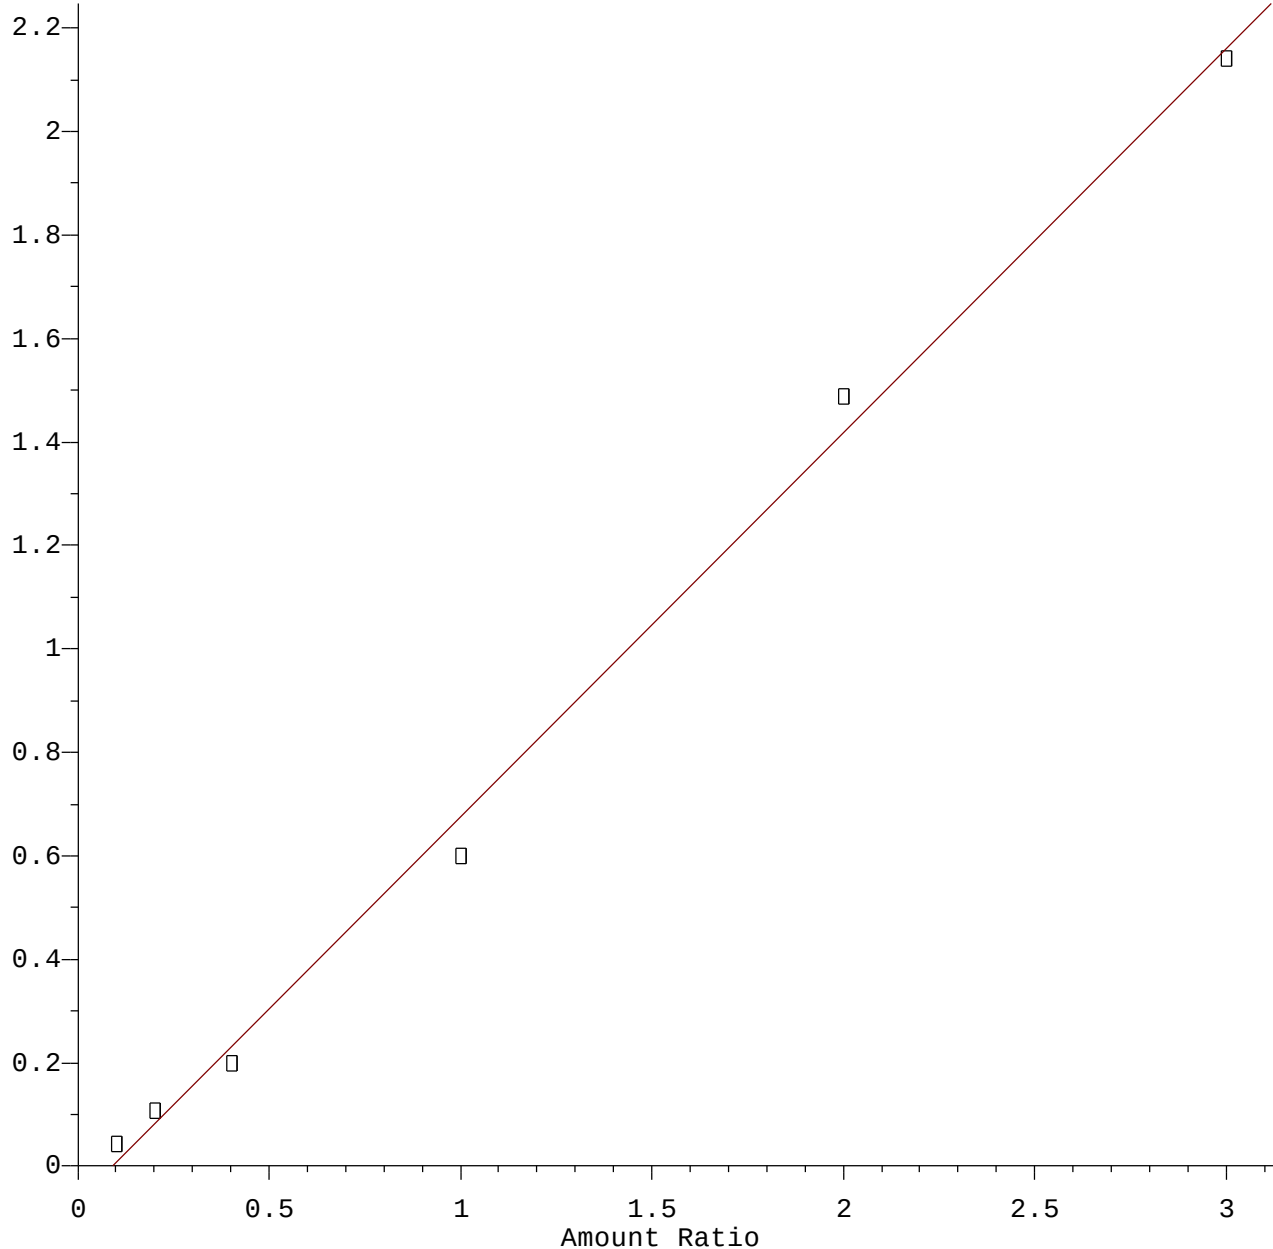


Resp Ratio =  $7.42 \times 10^{-1} \times \text{Amt} - 6.73 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.996    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

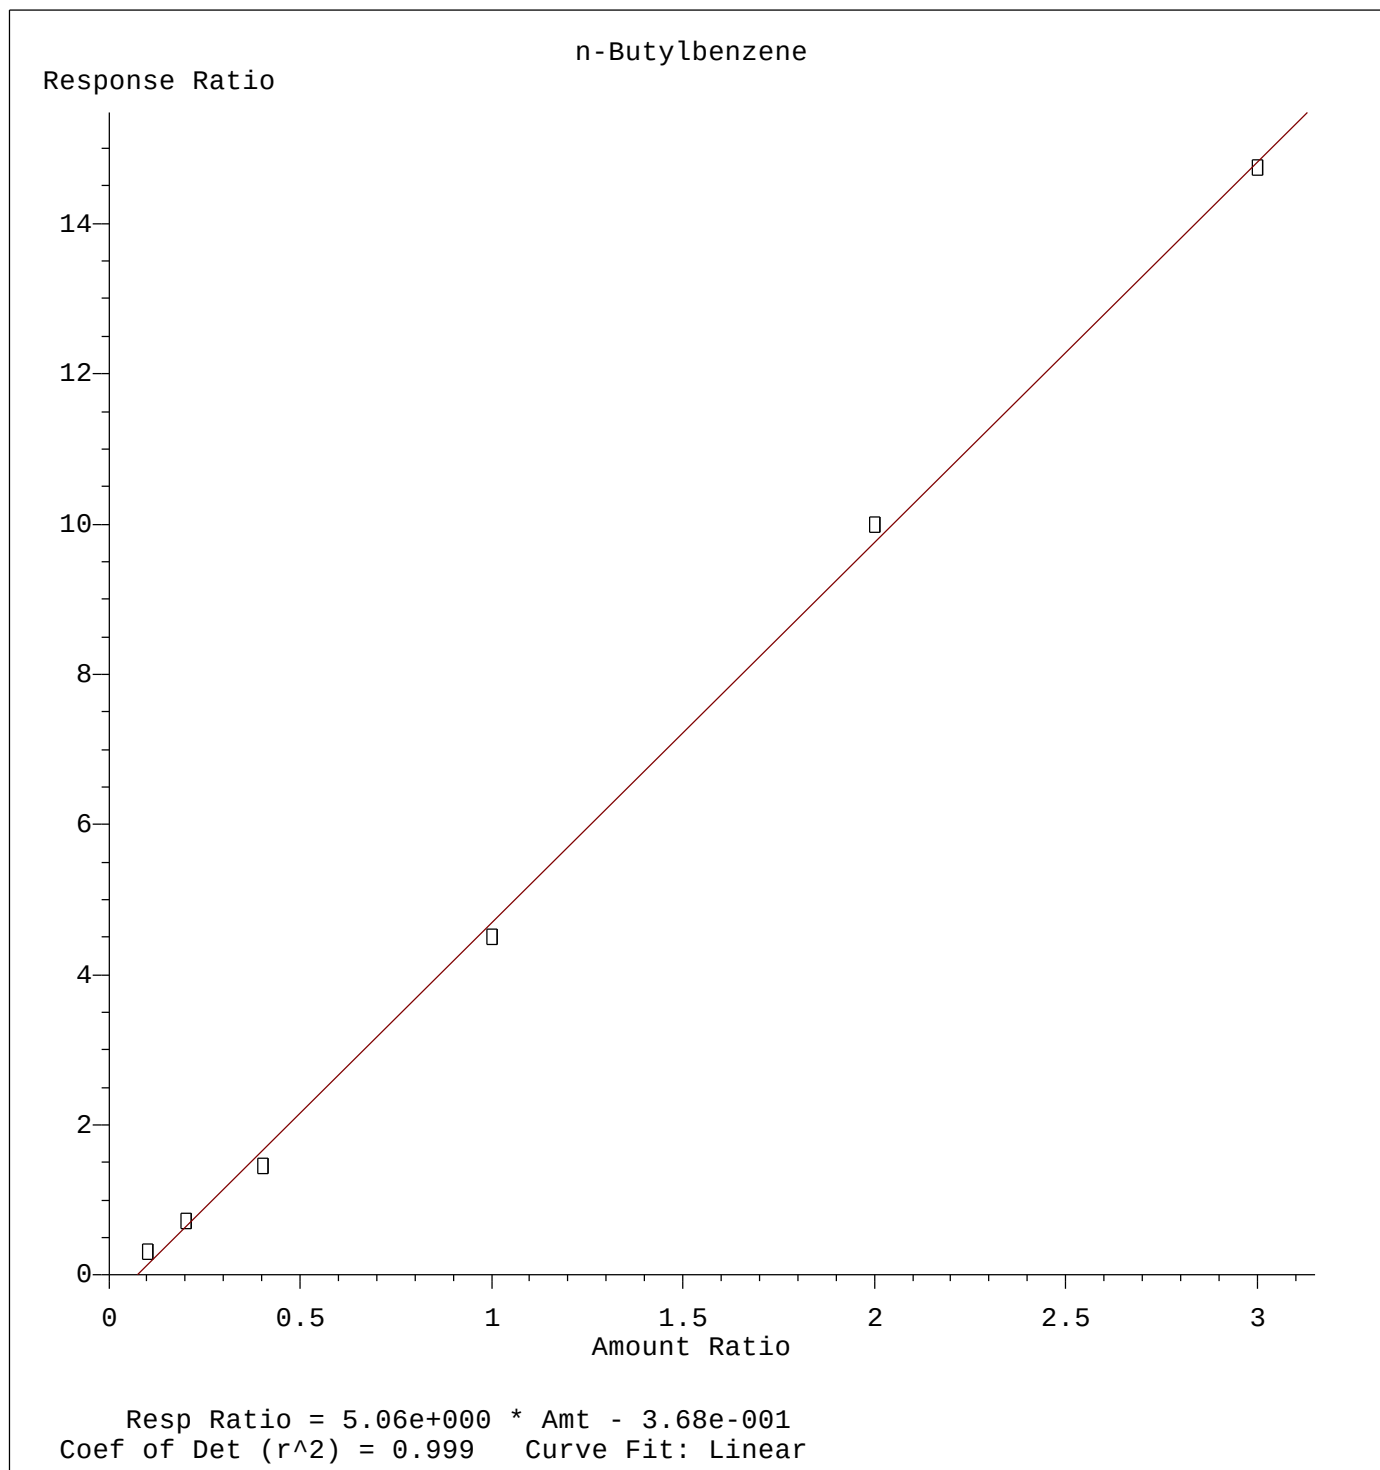


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

trans-1,4-Dichloro-2-butene

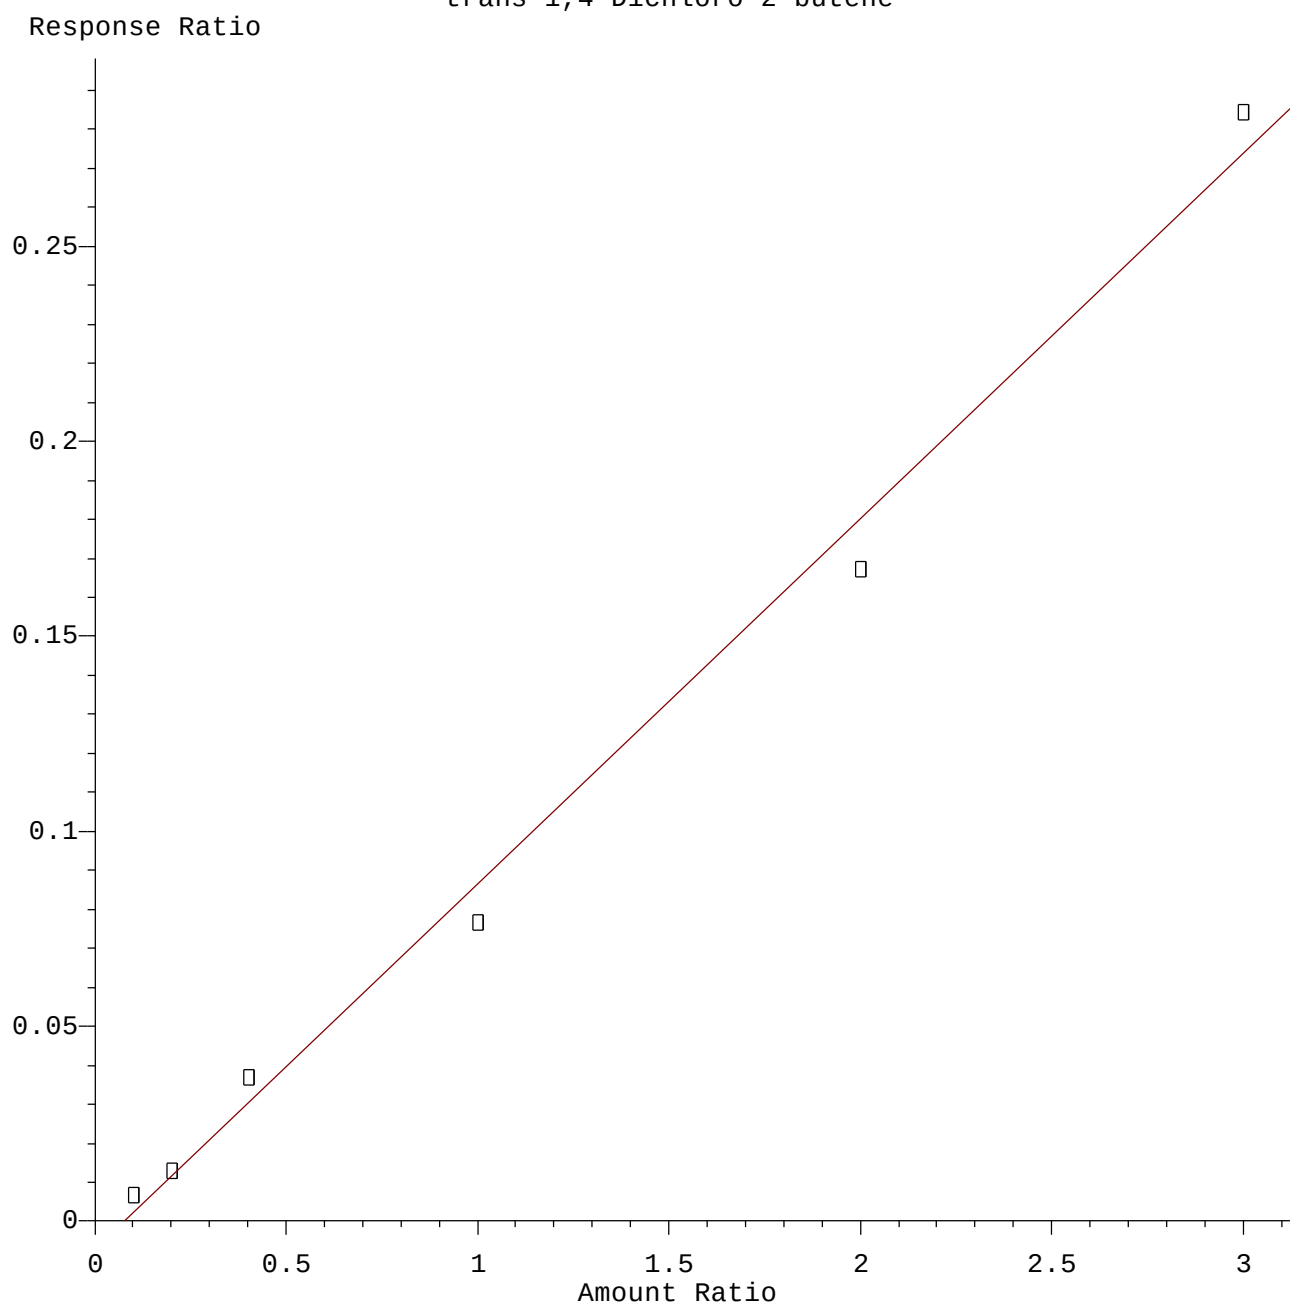


Resp Ratio =  $9.36 \times 10^{-2} \times \text{Amt} - 7.19 \times 10^{-3}$   
Coef of Det ( $r^2$ ) = 0.993    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

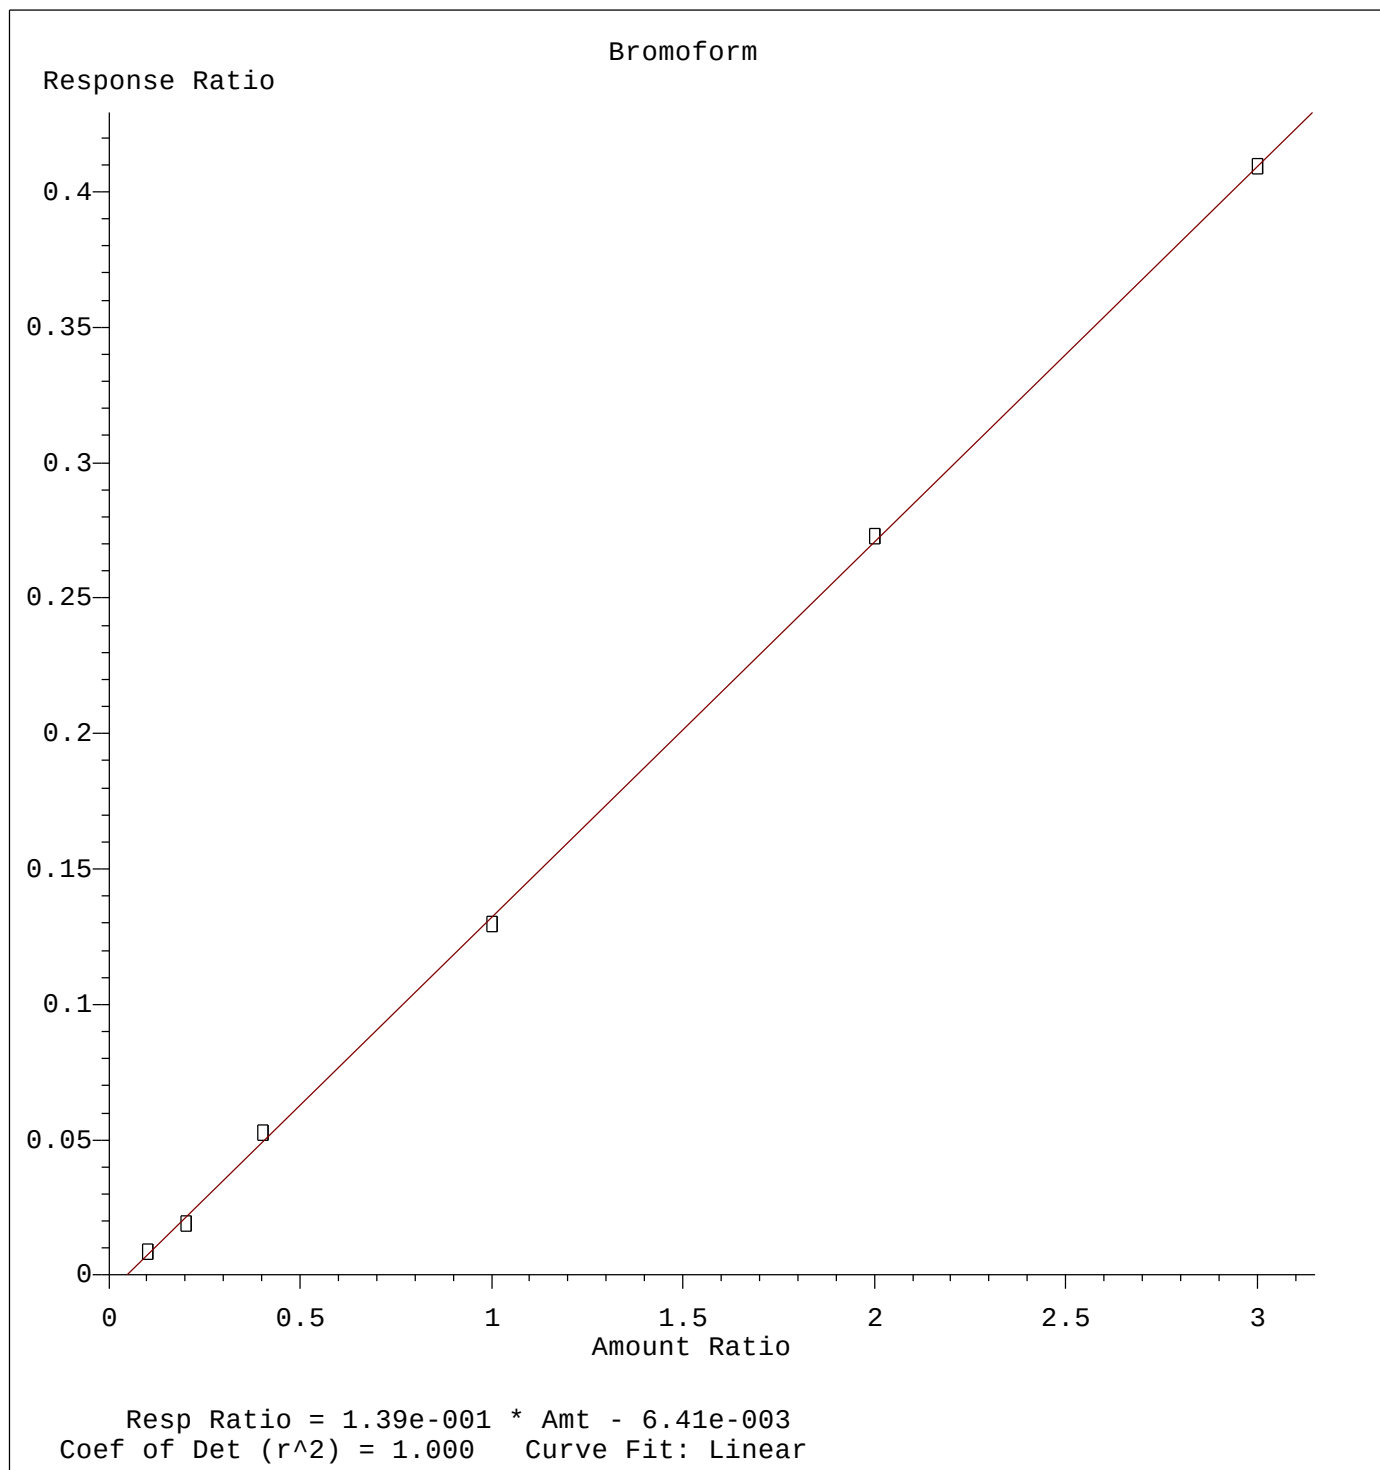

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

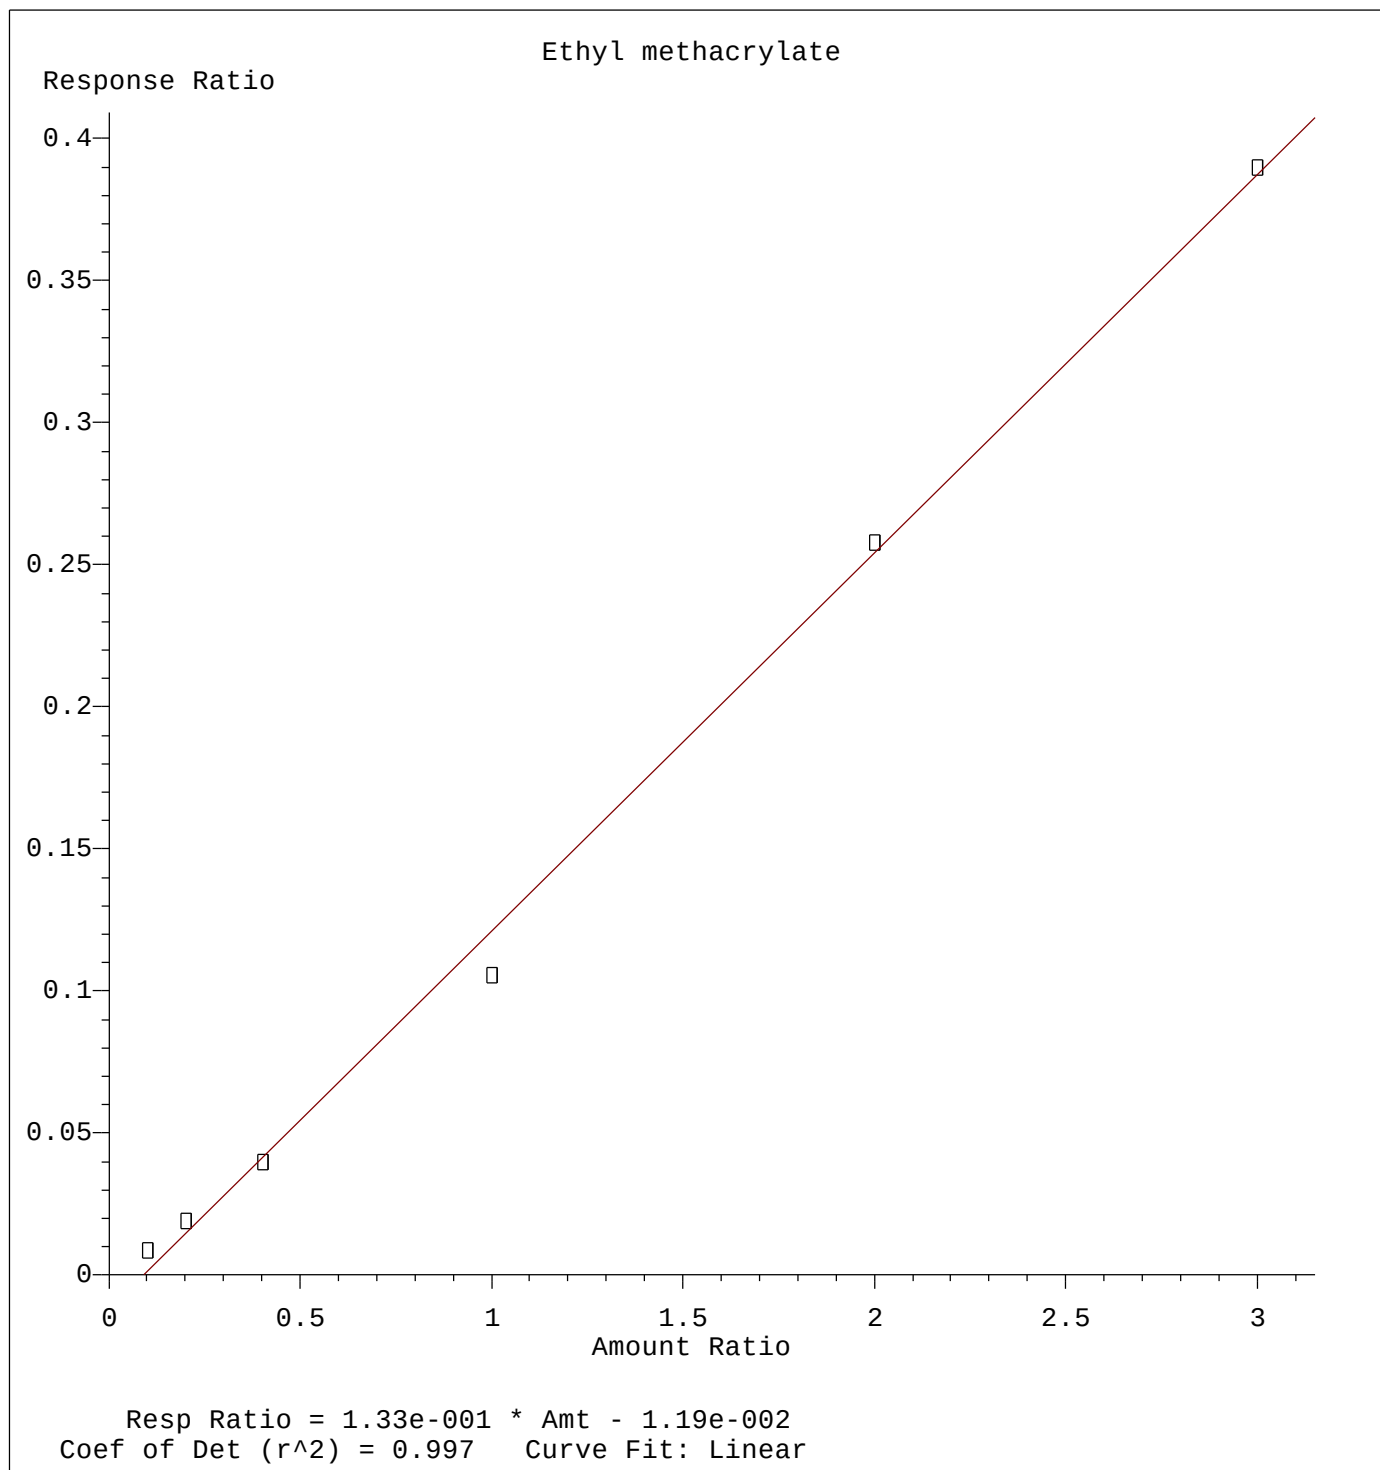


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018



cis-1,3-Dichloropropene

Response Ratio

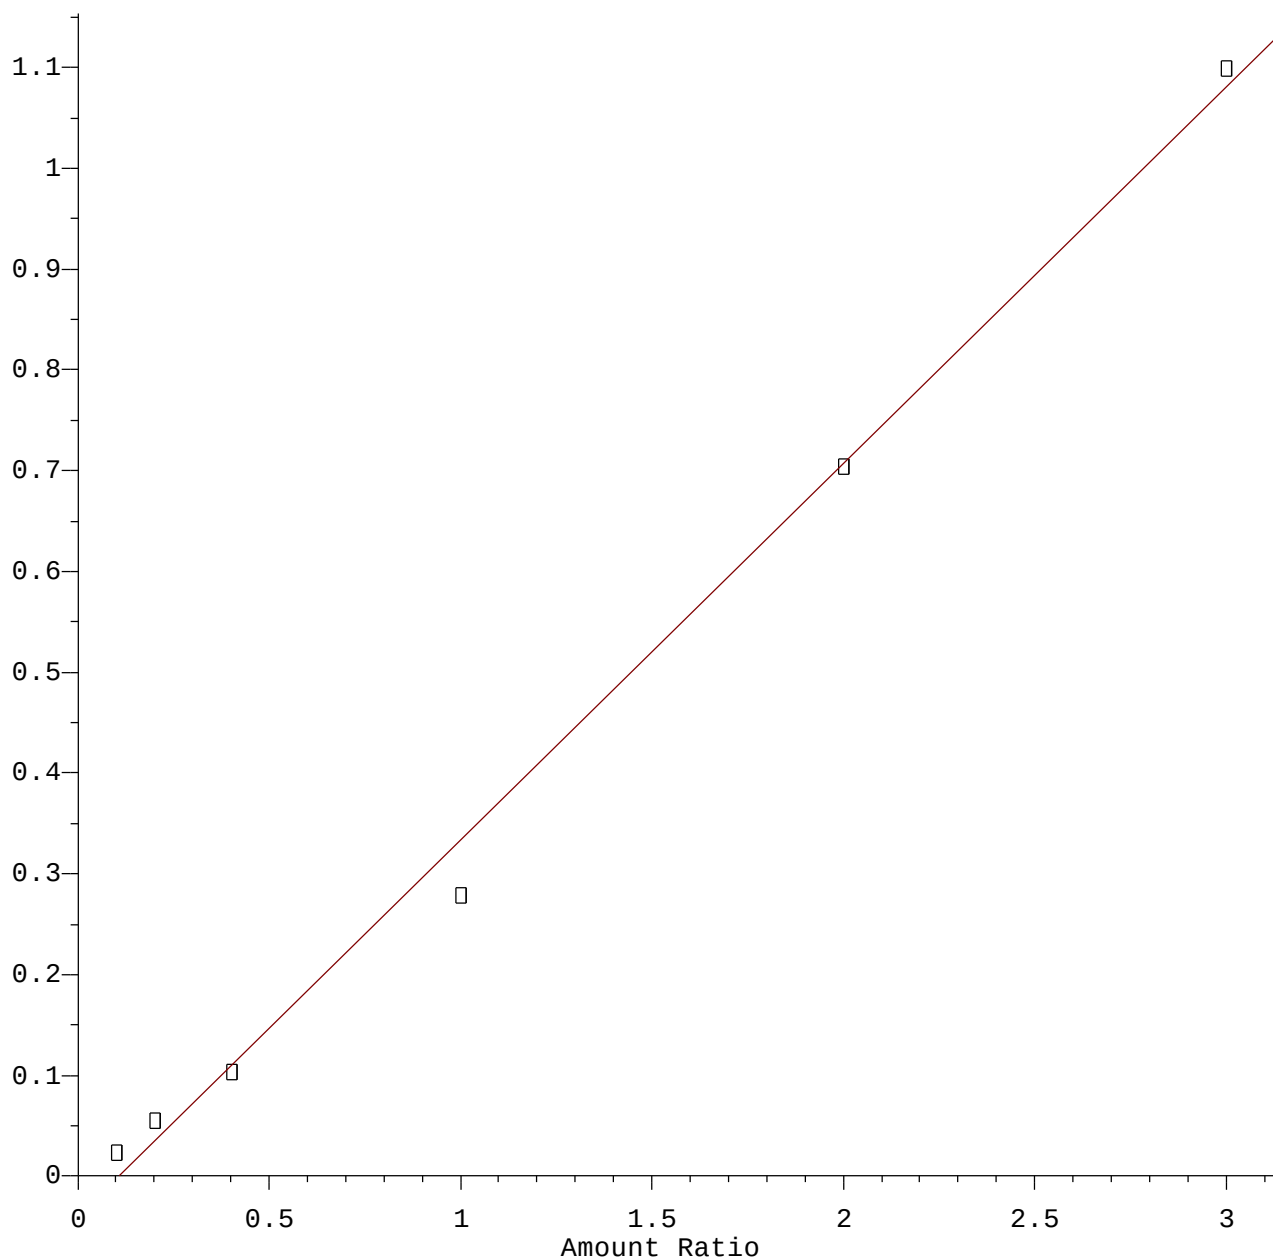


Resp Ratio =  $3.73 \times 10^{-1} \times \text{Amt} - 3.99 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.995    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018


t-1,3-Dichloropropene

Response Ratio

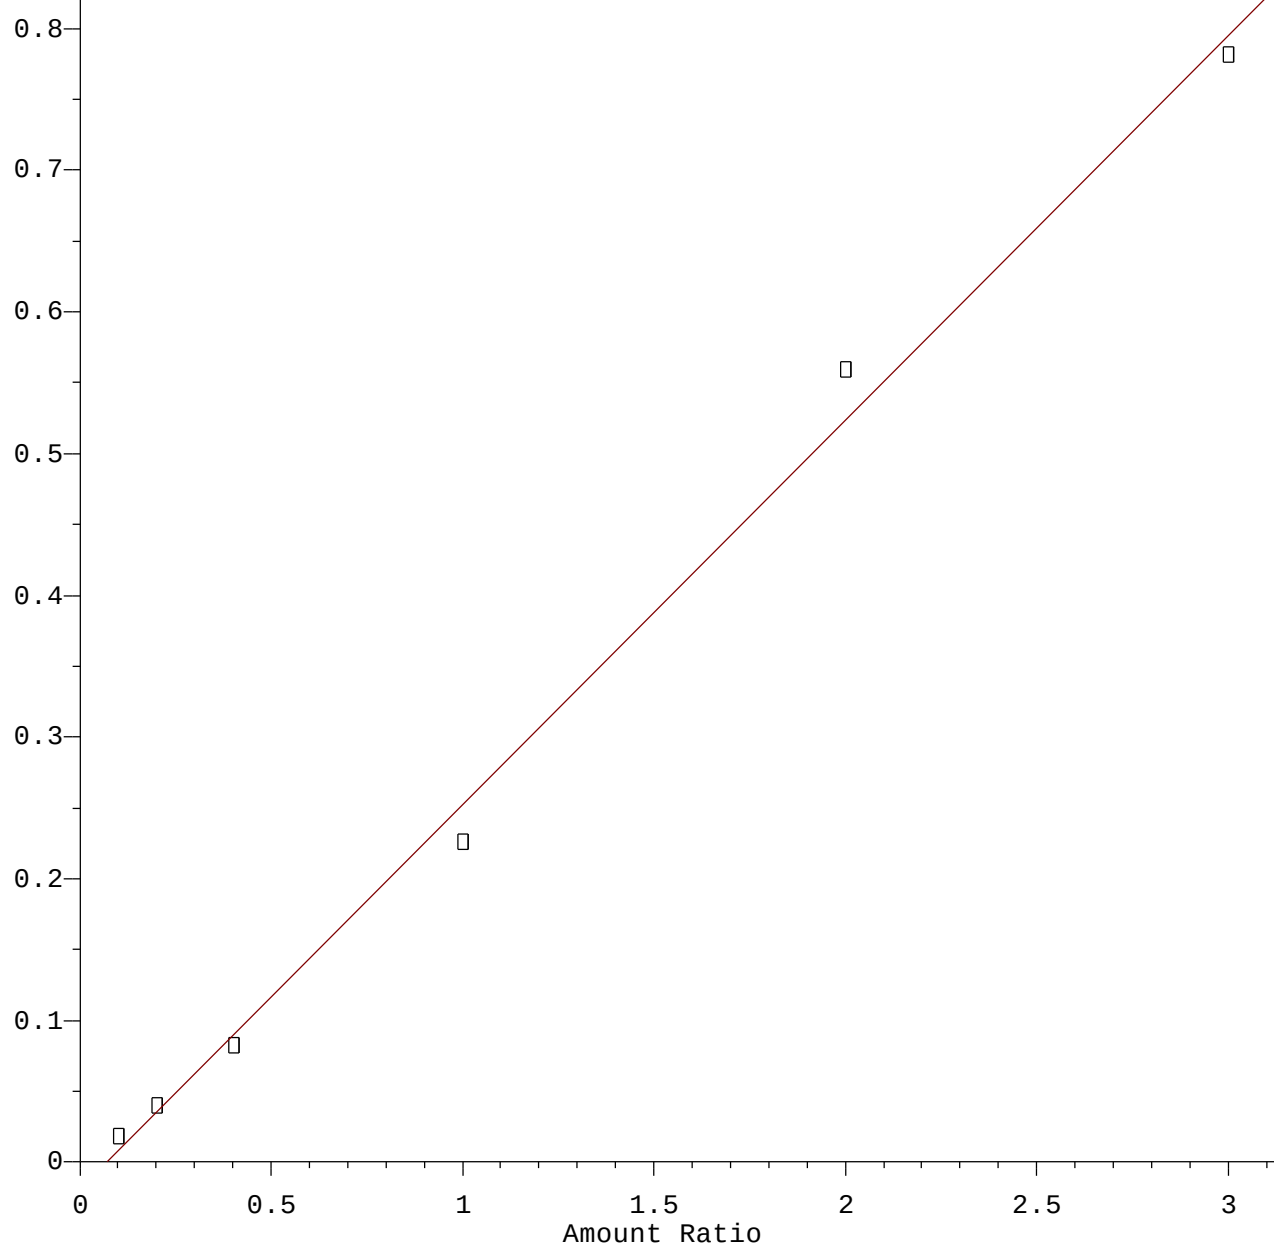


Resp Ratio =  $2.71 \times 10^{-1} \times \text{Amt} - 1.86 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.995    Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

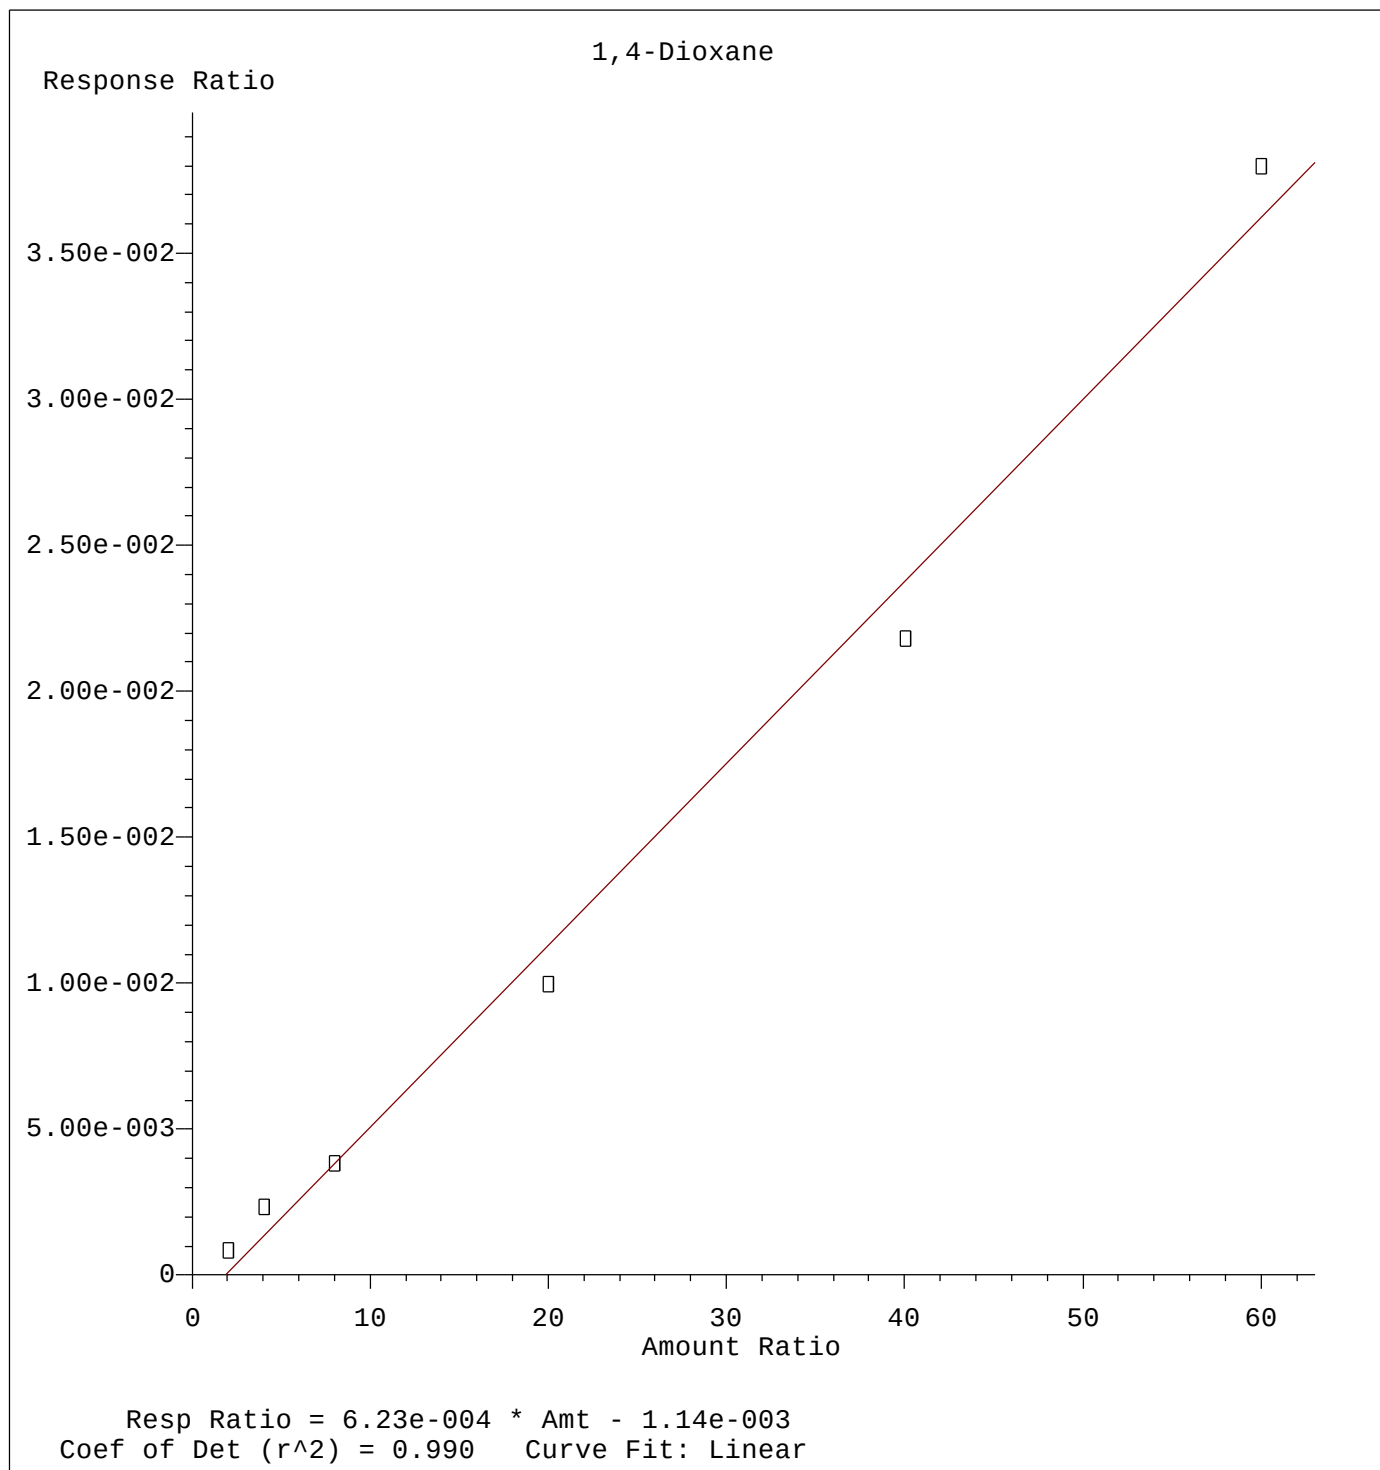


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

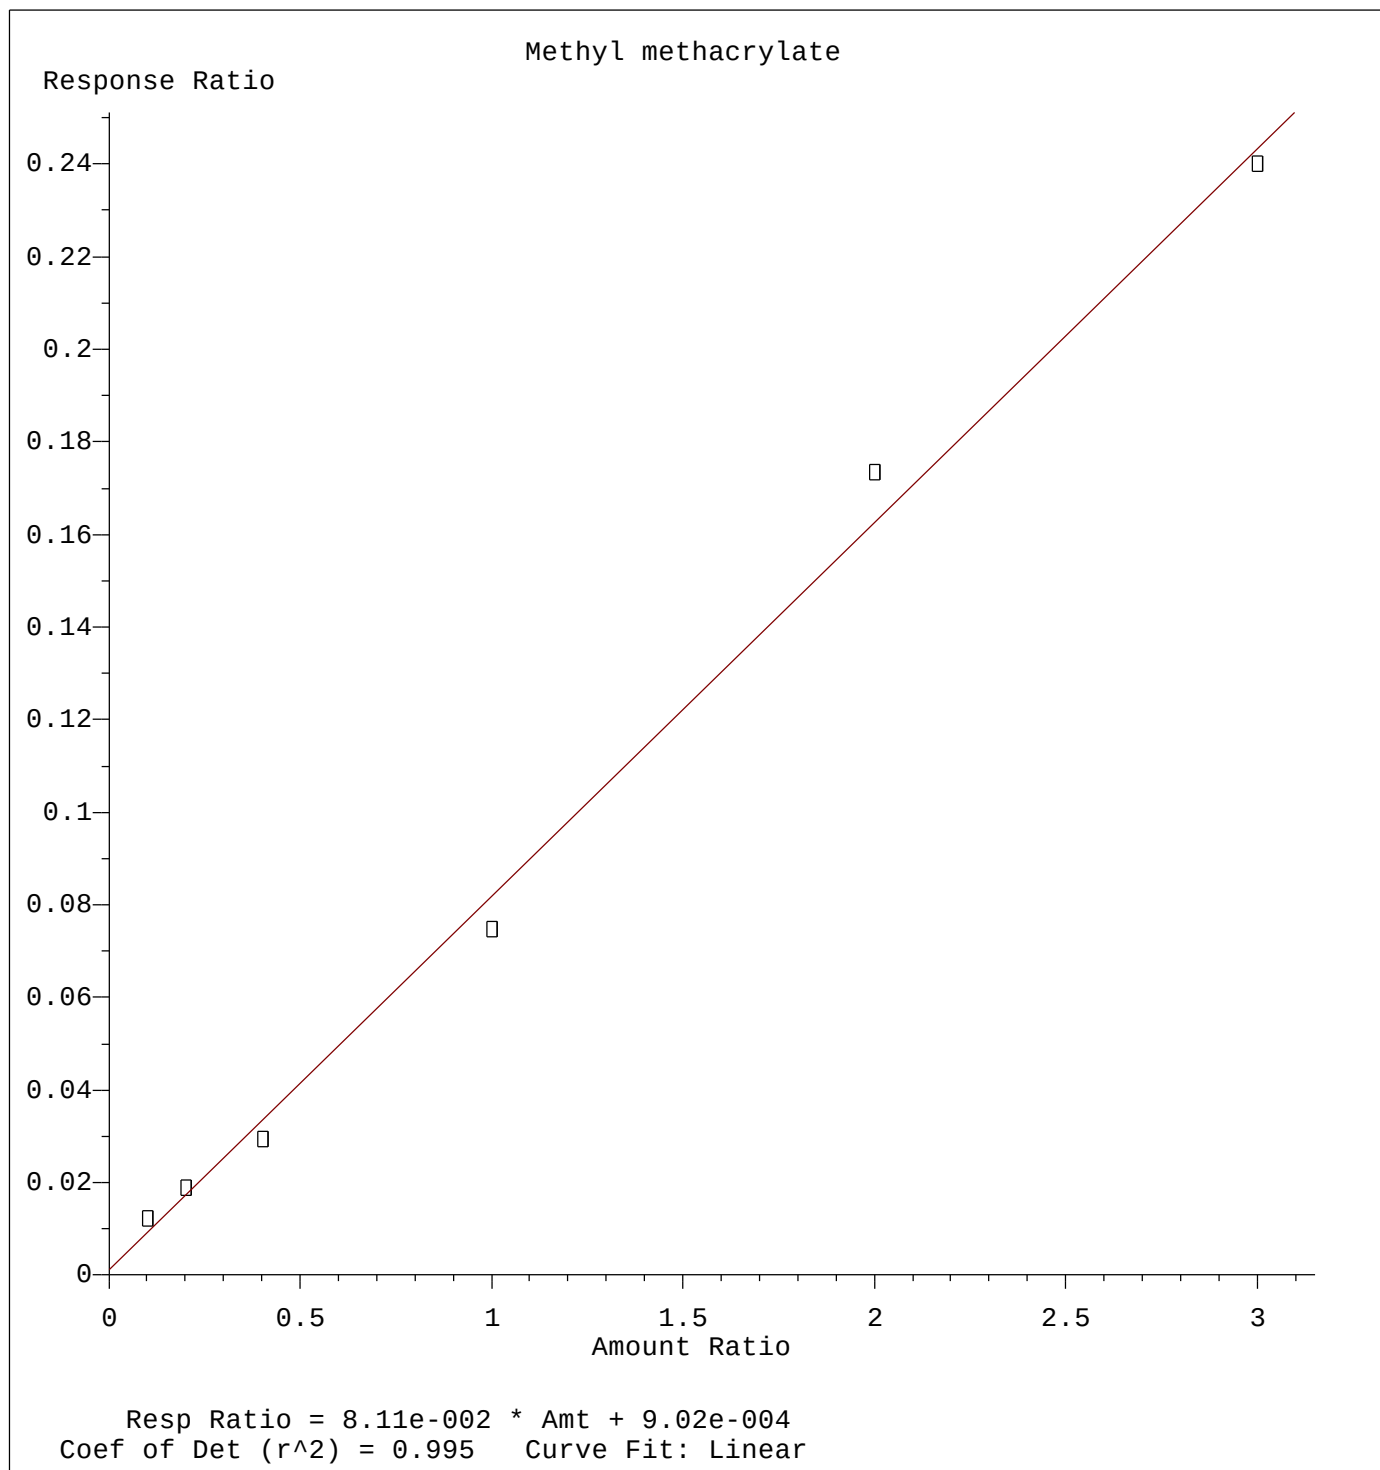


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

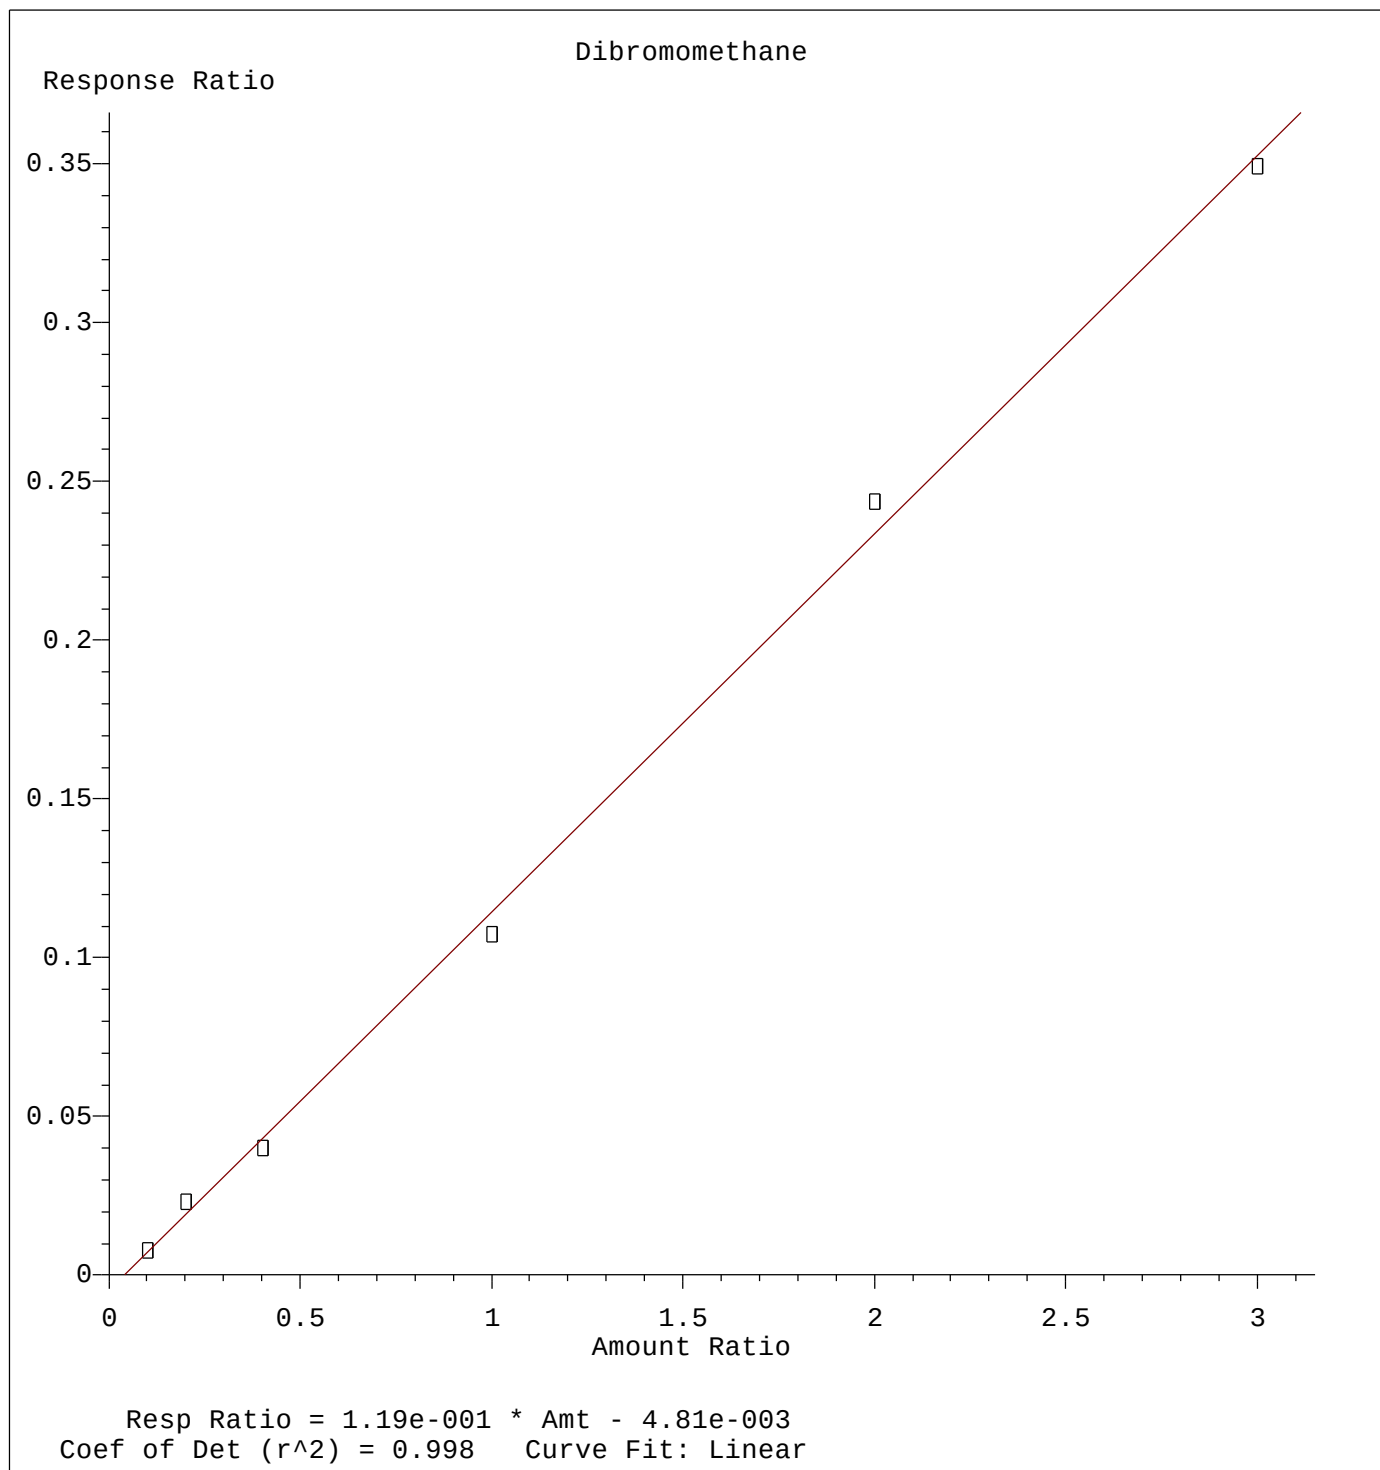

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

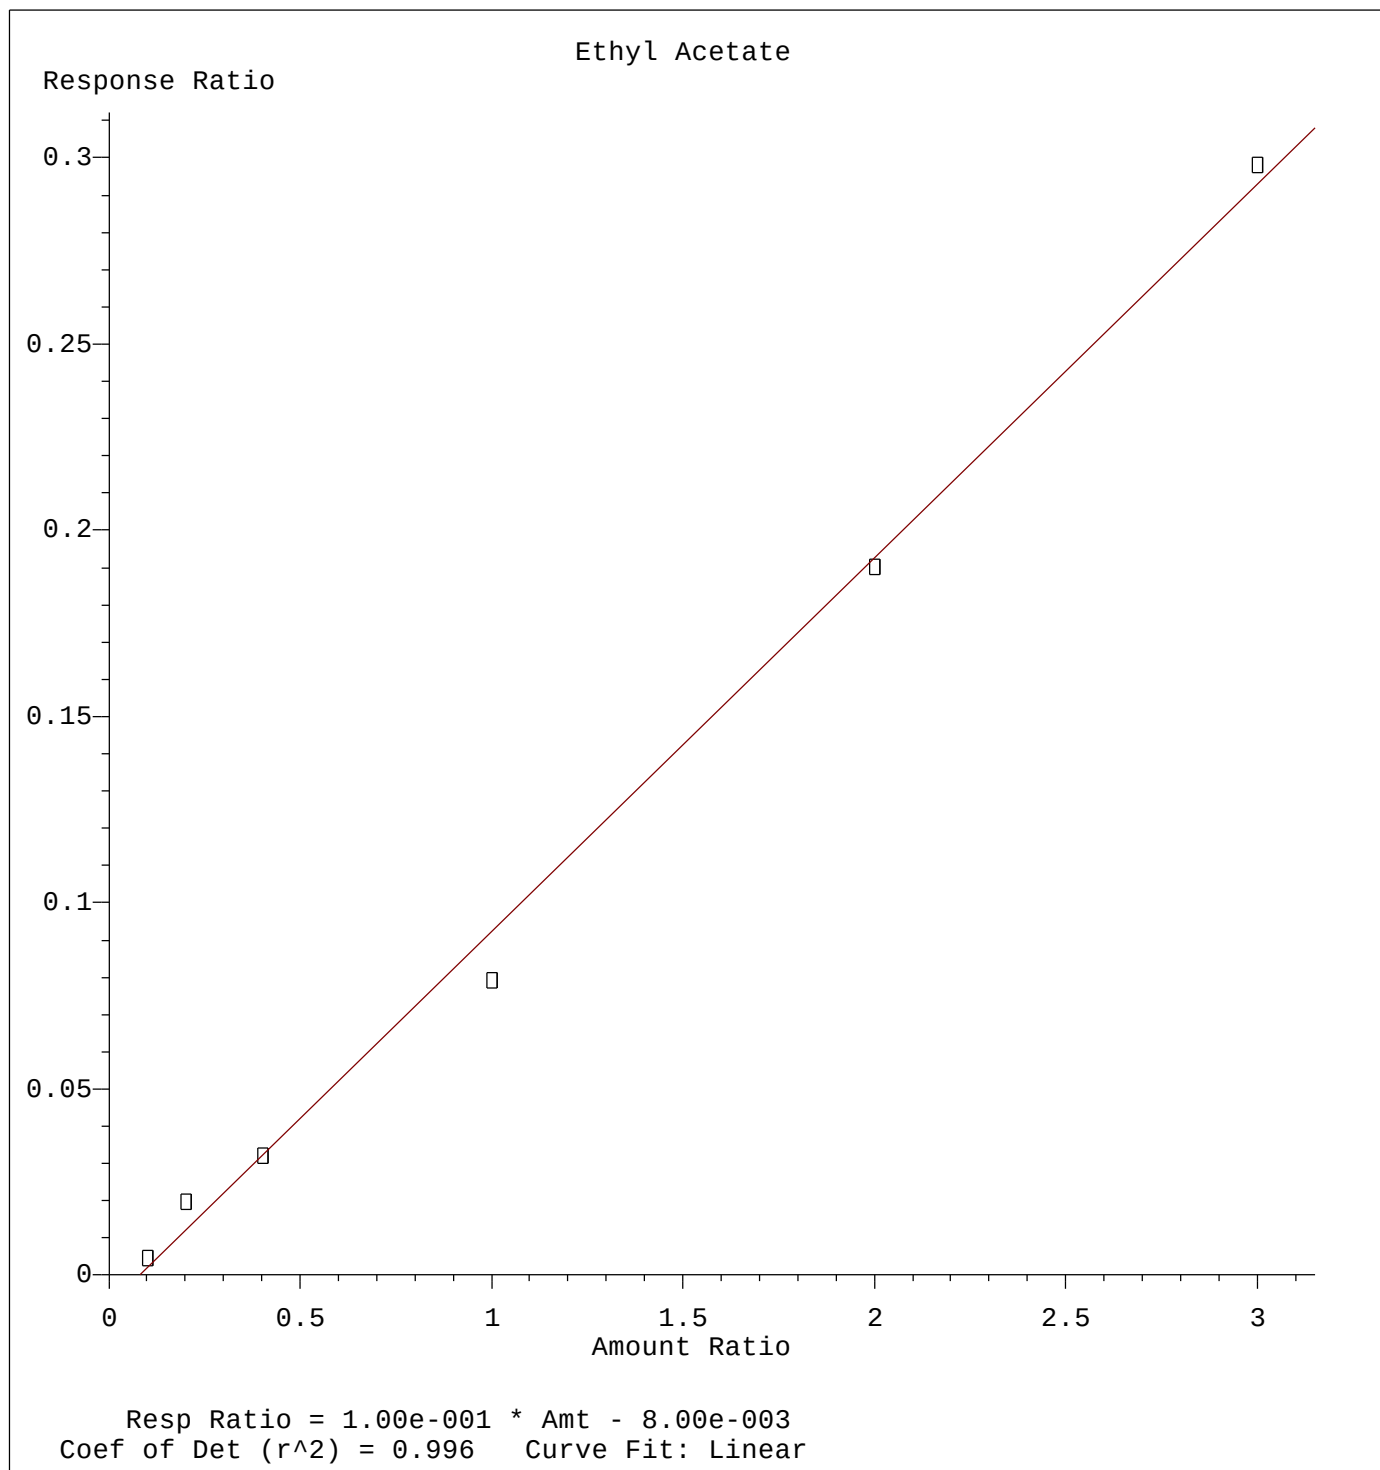


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

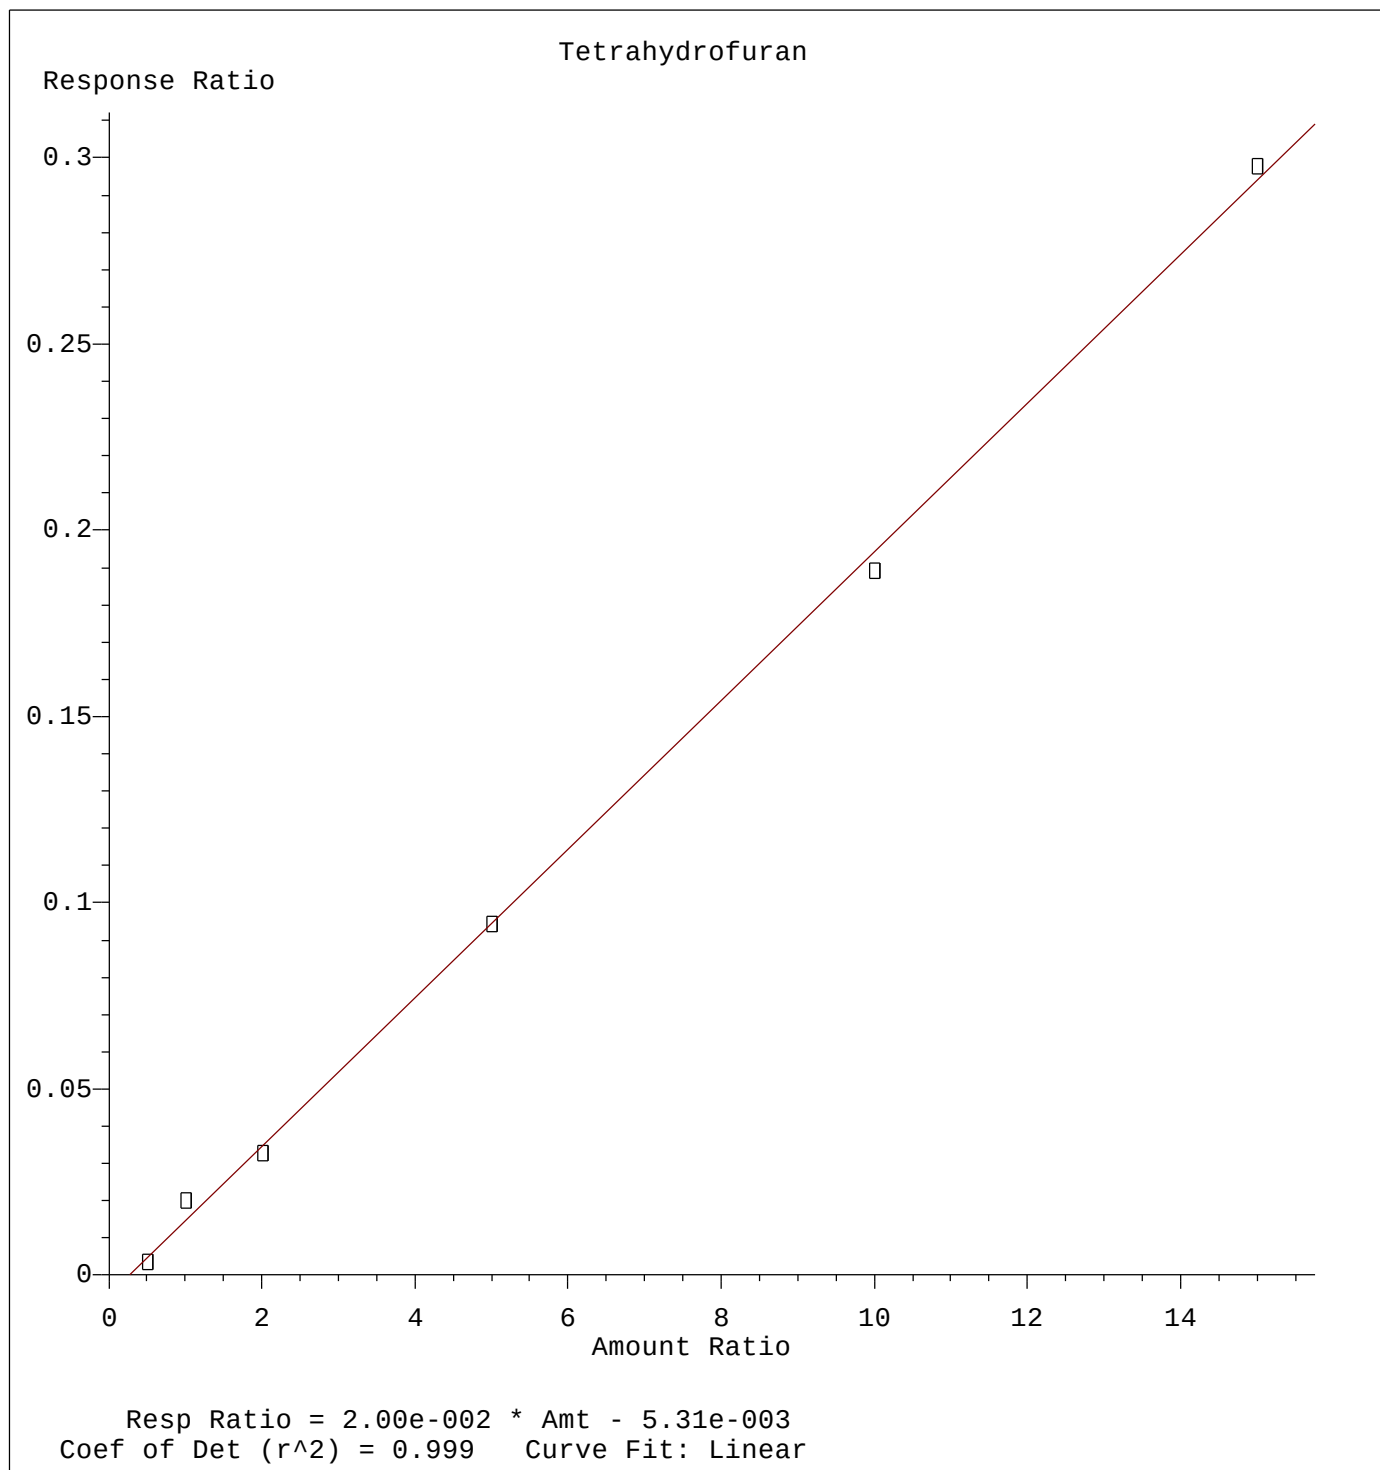

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

# 2,2-Dichloropropane


Response Ratio

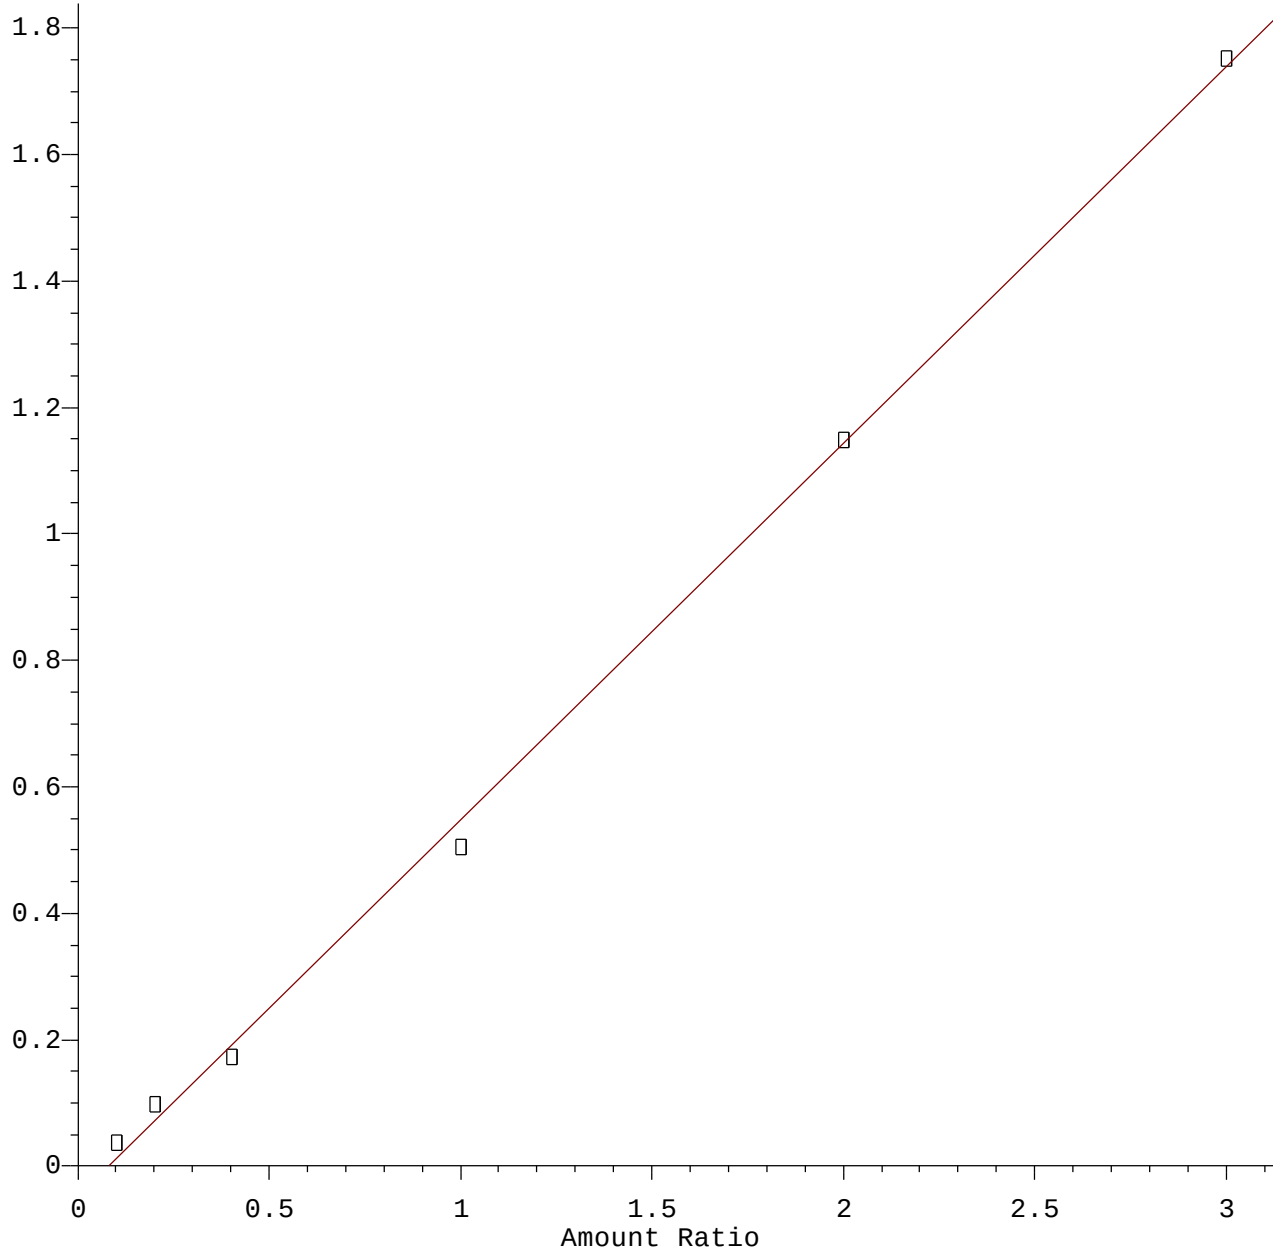

Resp Ratio =  $5.95 \times 10^{-1} \times \text{Amt} - 4.68 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.998    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018




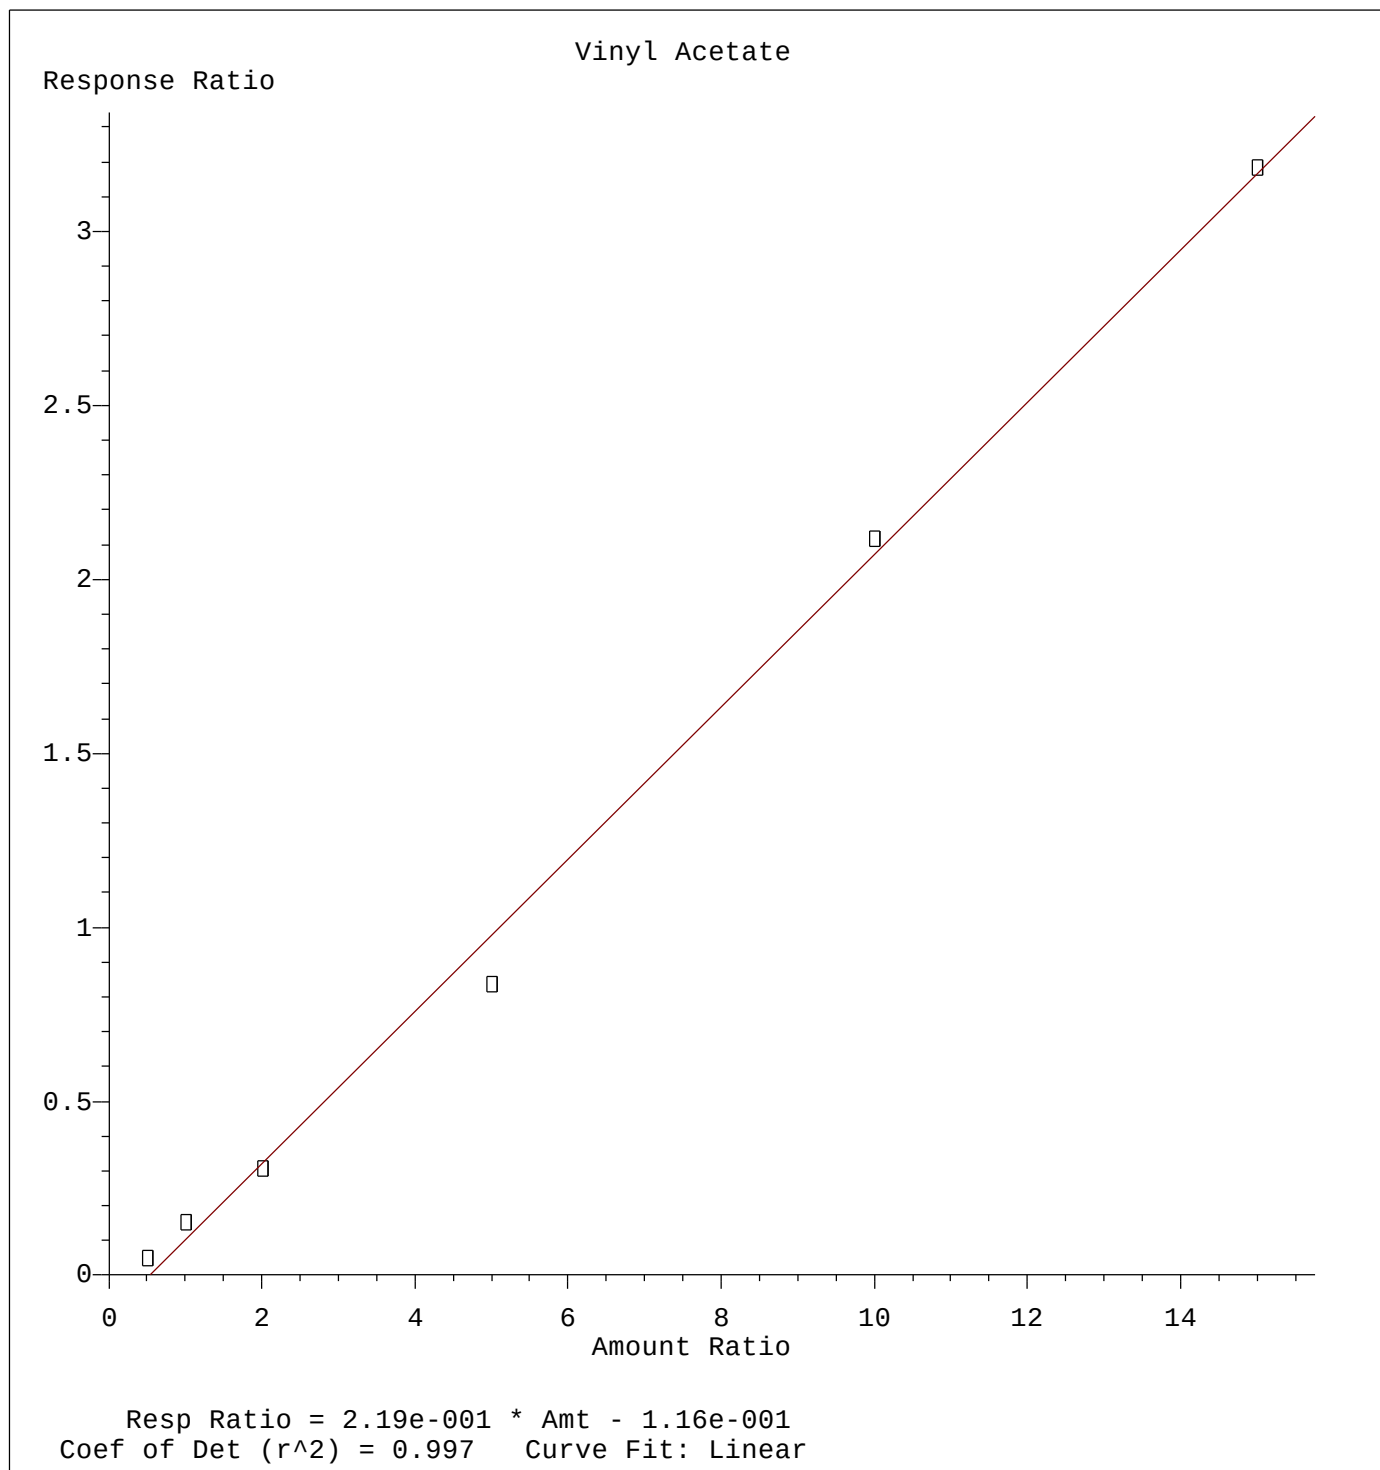

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018


# Methylene Chloride

Response Ratio

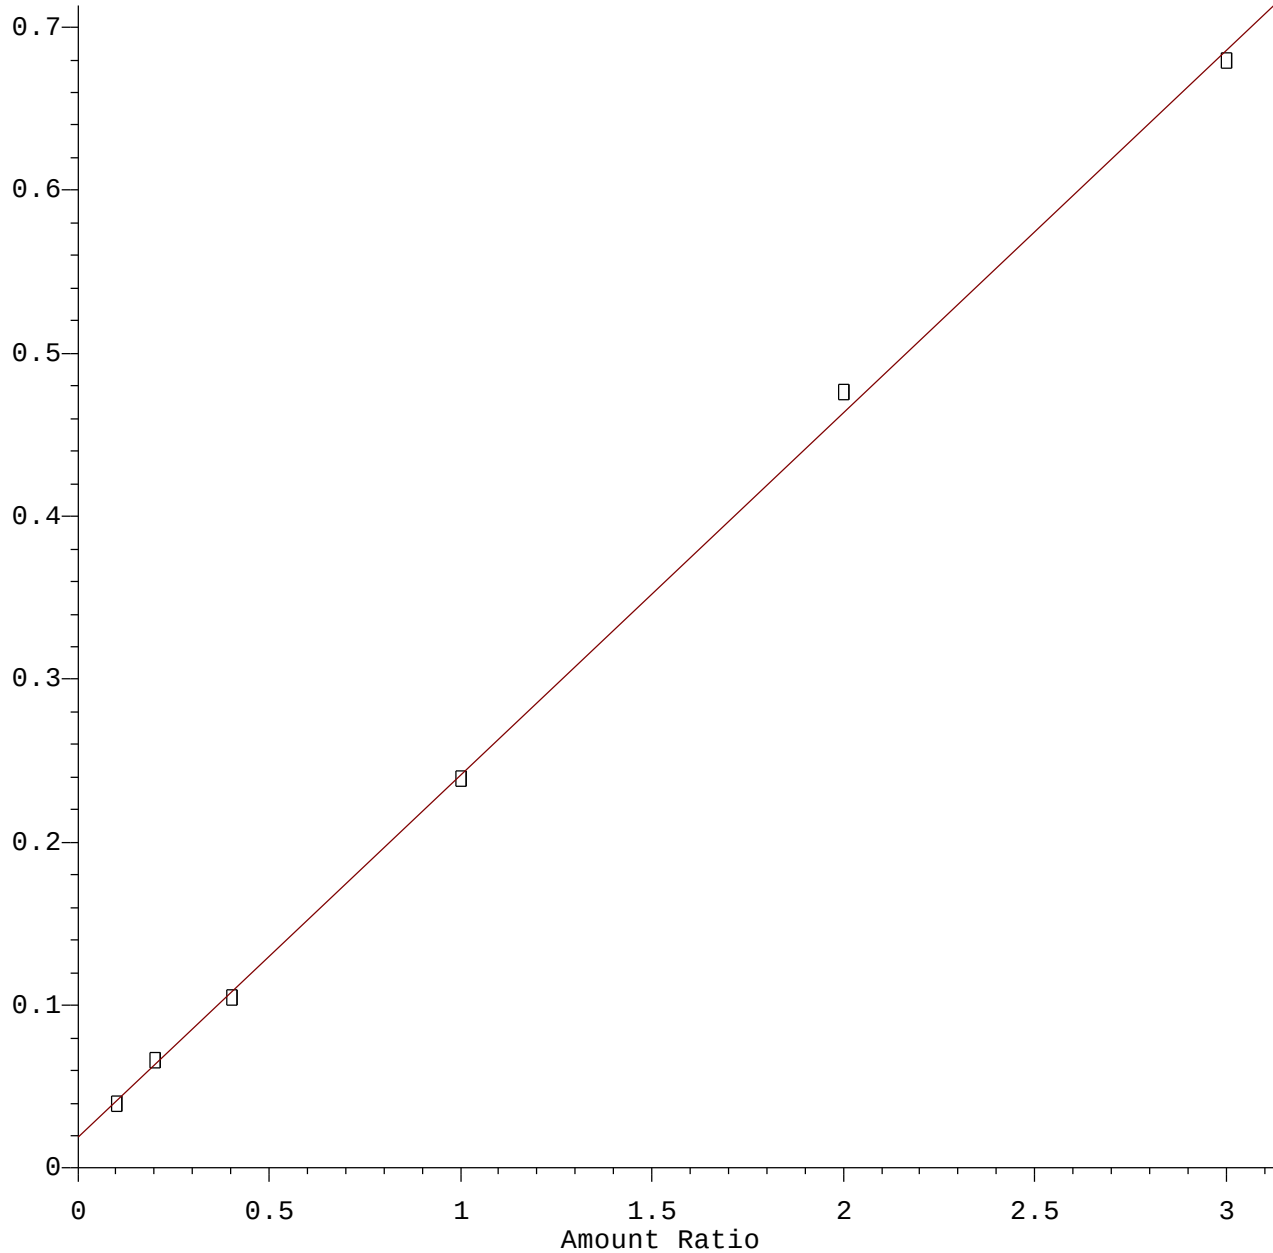


Resp Ratio =  $2.22 \times 10^{-1} \times \text{Amt} + 1.89 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

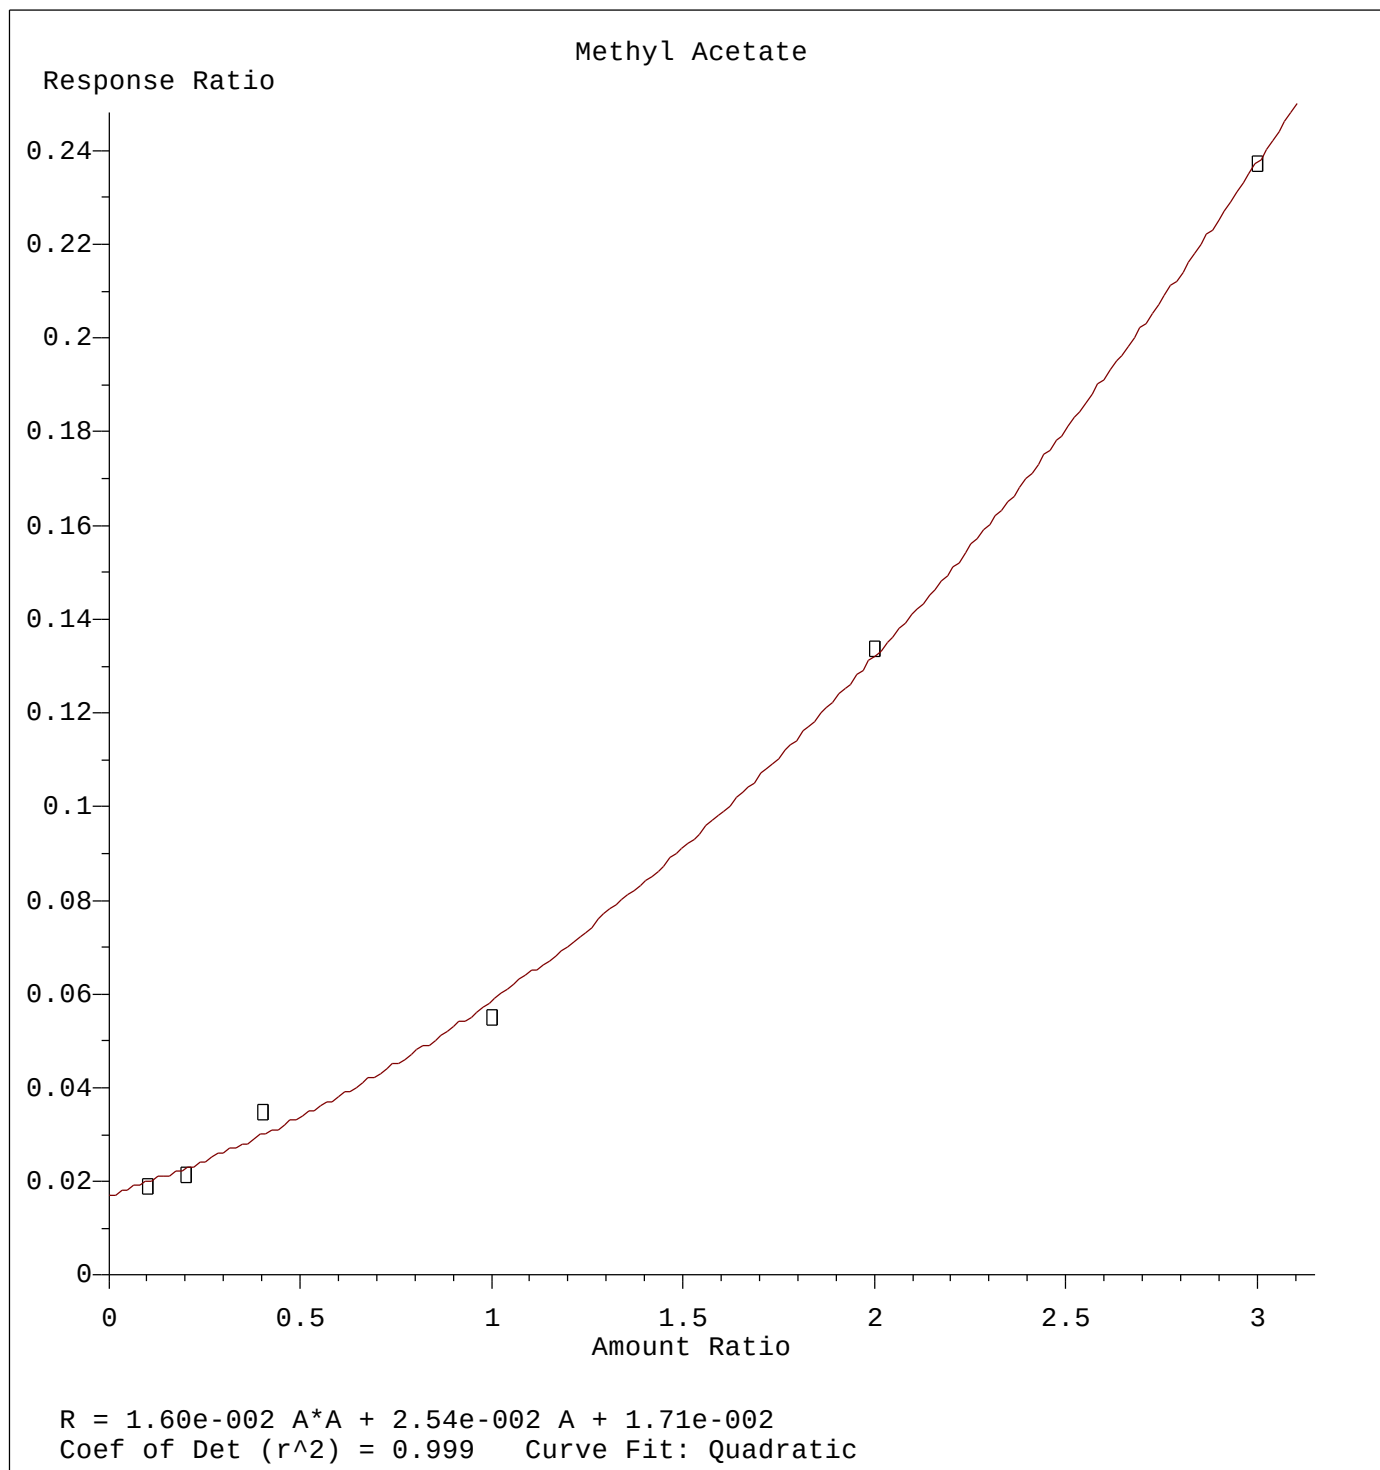

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018

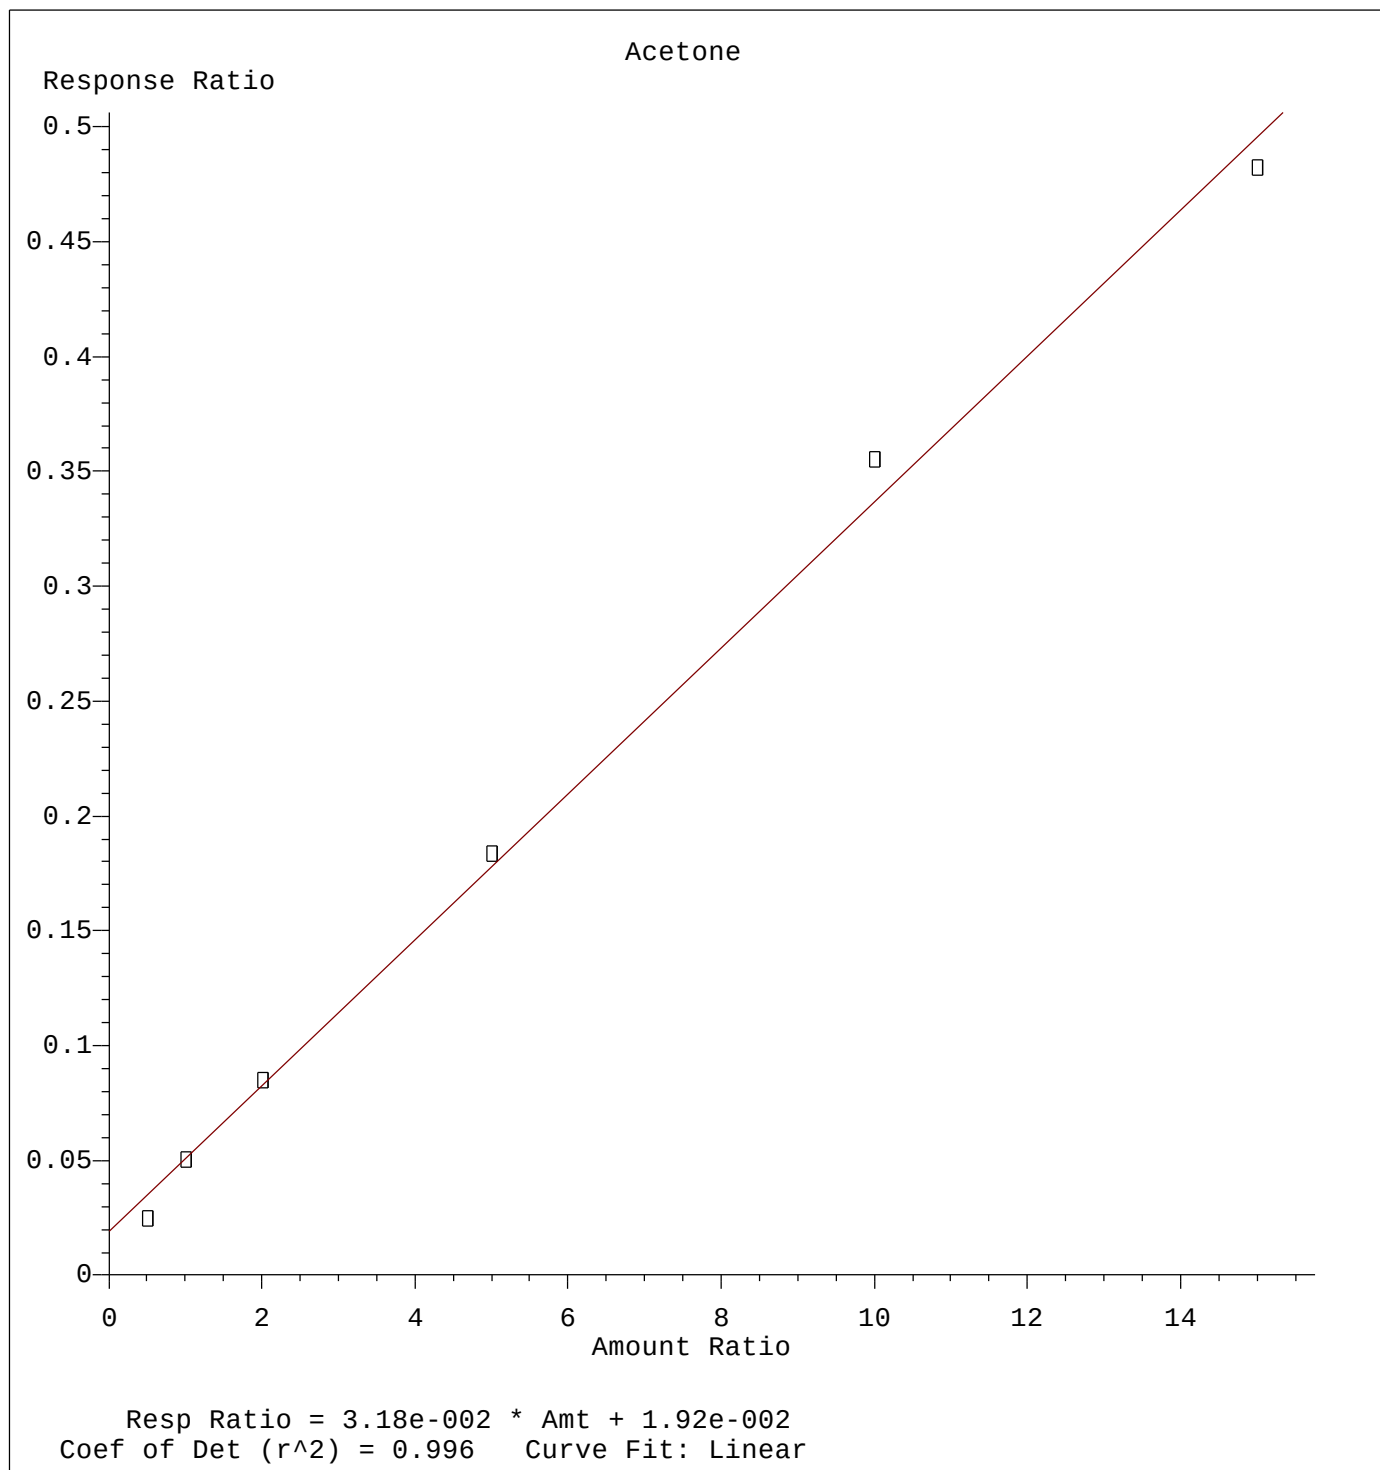

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F082918S.M  
Calibration Table Last Updated: Wed Aug 29 14:59:07 2018