


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF082918\
Data File : VF060165.D
Acq On : 28 Aug 2018 23:09
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F082918S.M
Title : SW846 8260
Last Update : Wed Aug 29 03:22:03 2018

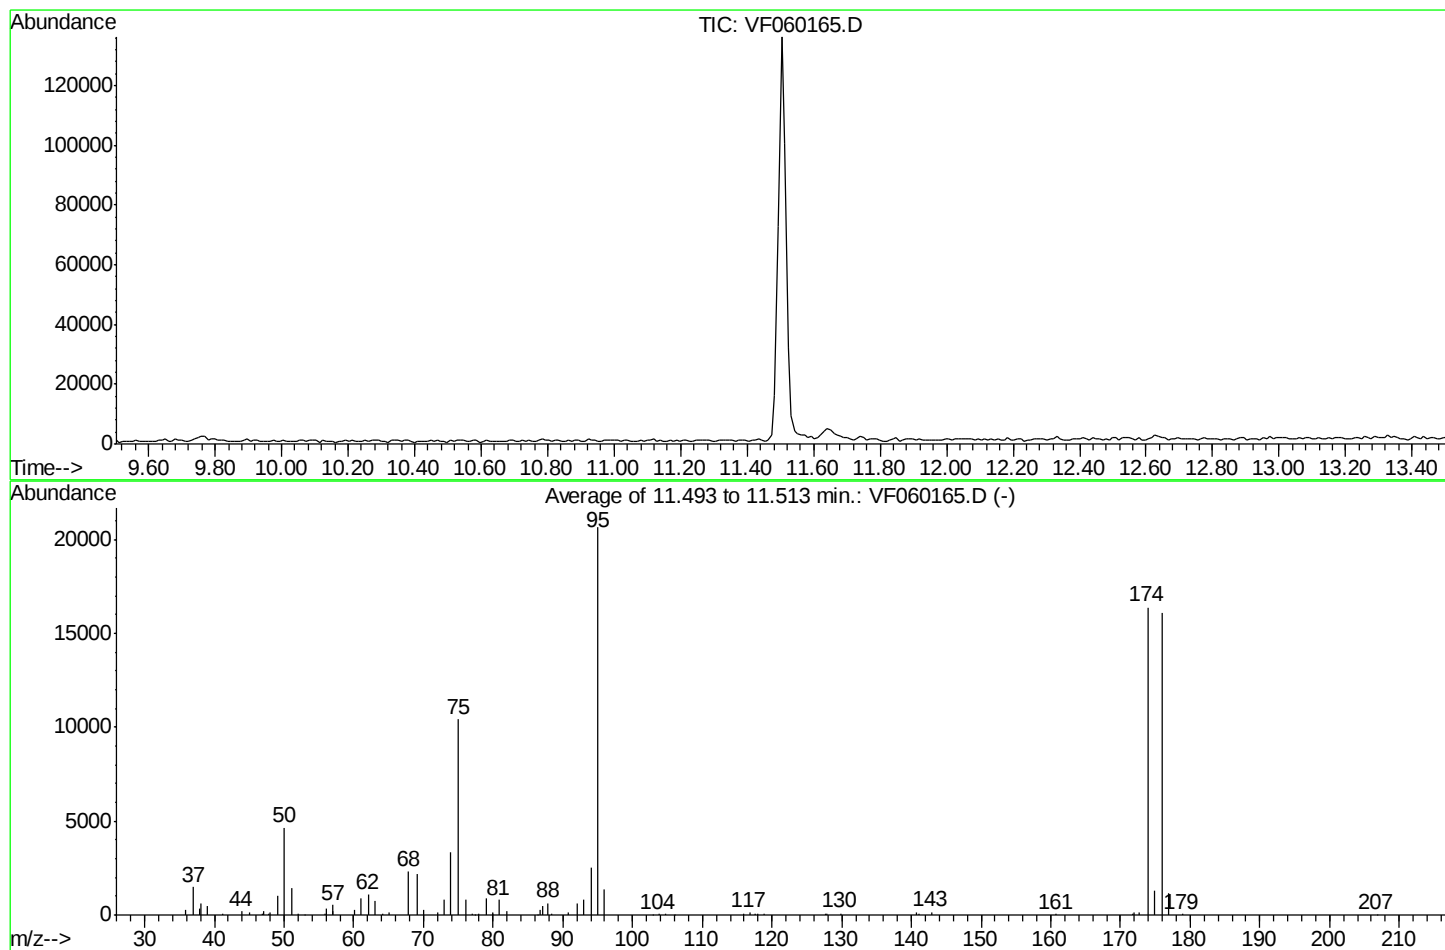

AutoFind: Scans 1112, 1113, 1114; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	4654	PASS
75	95	30	60	50.4	10410	PASS
95	95	100	100	100.0	20654	PASS
96	95	5	9	6.8	1399	PASS
173	174	0.00	2	1.0	163	PASS
174	95	50	100	79.3	16377	PASS
175	174	5	9	8.1	1319	PASS
176	174	95	101	98.5	16128	PASS
177	176	5	9	7.2	1169	PASS