


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF083018\
Data File : VF060188.D
Acq On : 29 Aug 2018 13:16
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F083018S.M
Title : SW846 8260
Last Update : Thu Aug 30 08:36:31 2018

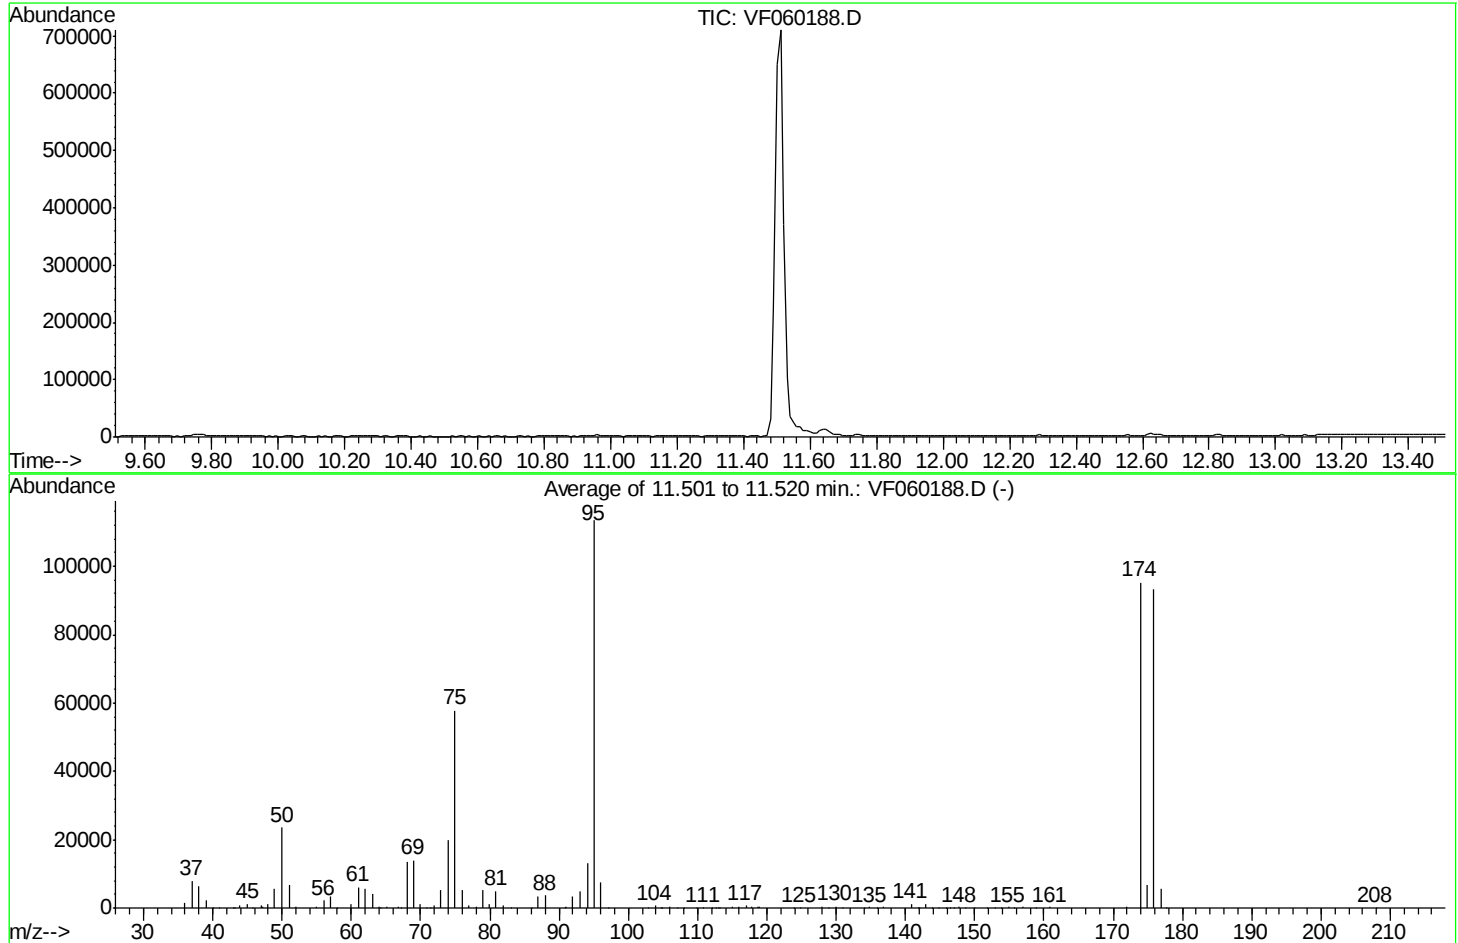

AutoFind: Scans 1113, 1114, 1115; Background Corrected with Scan 1107

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	23579	PASS
75	95	30	60	51.0	57858	PASS
95	95	100	100	100.0	113472	PASS
96	95	5	9	6.8	7683	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.9	95184	PASS
175	174	5	9	7.0	6663	PASS
176	174	95	101	98.1	93373	PASS
177	176	5	9	6.2	5761	PASS