



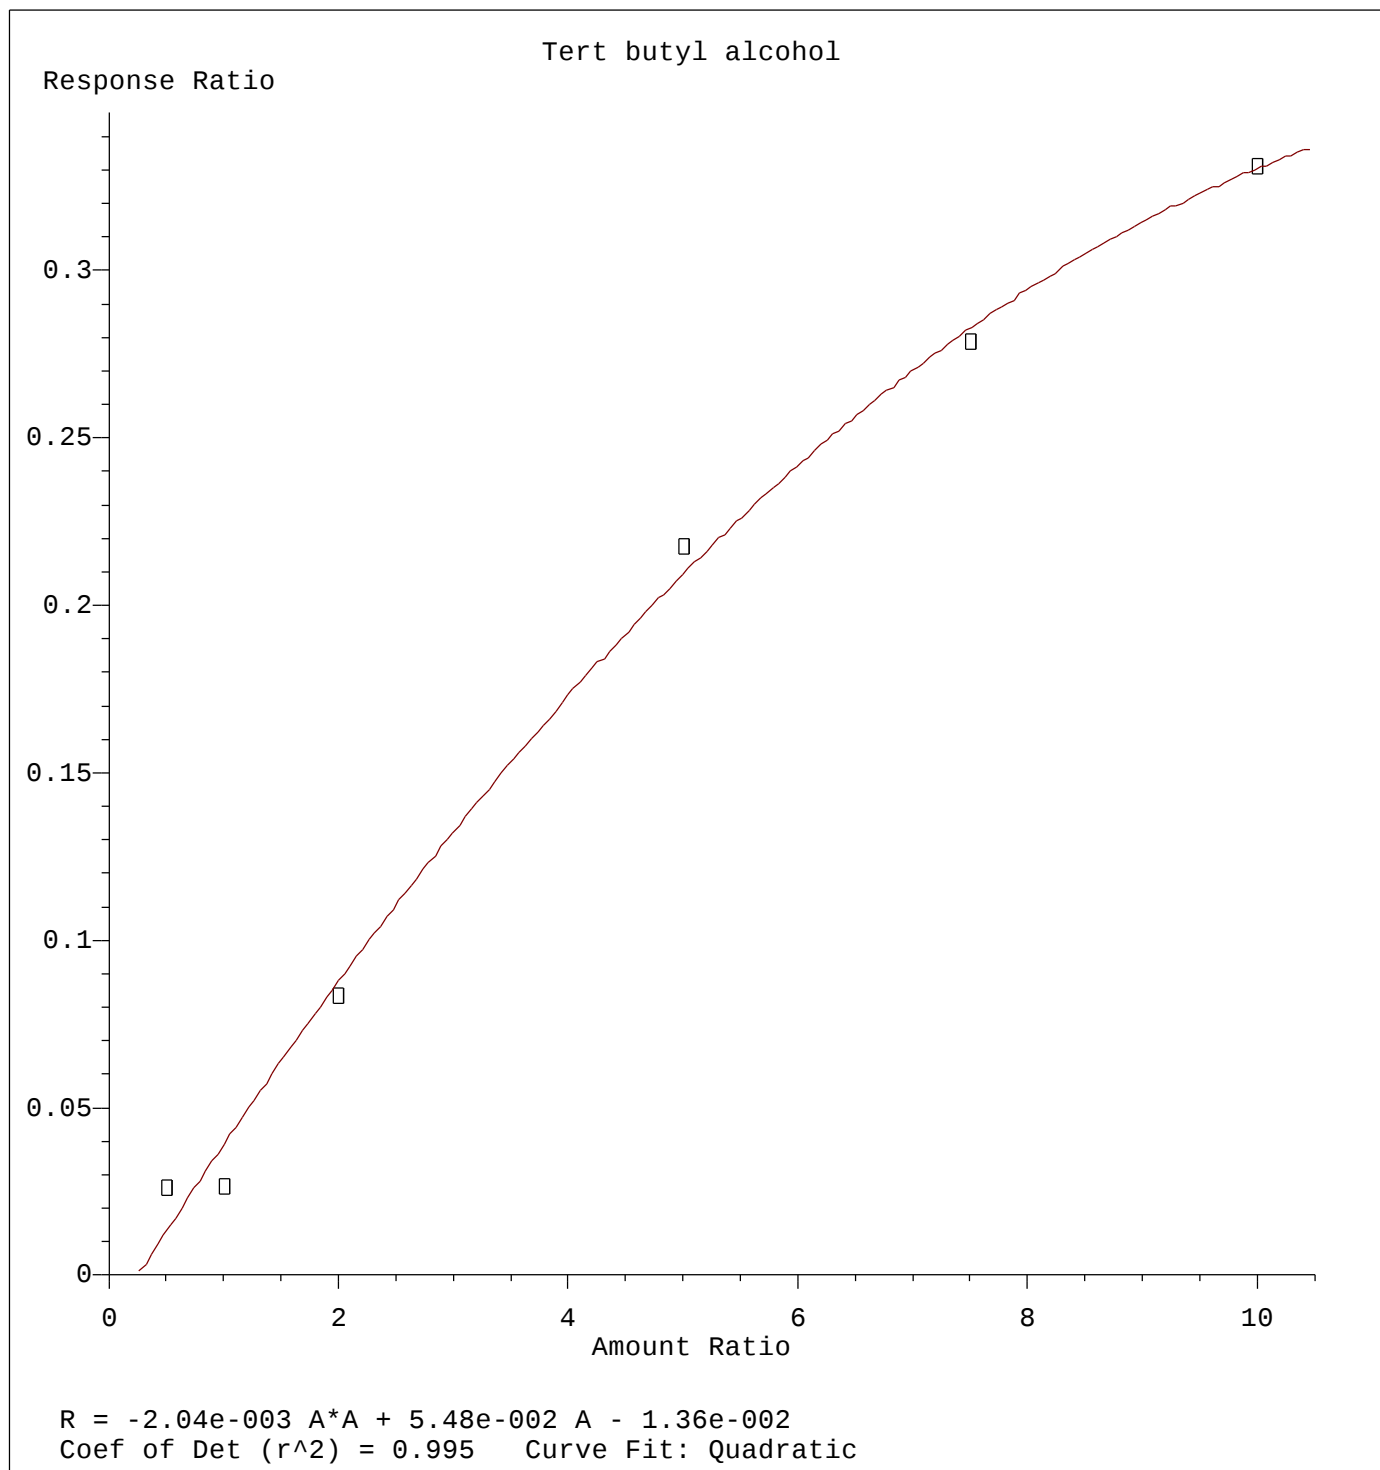


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

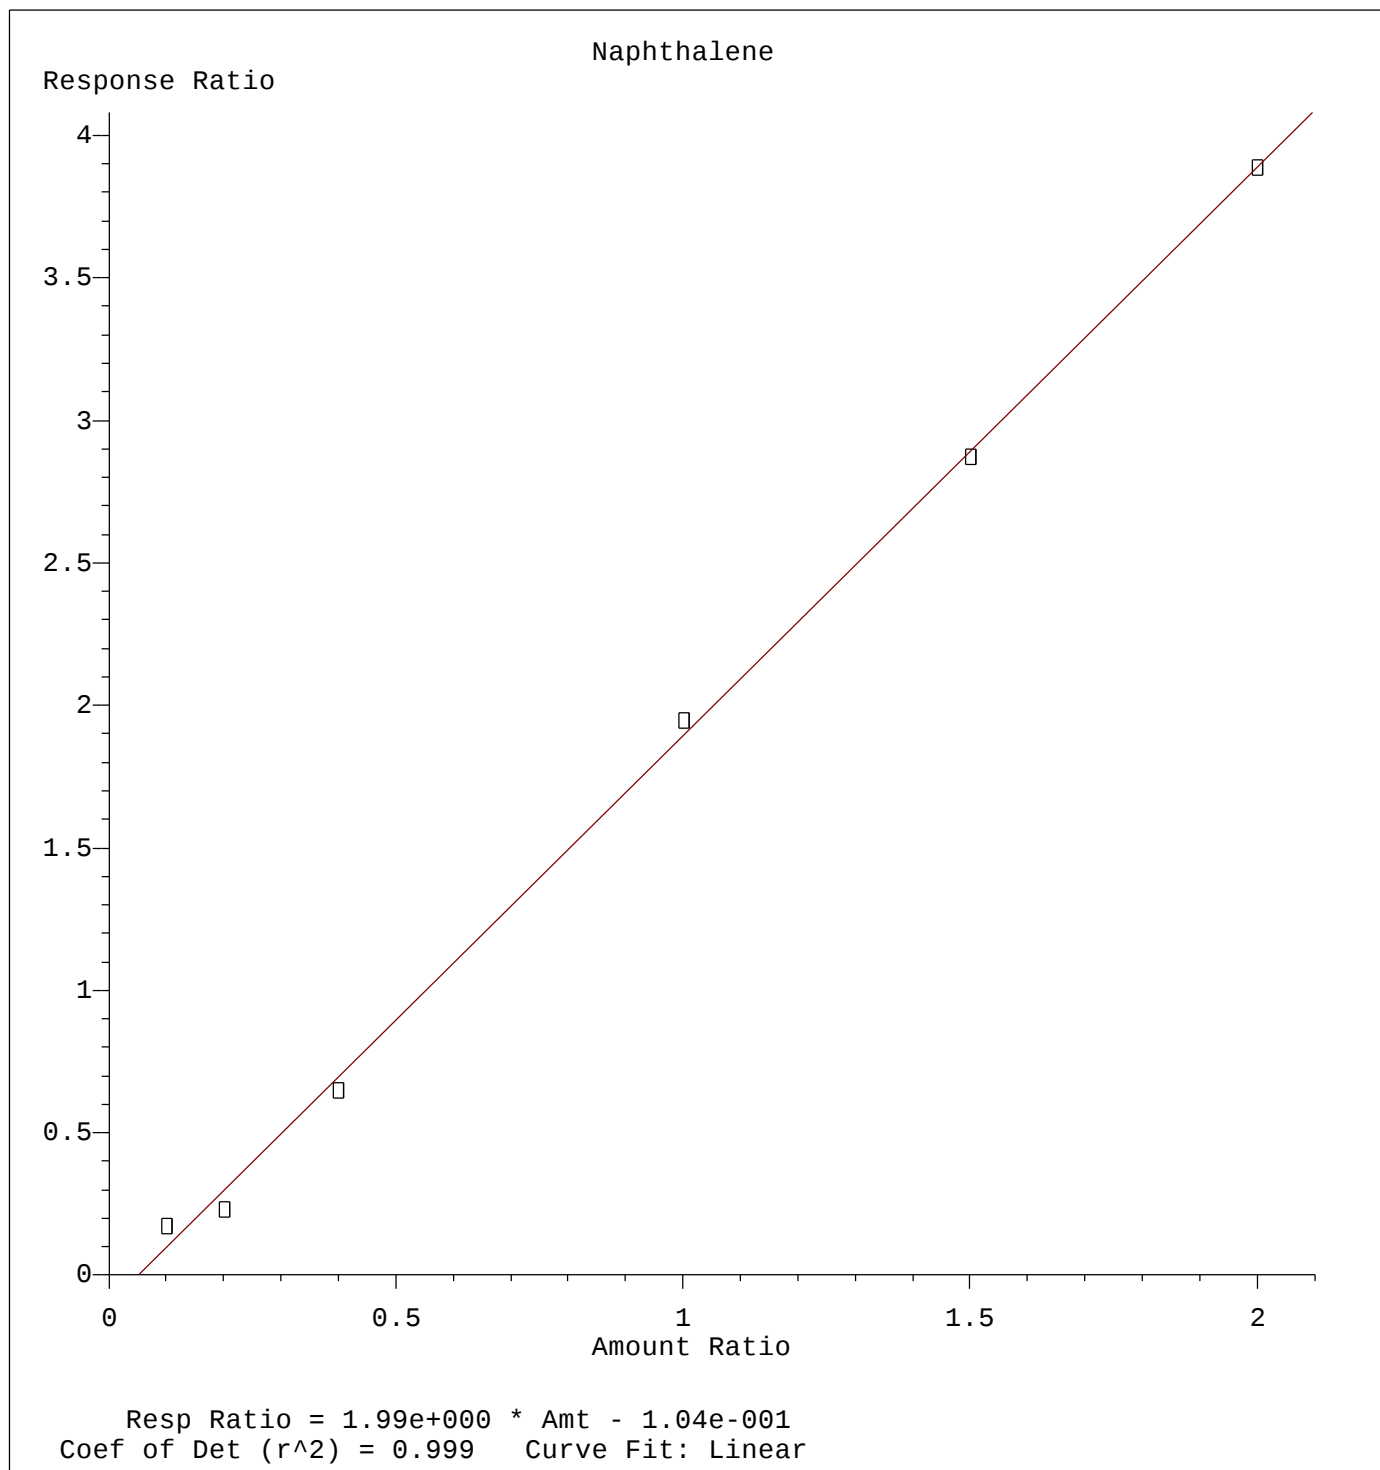


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

trans-1,4-Dichloro-2-butene

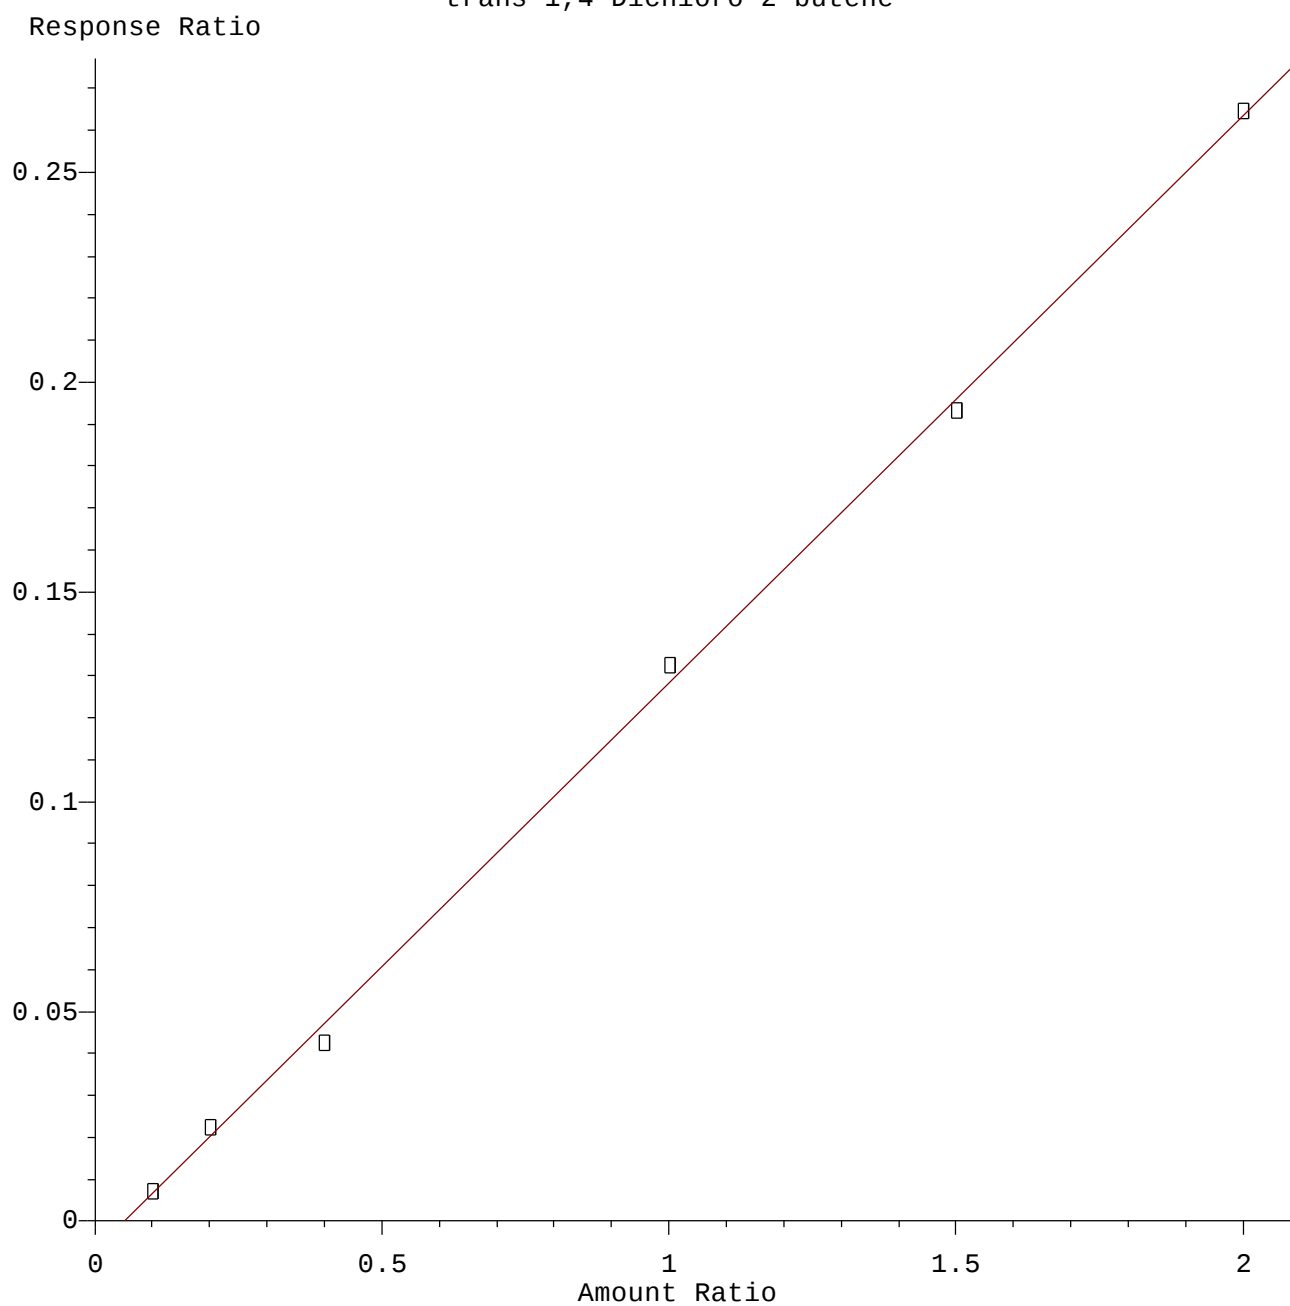


Resp Ratio = $1.35 \times 10^{-1} \times \text{Amt} - 6.88 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

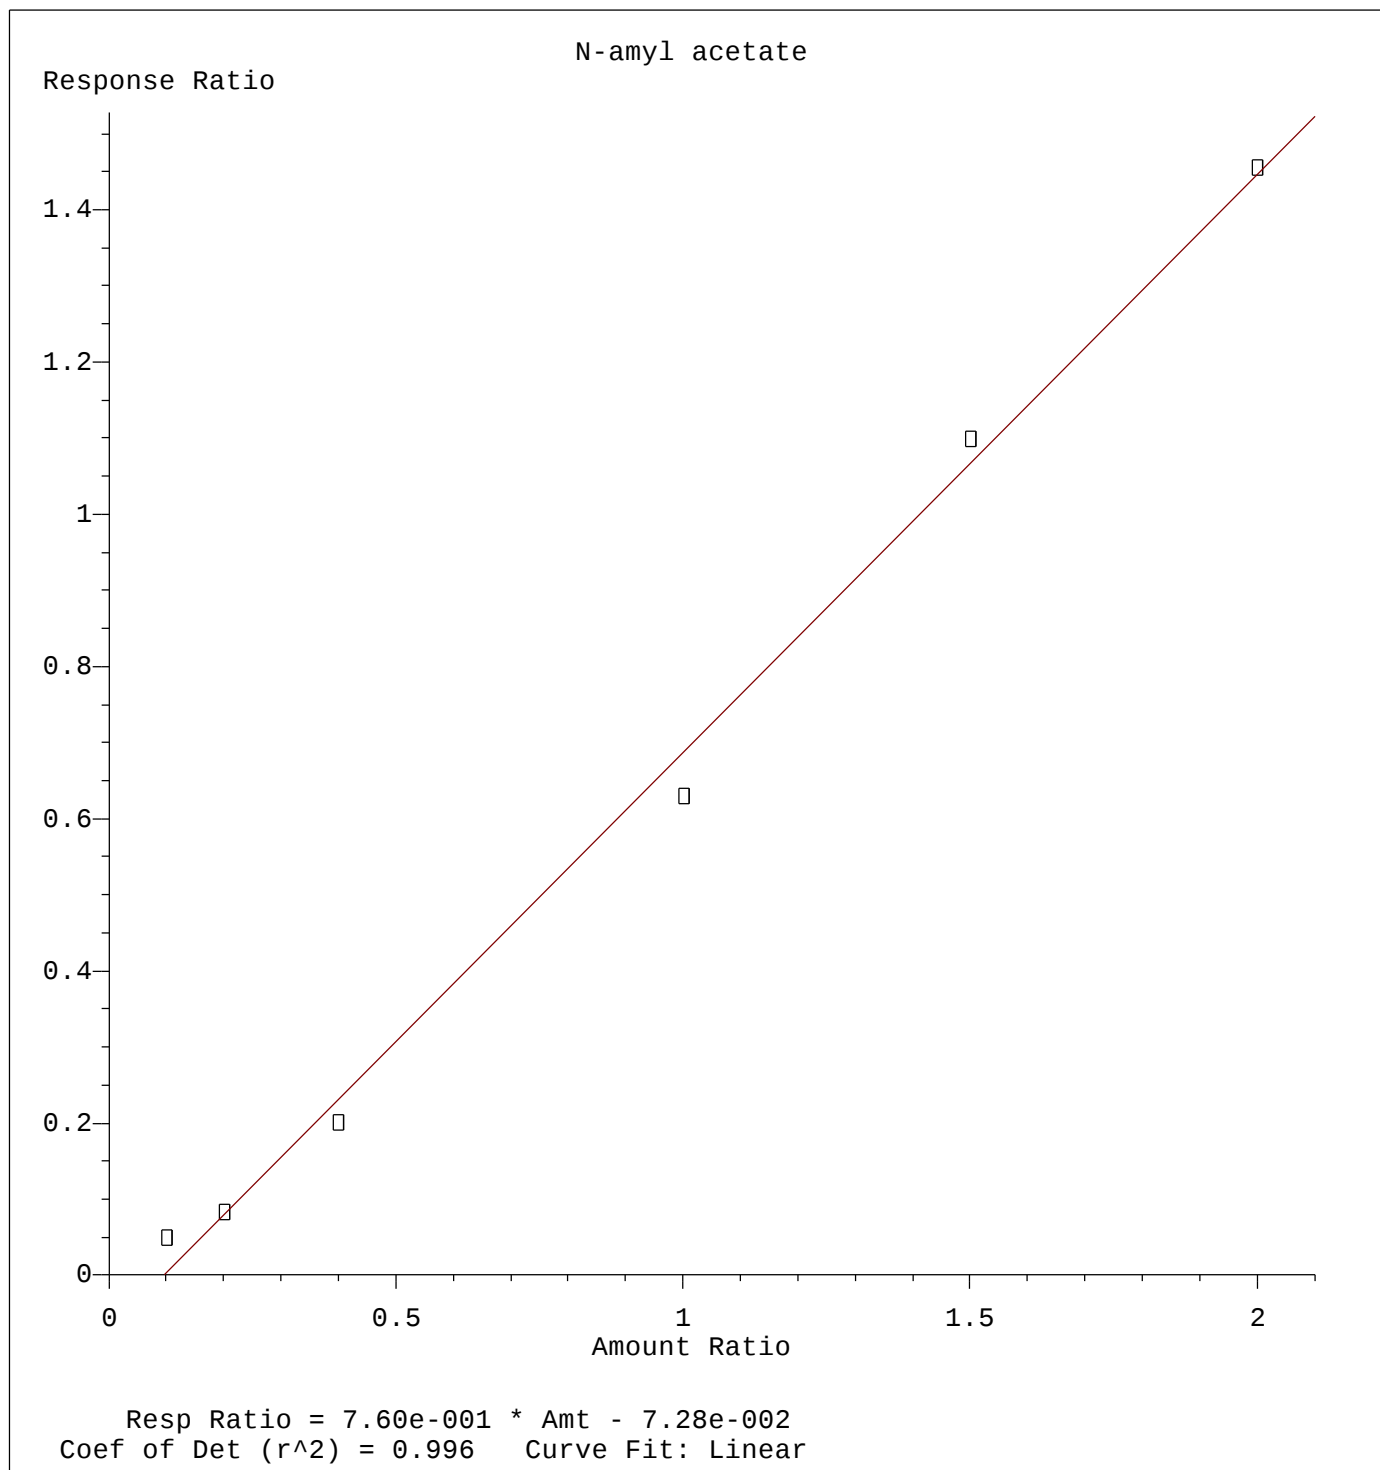


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

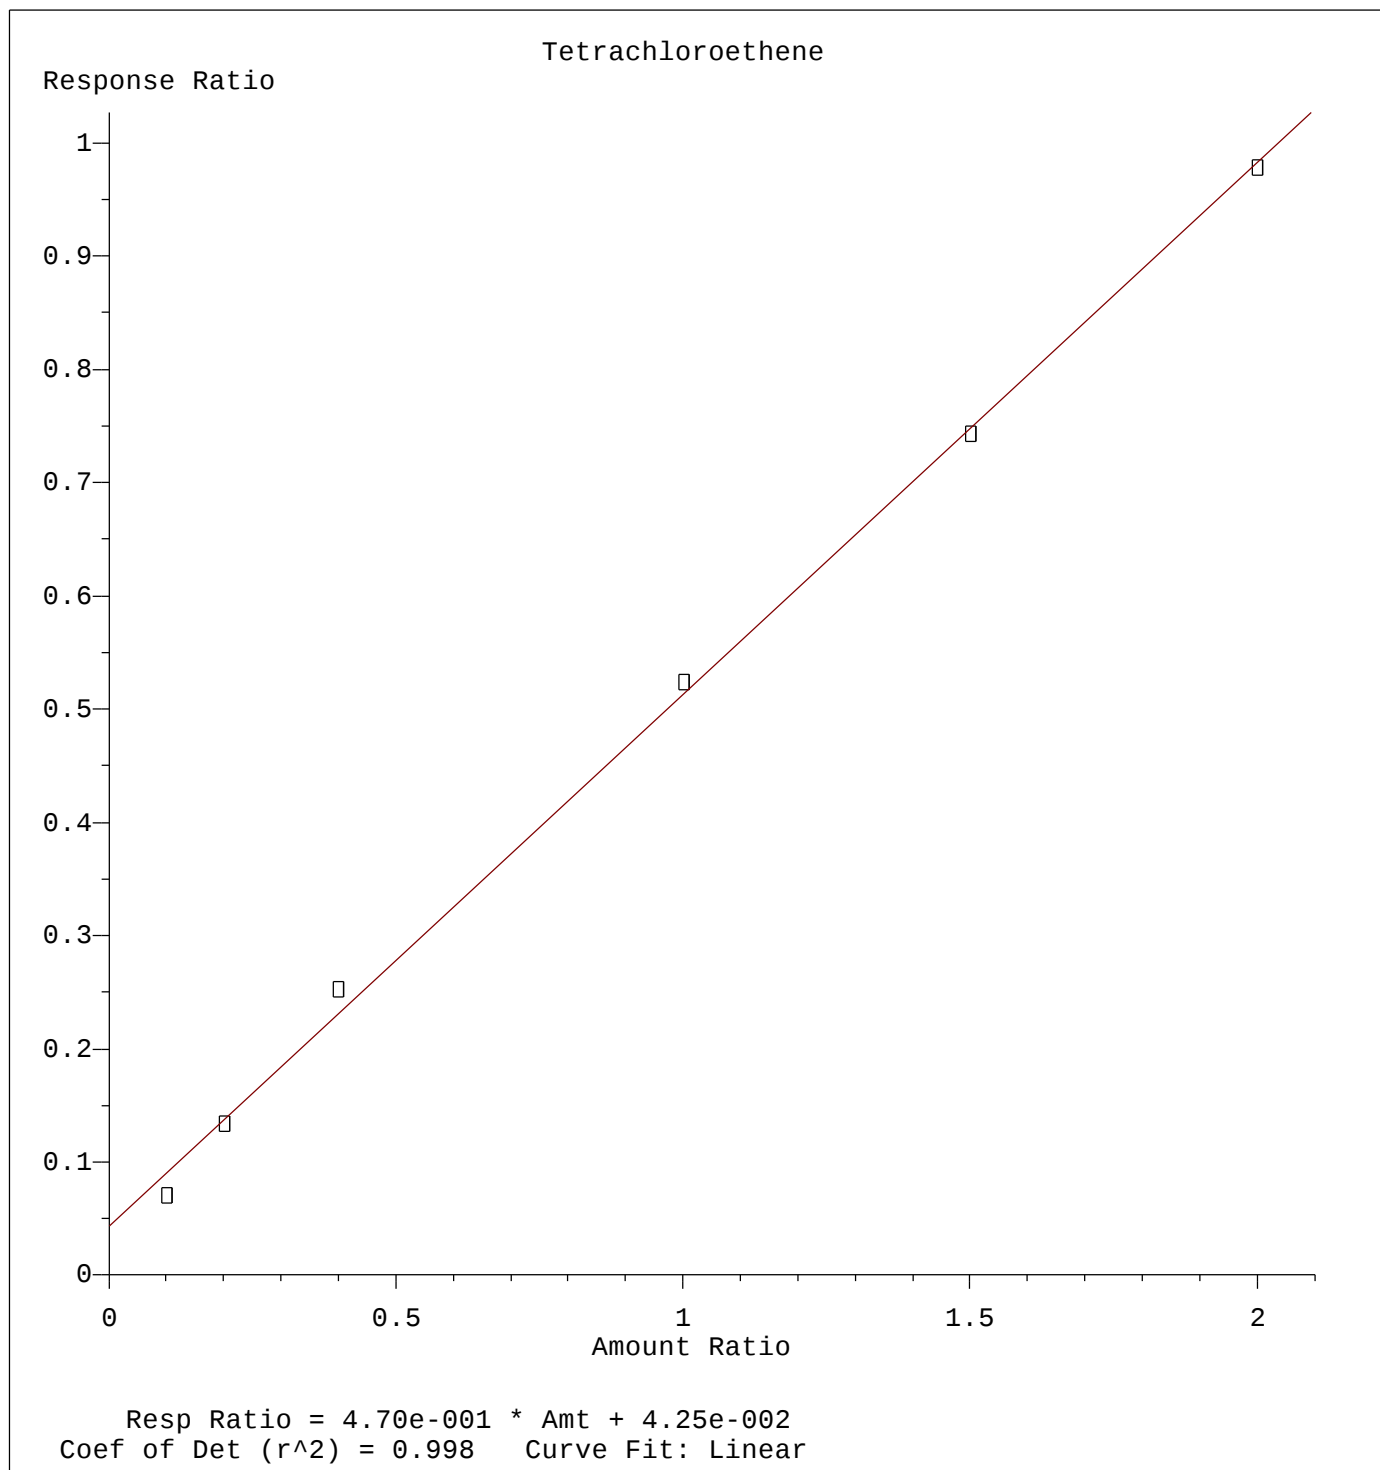

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018


2-Hexanone

Response Ratio

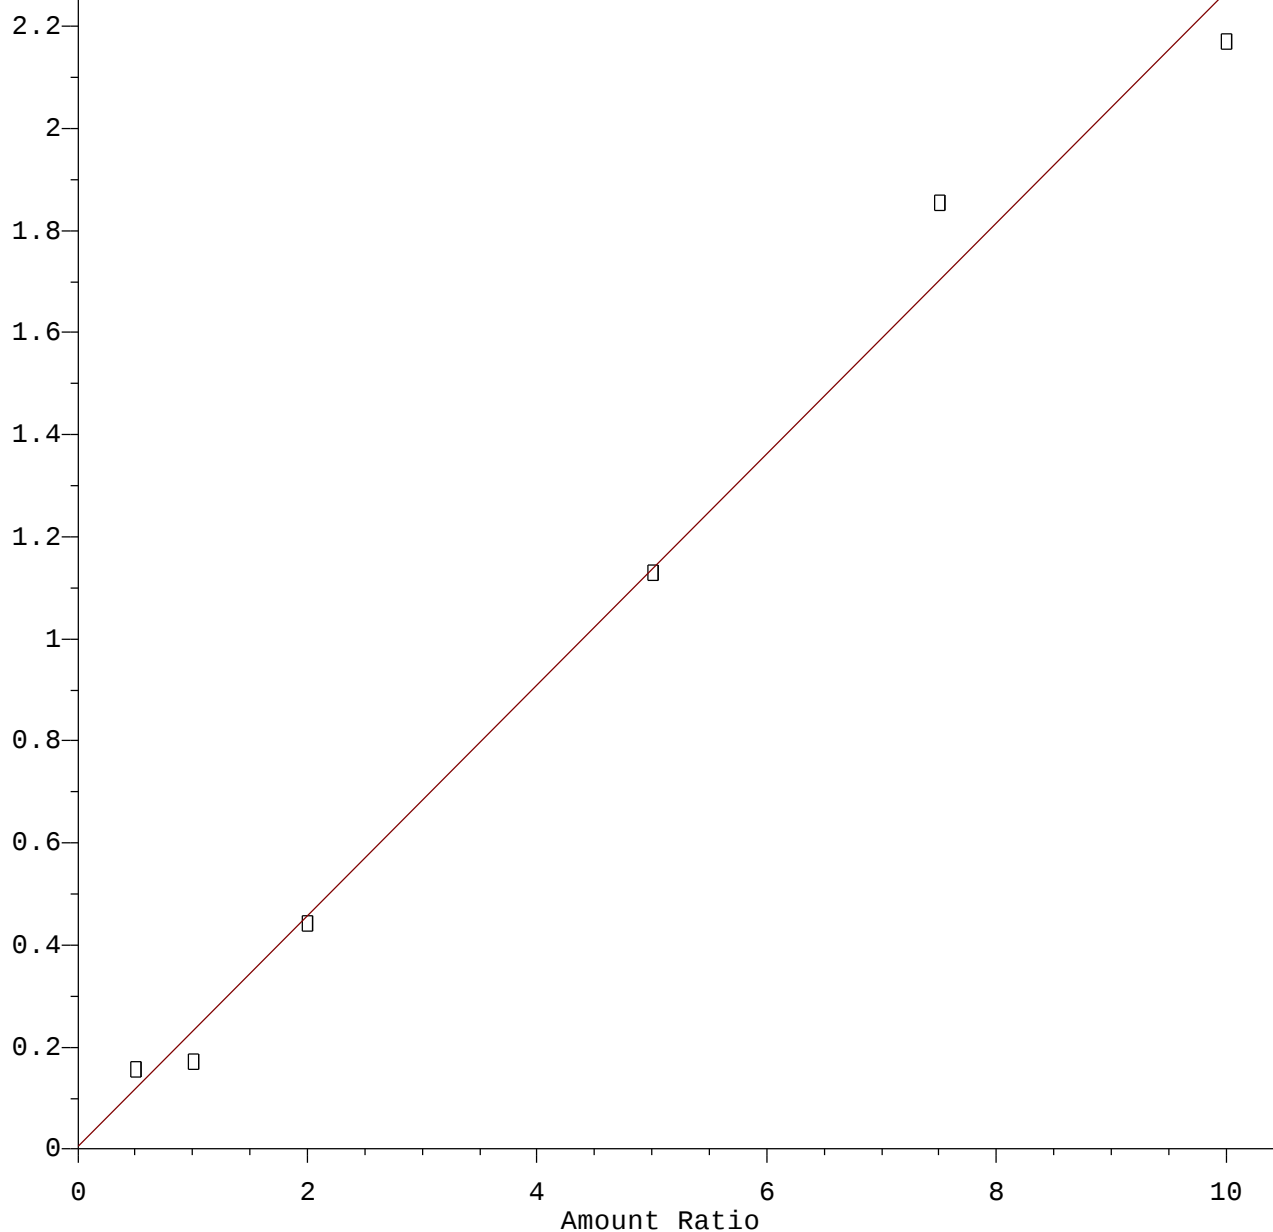


Resp Ratio = $2.26 \times 10^{-1} \times \text{Amt} + 5.34 \times 10^{-3}$
Coef of Det (r^2) = 0.990 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

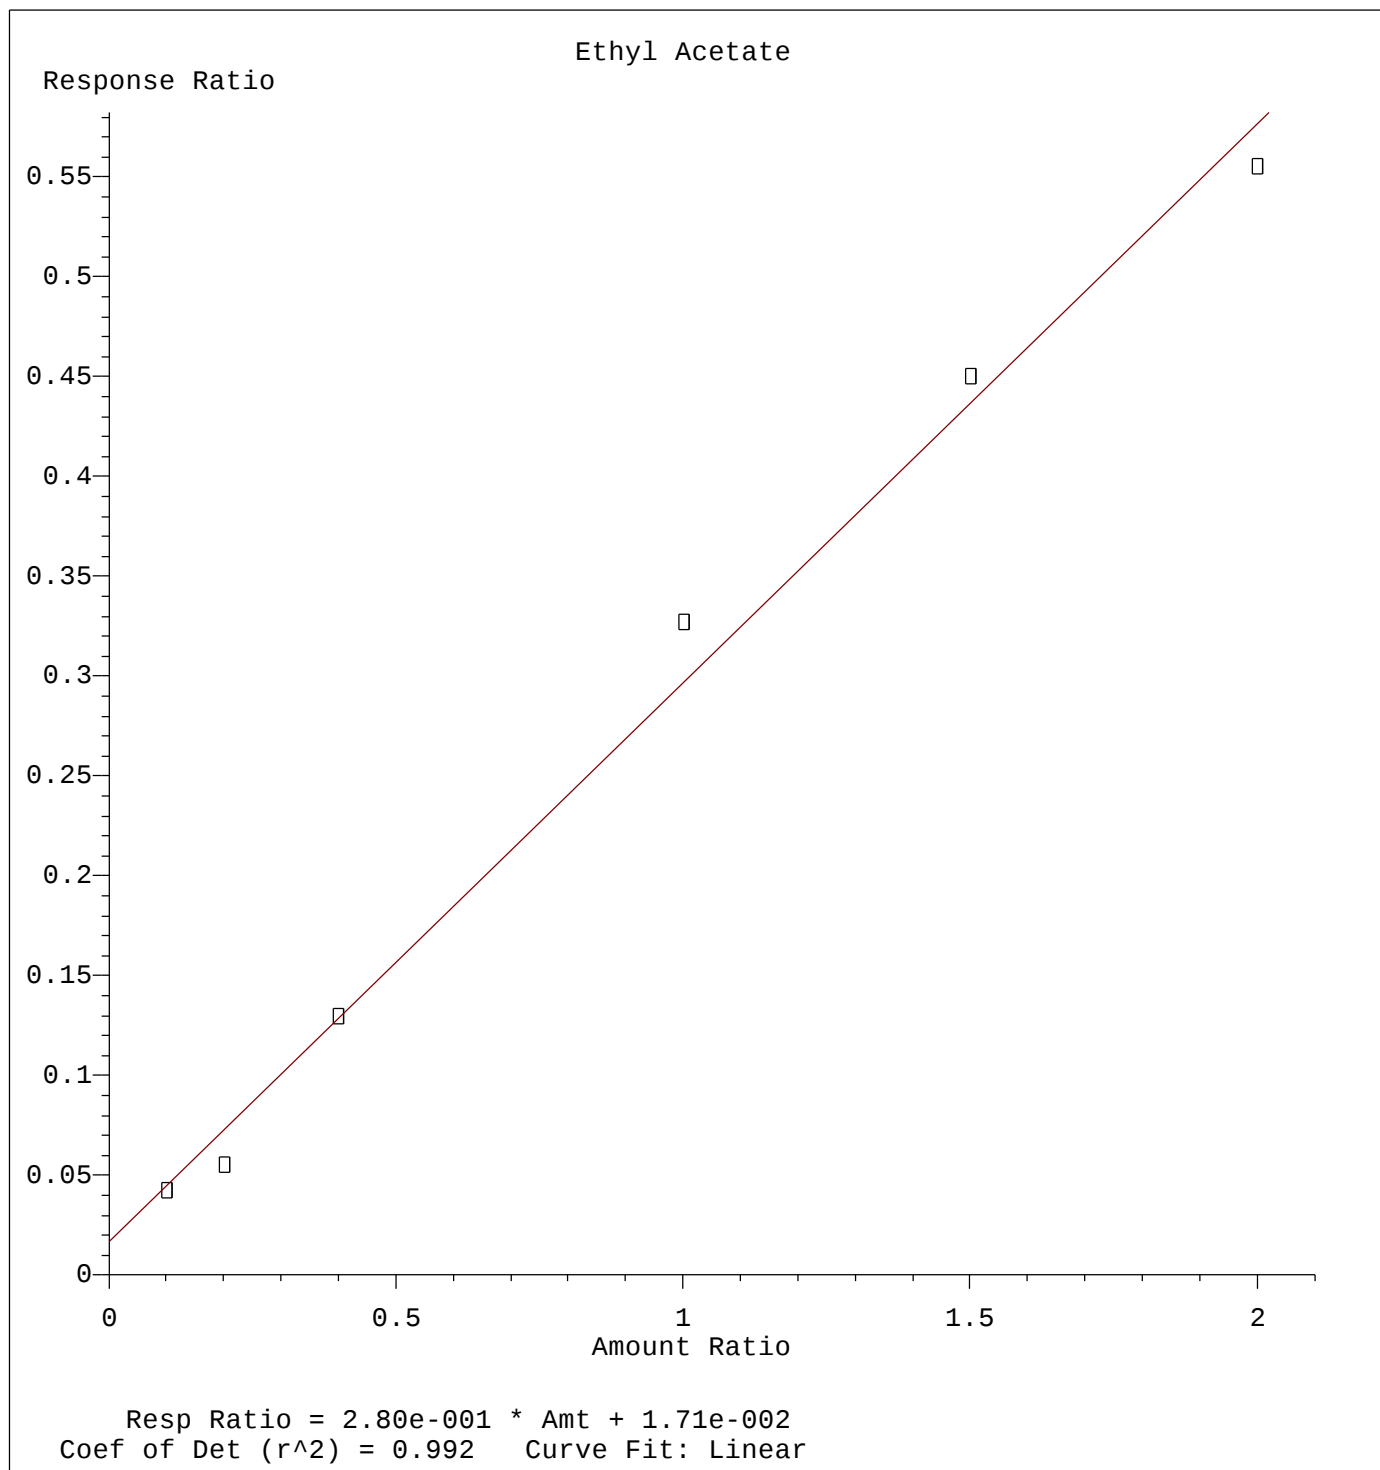


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

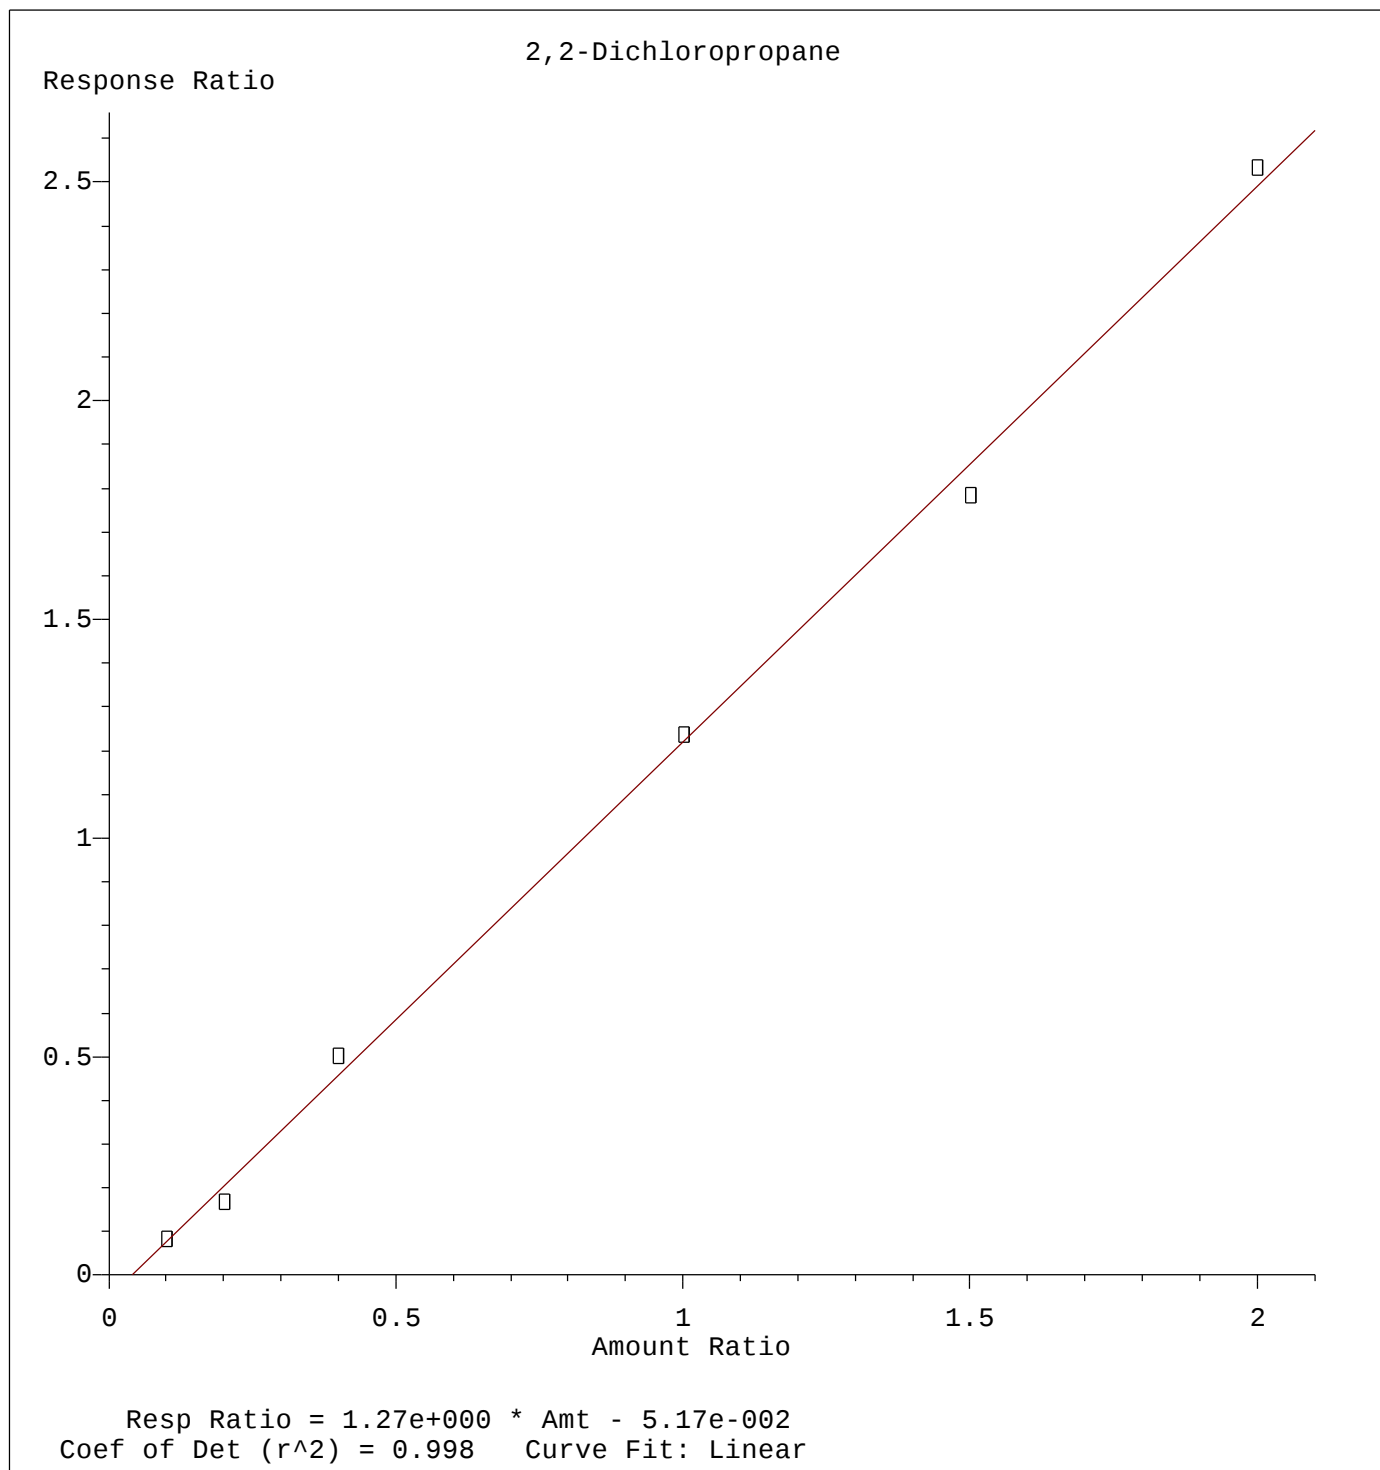


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

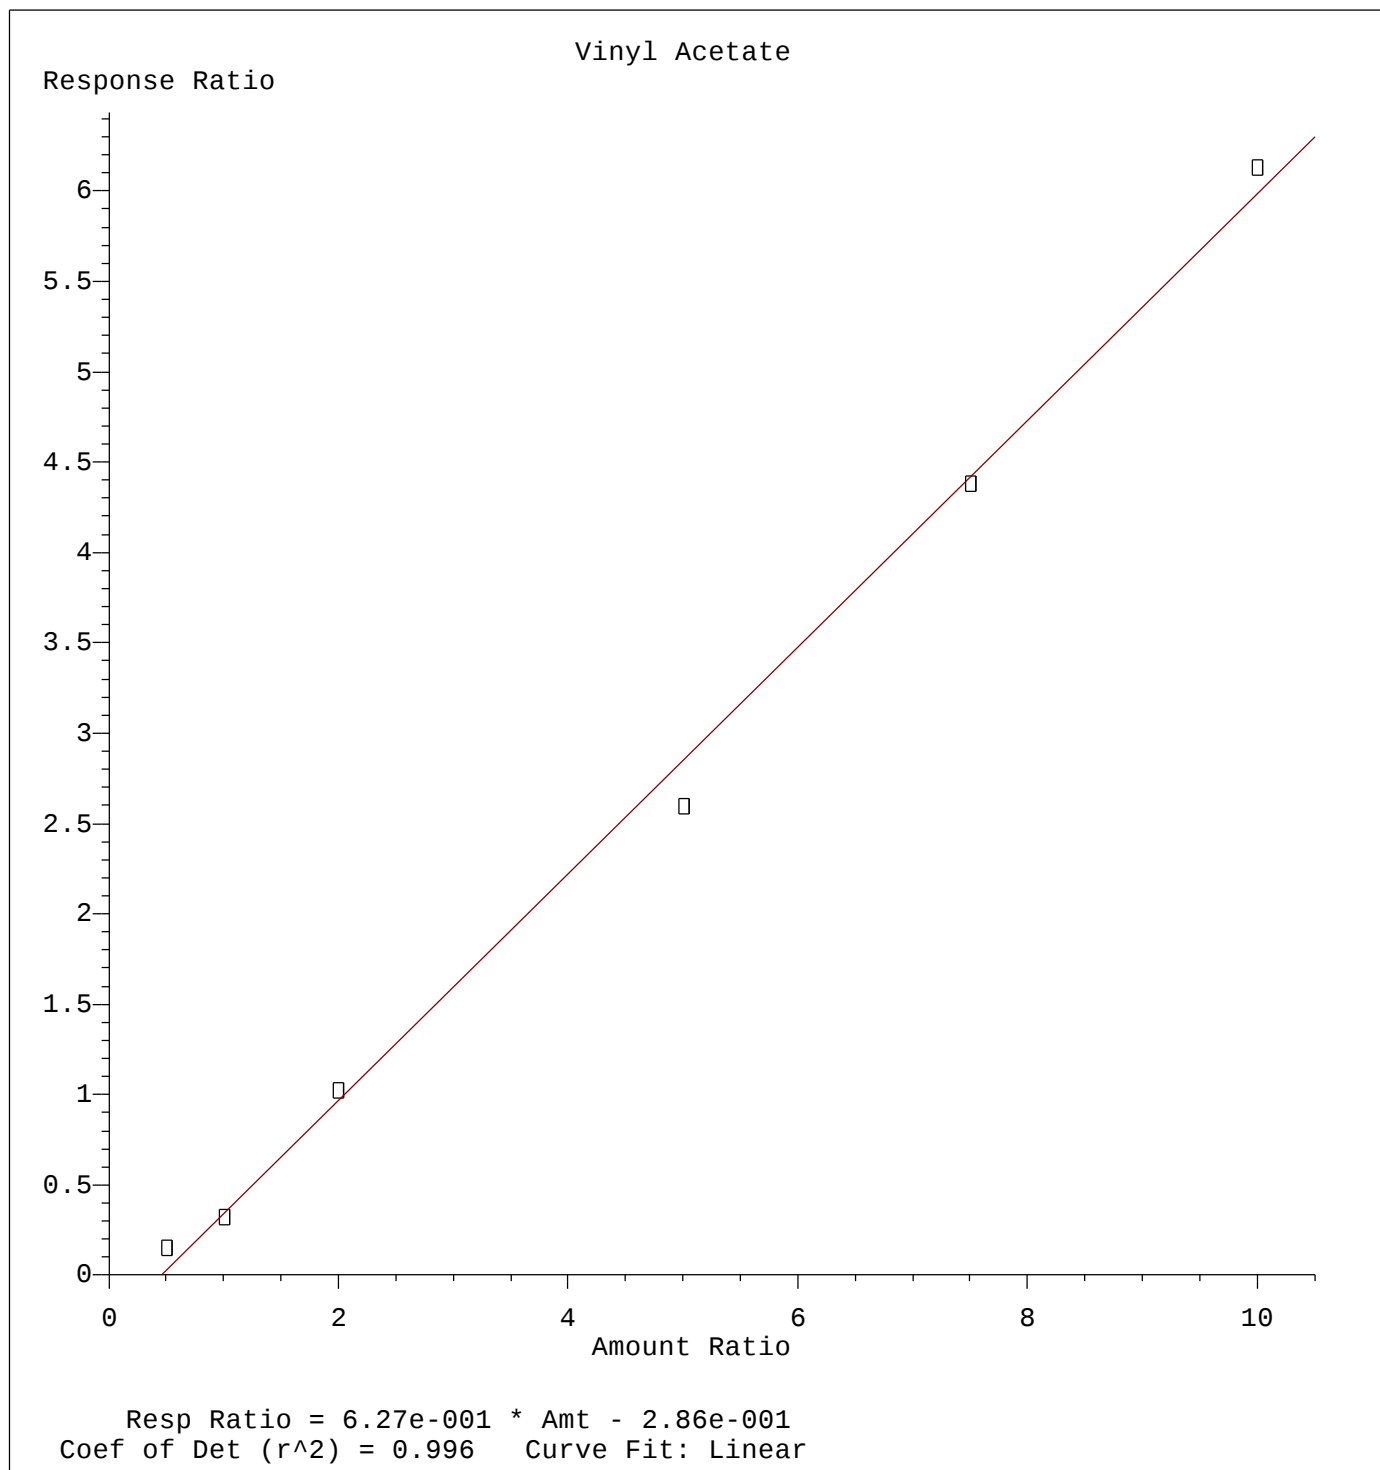


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

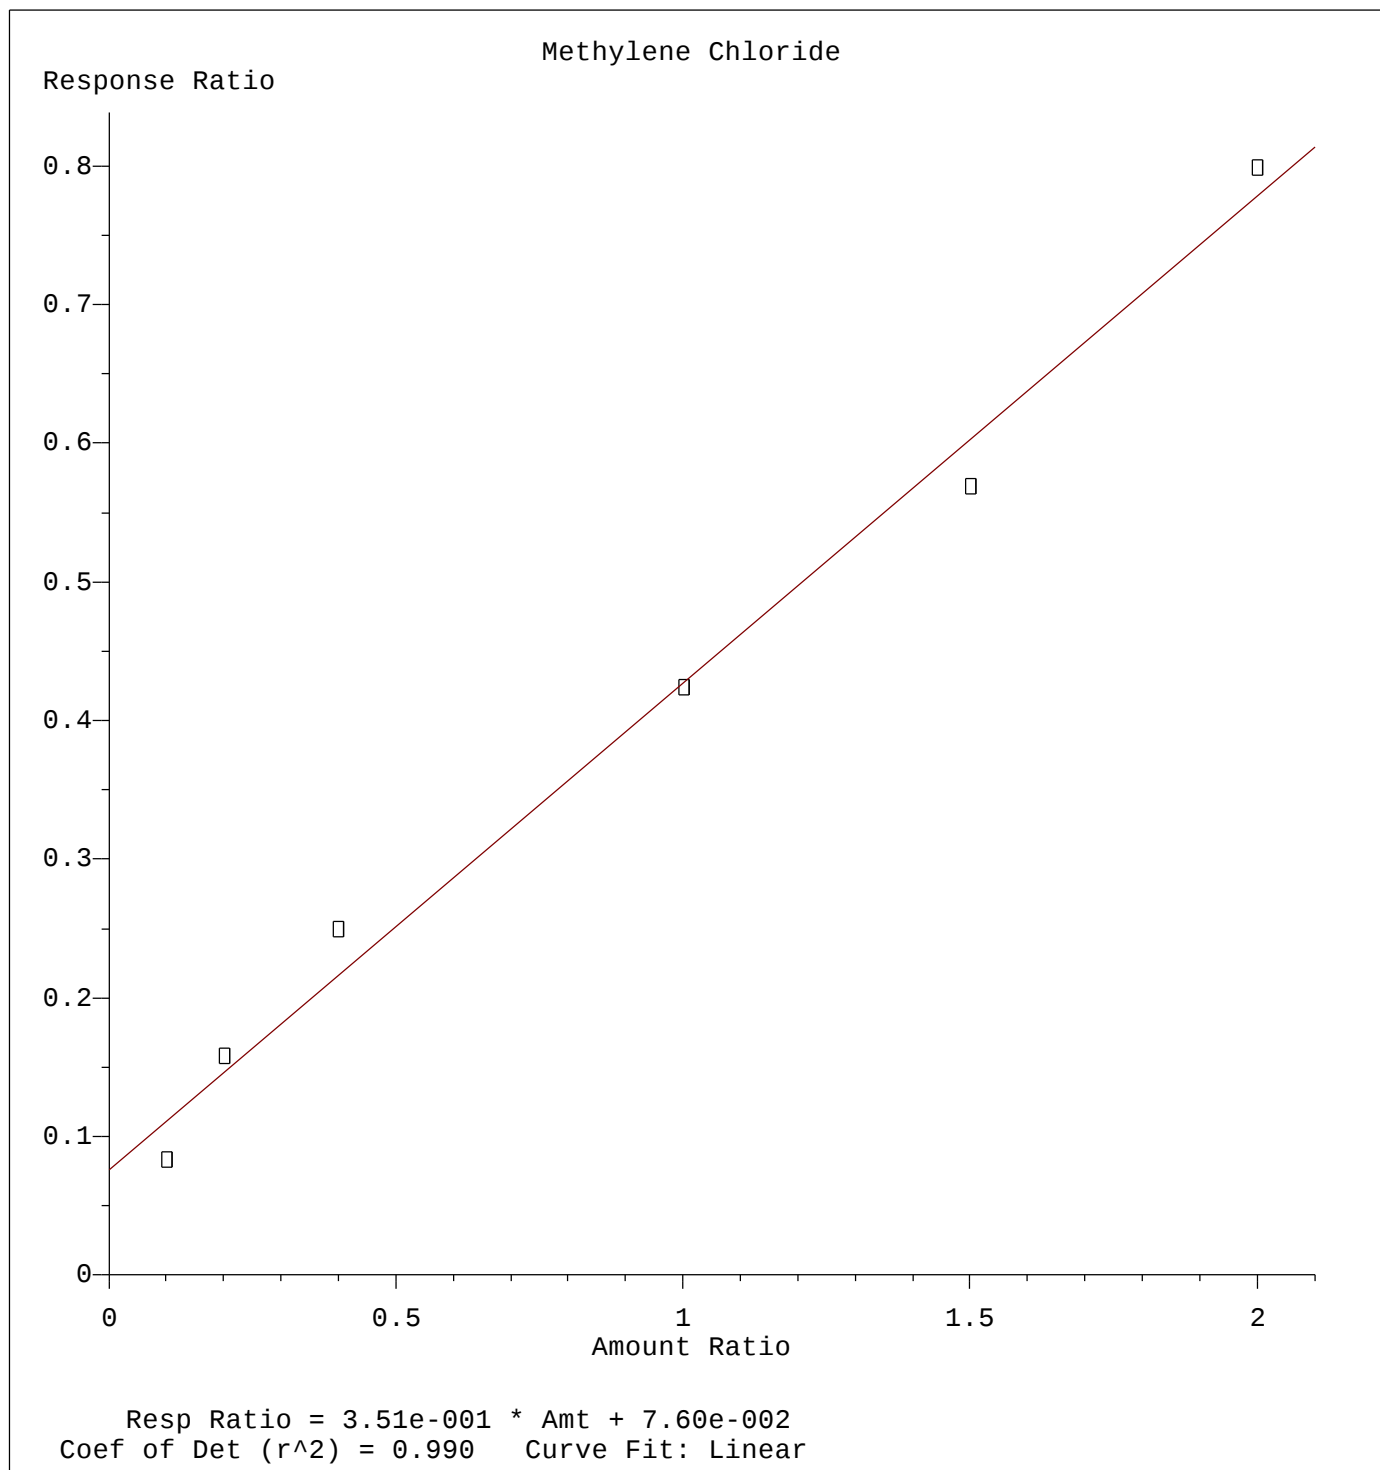

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

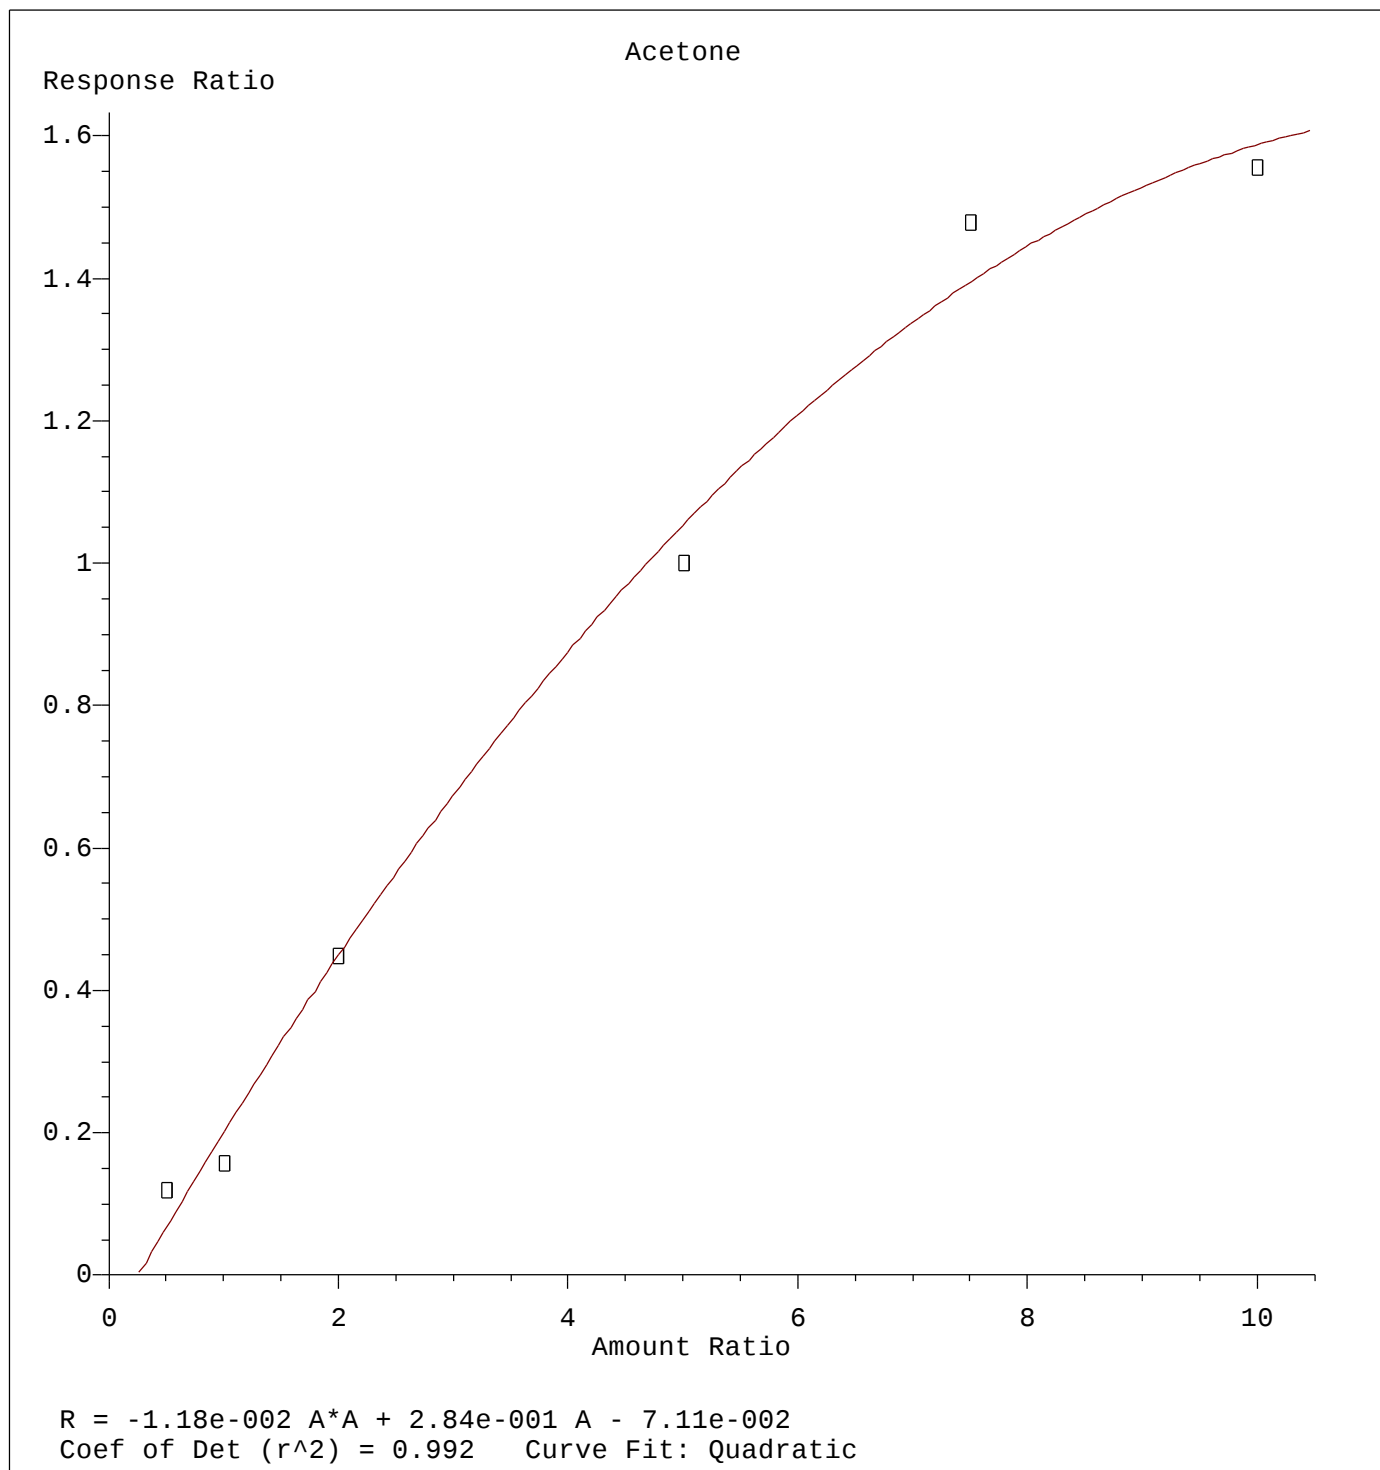

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018

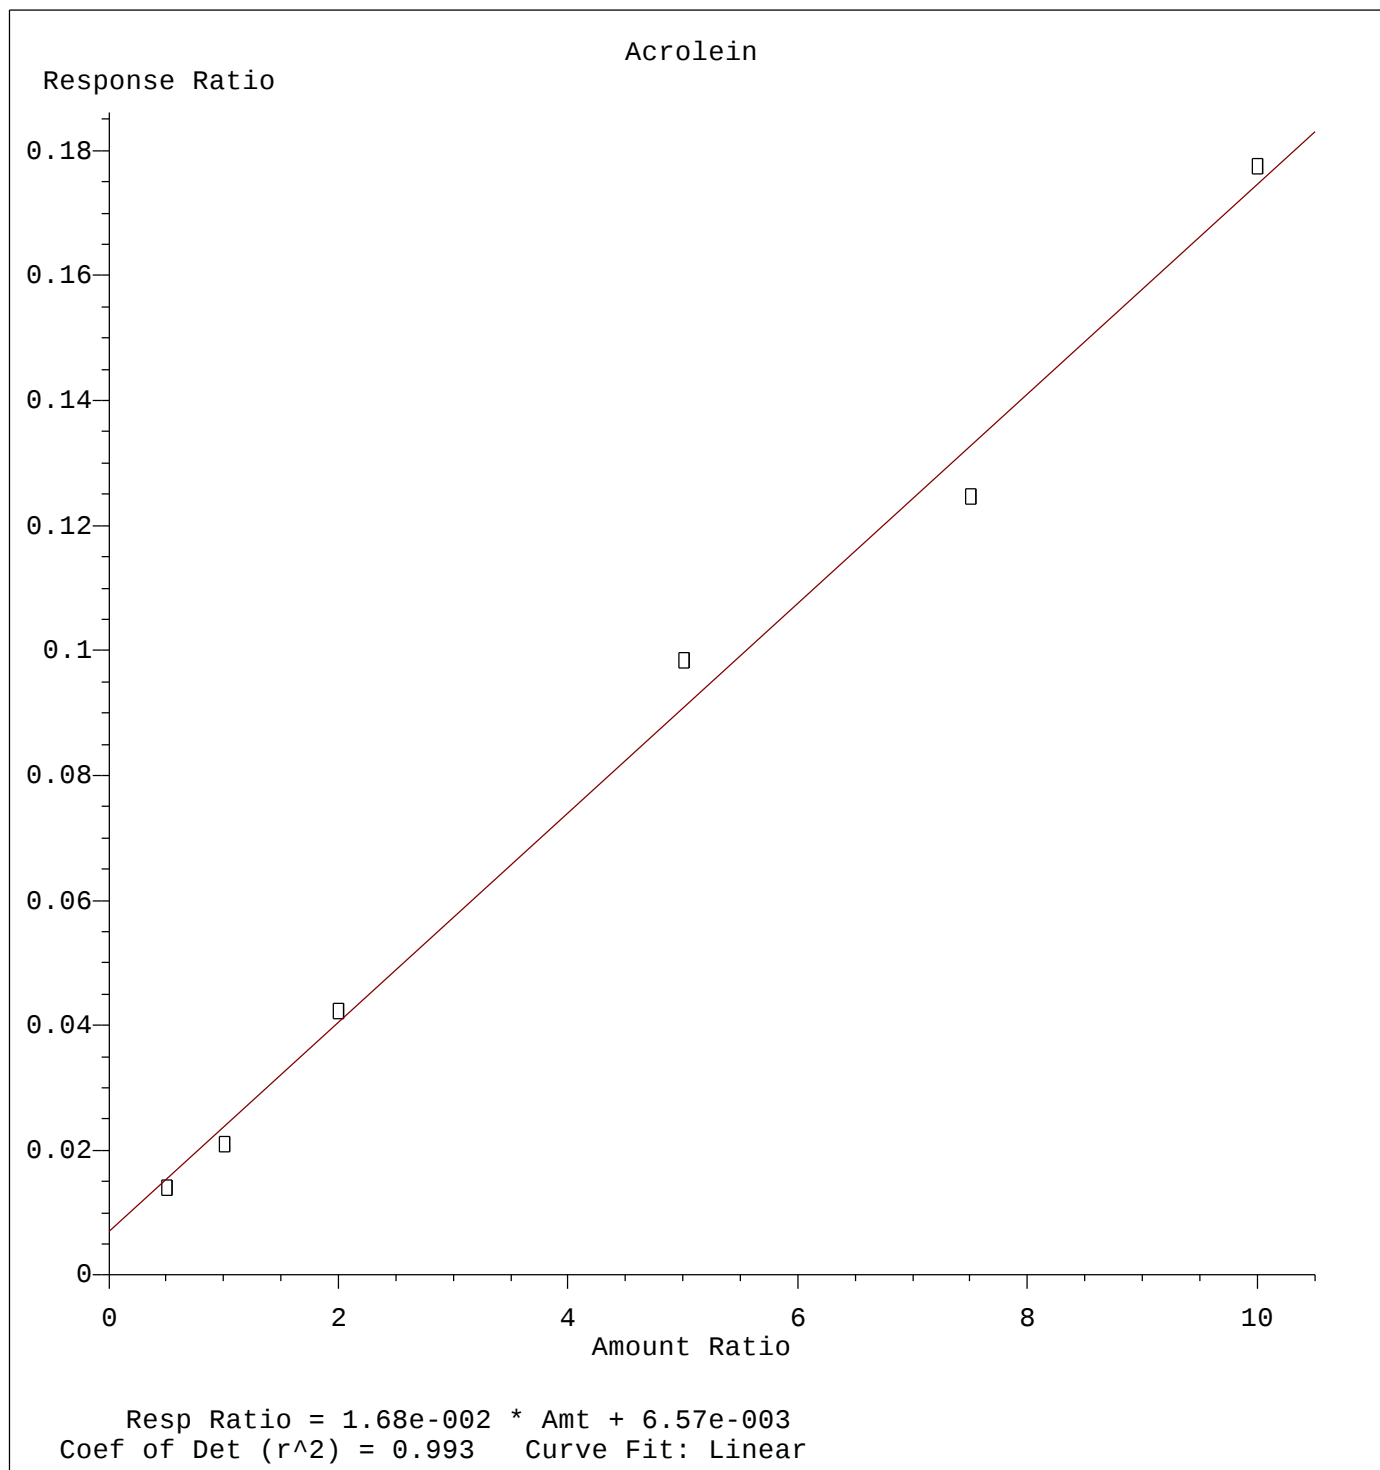

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Calibration Table Last Updated: Fri Sep 07 10:44:05 2018