


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF090618\
Data File : VF060196.D
Acq On : 6 Sep 2018 10:25
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Title : SW846 8260
Last Update : Fri Sep 07 10:44:05 2018

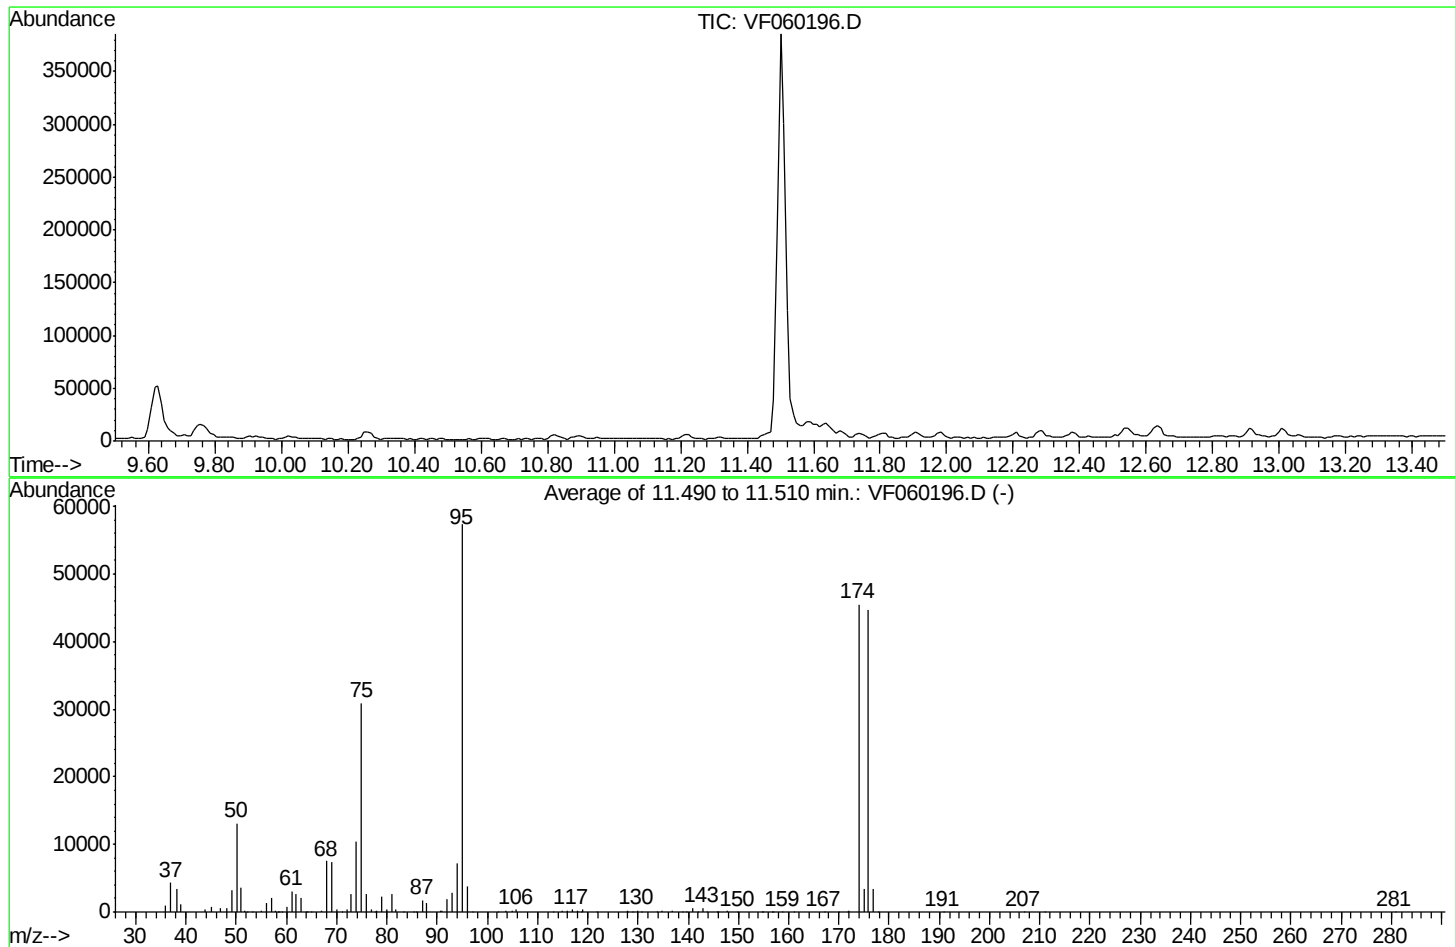

AutoFind: Scans 1061, 1062, 1063; Background Corrected with Scan 1056

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	13143	PASS
75	95	30	60	53.8	30864	PASS
95	95	100	100	100.0	57338	PASS
96	95	5	9	6.6	3804	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.3	45466	PASS
175	174	5	9	7.6	3469	PASS
176	174	95	101	98.1	44600	PASS
177	176	5	9	7.8	3474	PASS