


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF090718\
 Data File : VF060205.D
 Acq On : 7 Sep 2018 9:58
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
 Title : SW846 8260
 Last Update : Fri Sep 07 10:44:05 2018

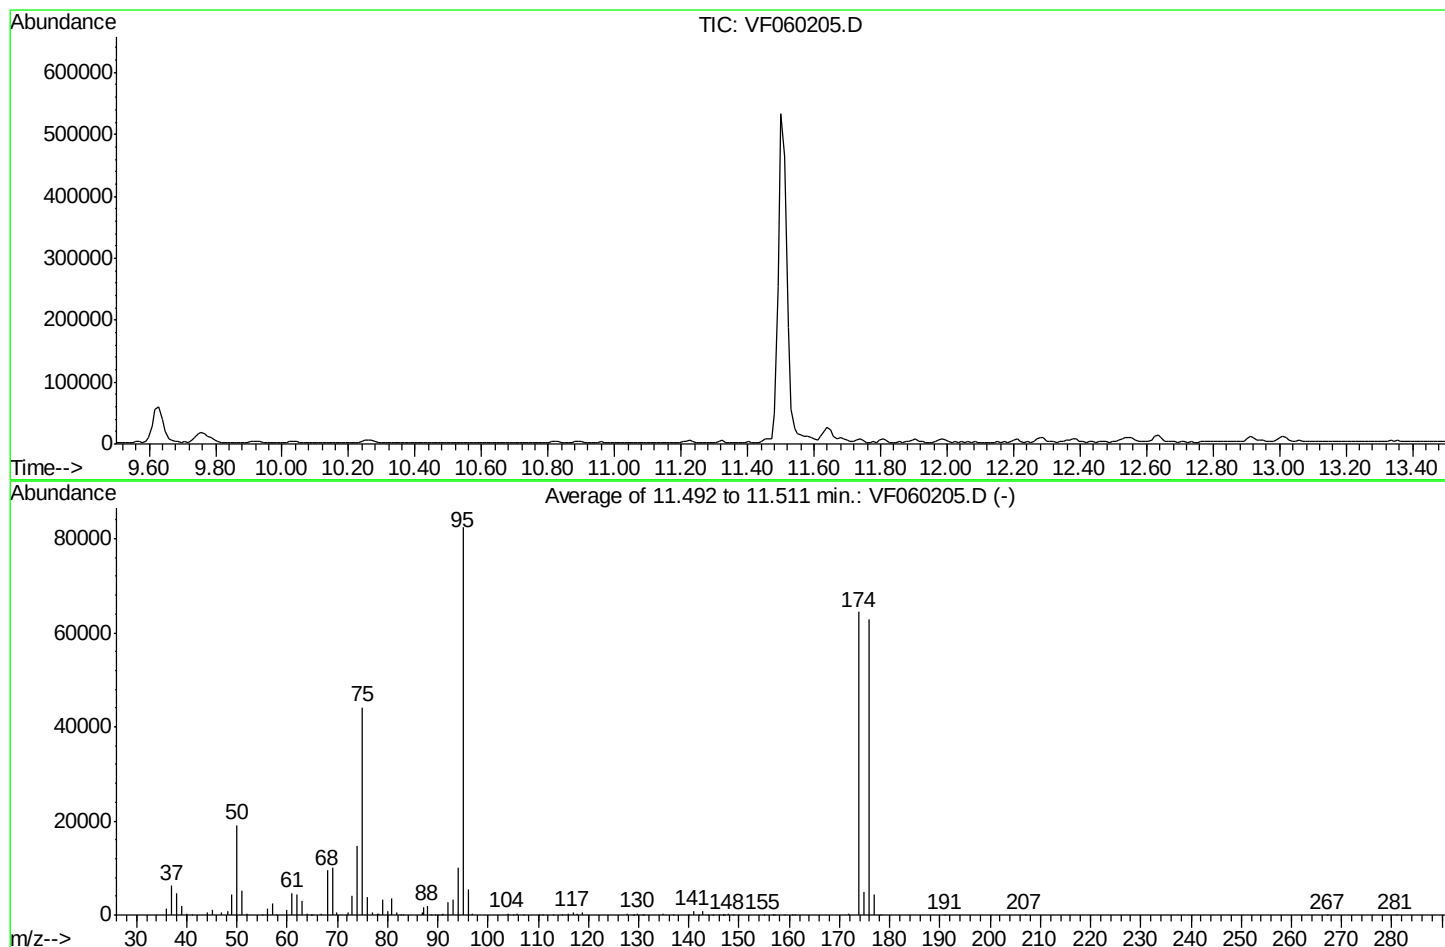

AutoFind: Scans 1102, 1103, 1104; Background Corrected with Scan 1097

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	19107	PASS
75	95	30	60	53.6	44152	PASS
95	95	100	100	100.0	82413	PASS
96	95	5	9	6.7	5516	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.2	64488	PASS
175	174	5	9	7.7	4977	PASS
176	174	95	101	97.6	62965	PASS
177	176	5	9	6.8	4294	PASS