


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF091018\
Data File : VF060225.D
Acq On : 10 Sep 2018 9:41
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F090618S.M
Title : SW846 8260
Last Update : Fri Sep 07 10:44:05 2018

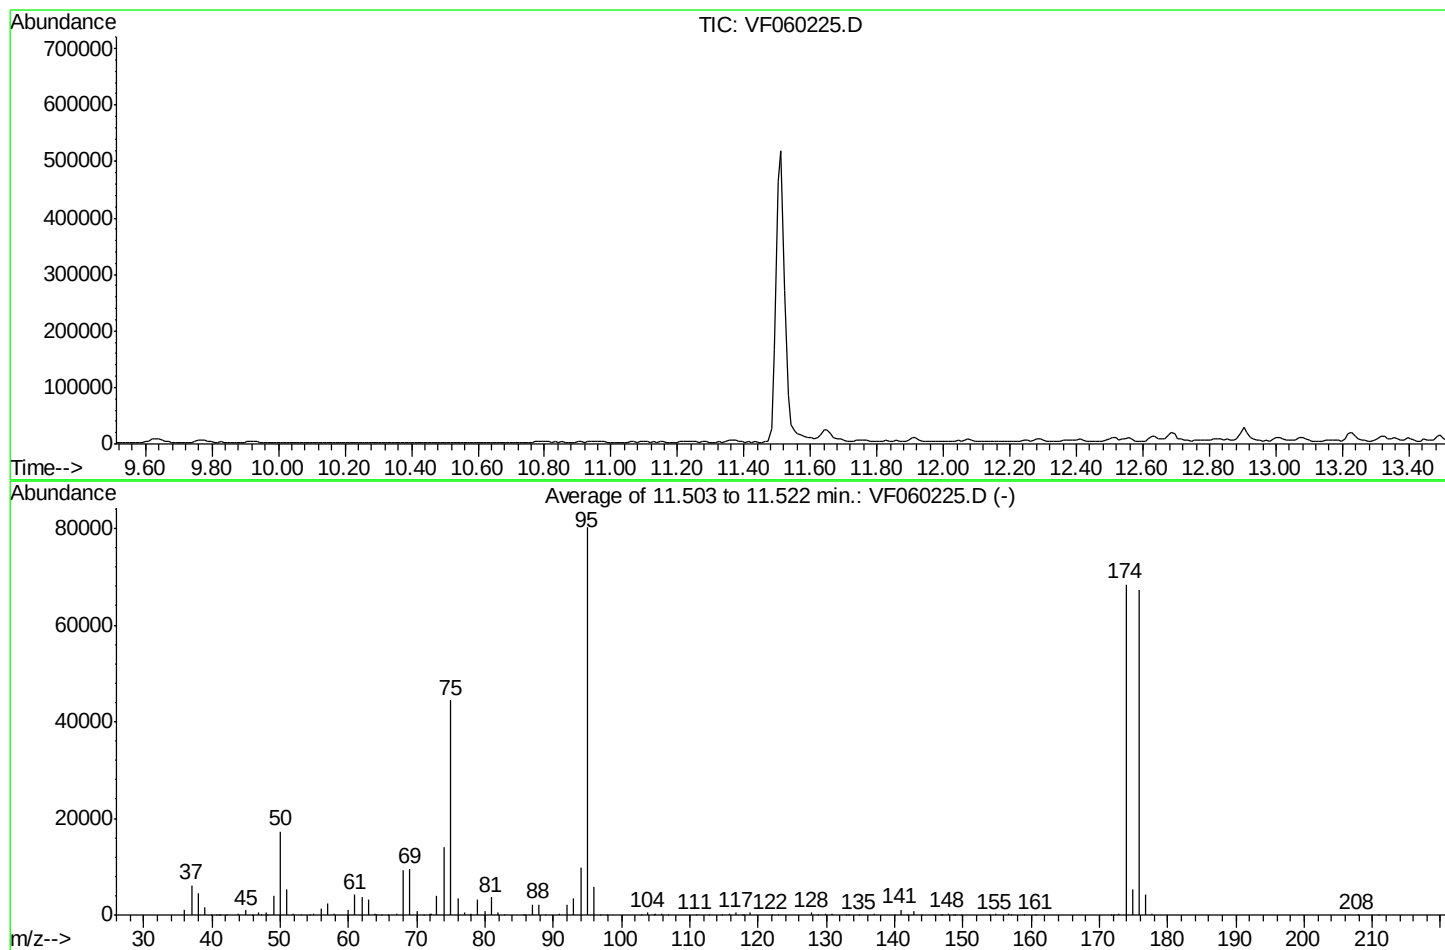

AutoFind: Scans 1103, 1104, 1105; Background Corrected with Scan 1097

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	17254	PASS
75	95	30	60	55.3	44402	PASS
95	95	100	100	100.0	80250	PASS
96	95	5	9	7.2	5776	PASS
173	174	0.00	2	0.4	252	PASS
174	95	50	100	85.3	68416	PASS
175	174	5	9	7.8	5314	PASS
176	174	95	101	98.2	67182	PASS
177	176	5	9	6.4	4280	PASS