



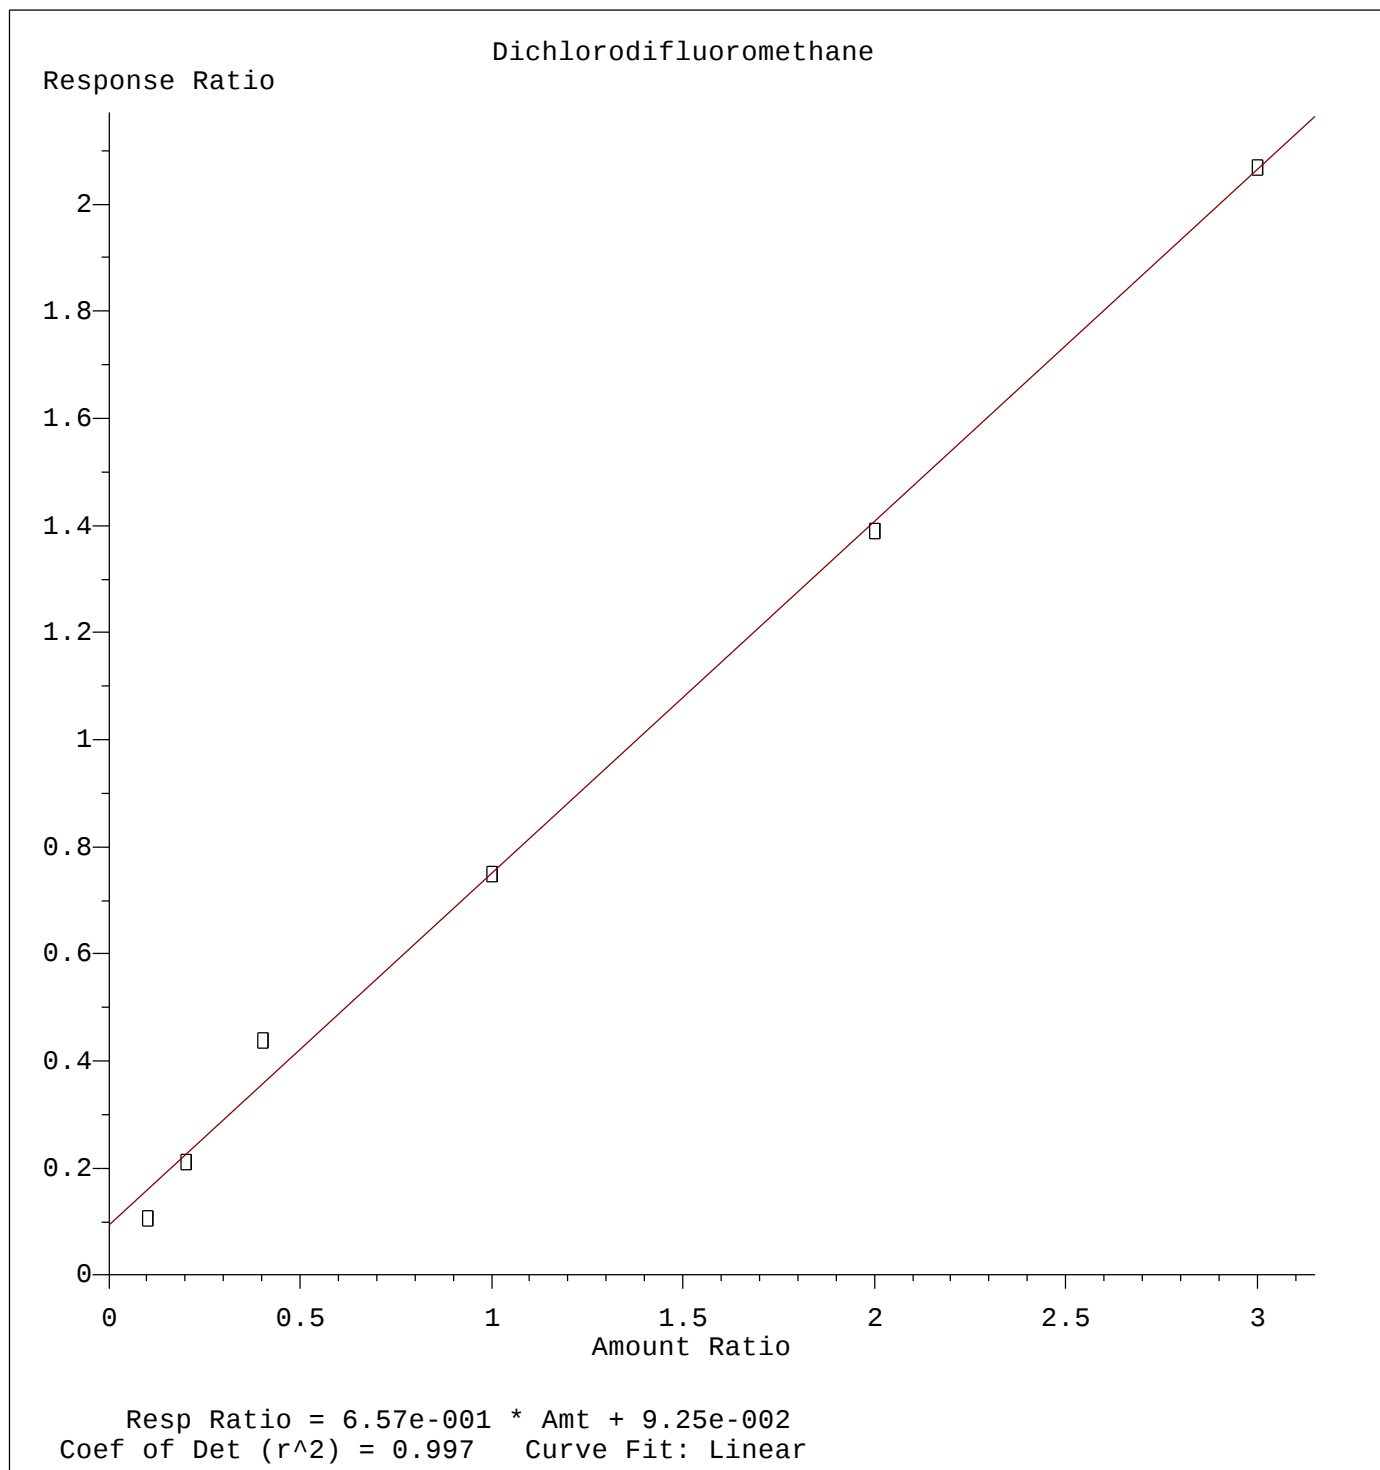


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018

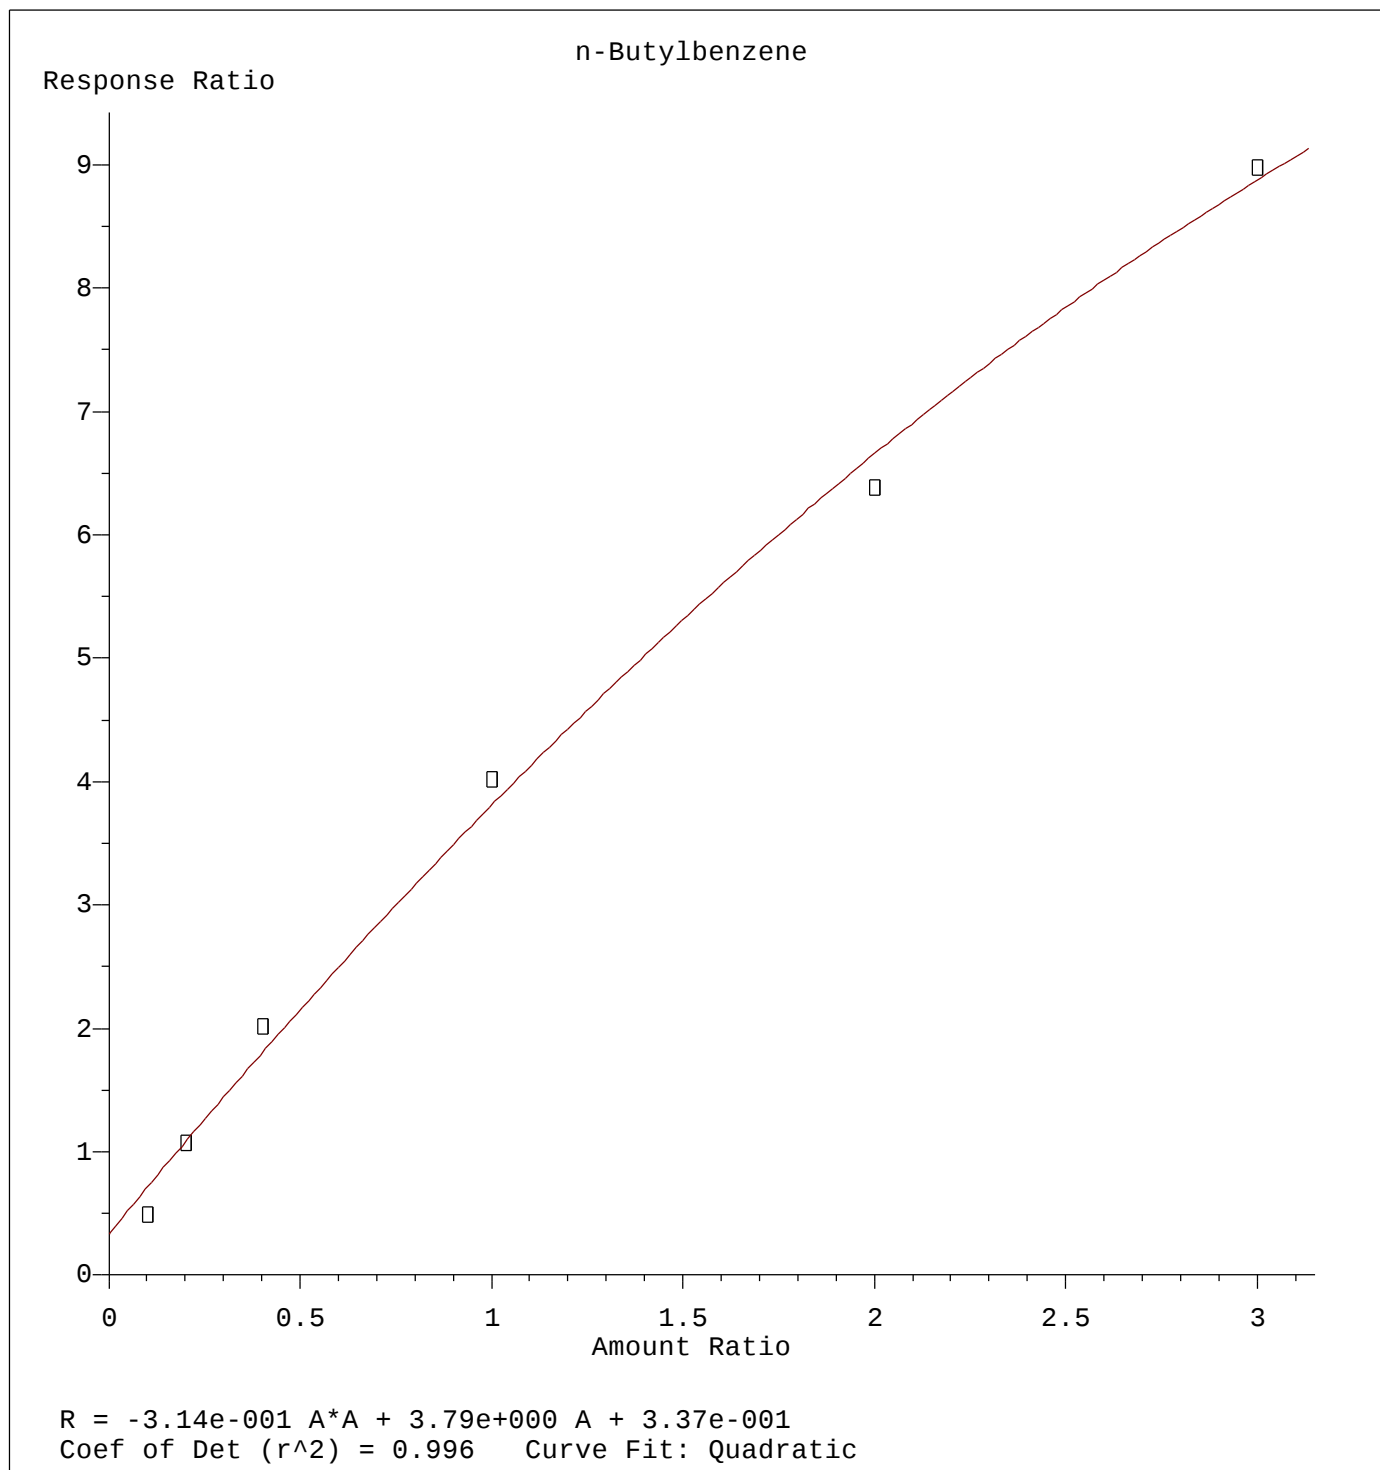

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018

p-Isopropyltoluene

Response Ratio

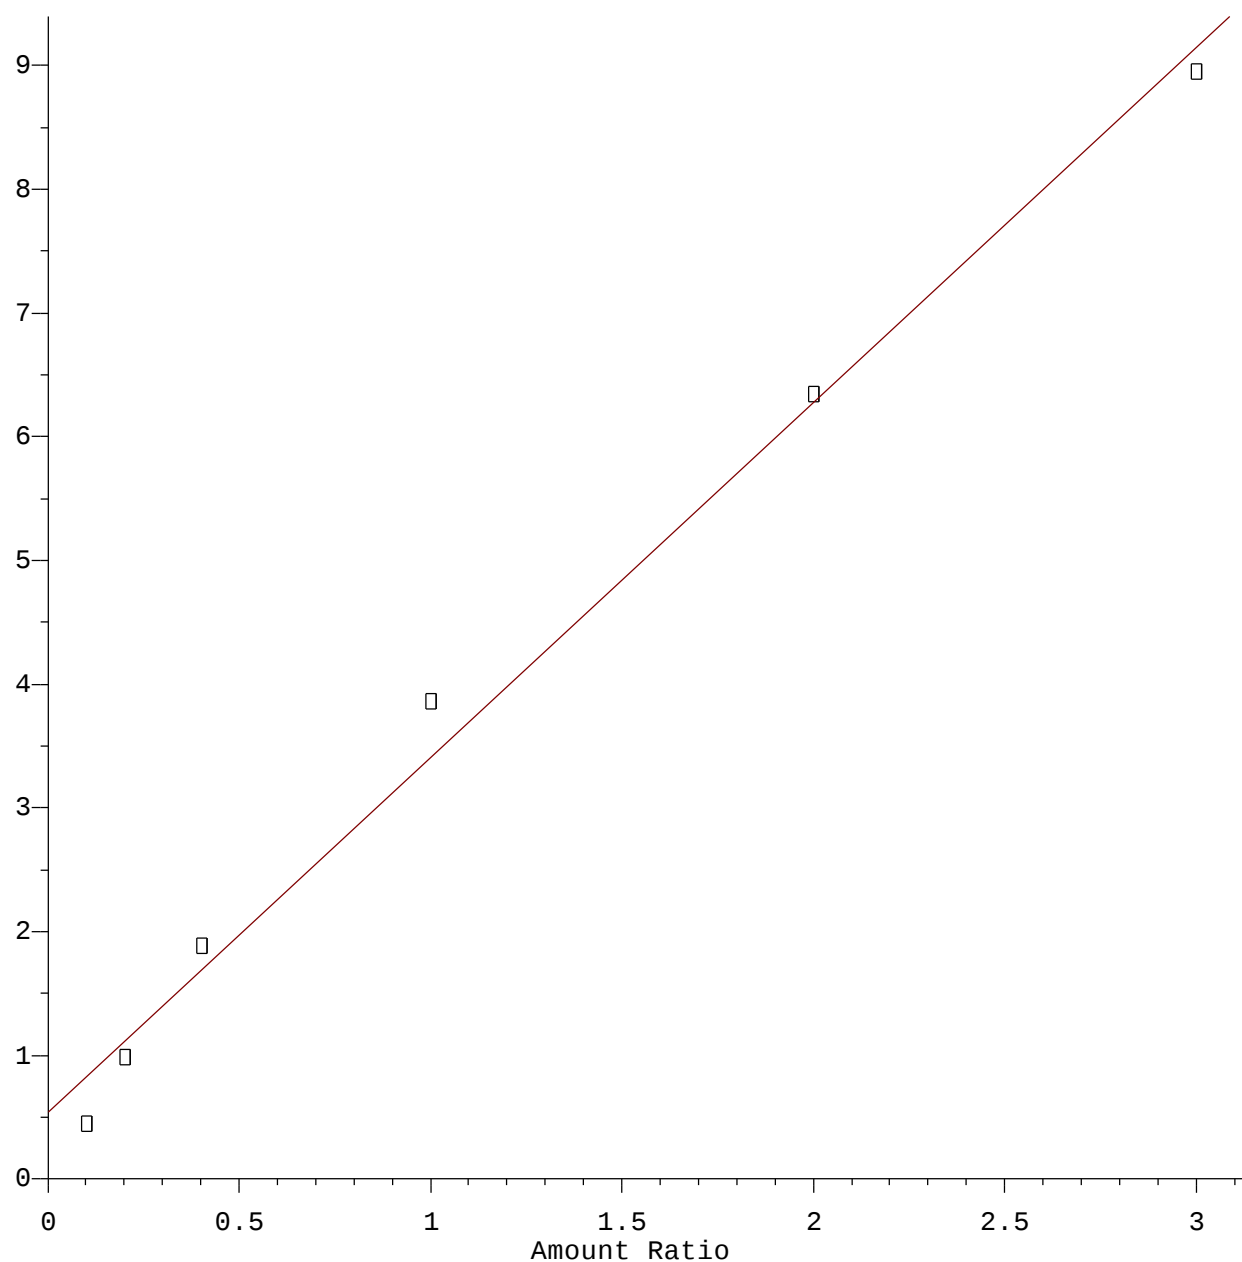


Resp Ratio = 2.87e+000 \* Amt + 5.40e-001  
Coef of Det (r^2) = 0.992    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018


sec-Butylbenzene

Response Ratio

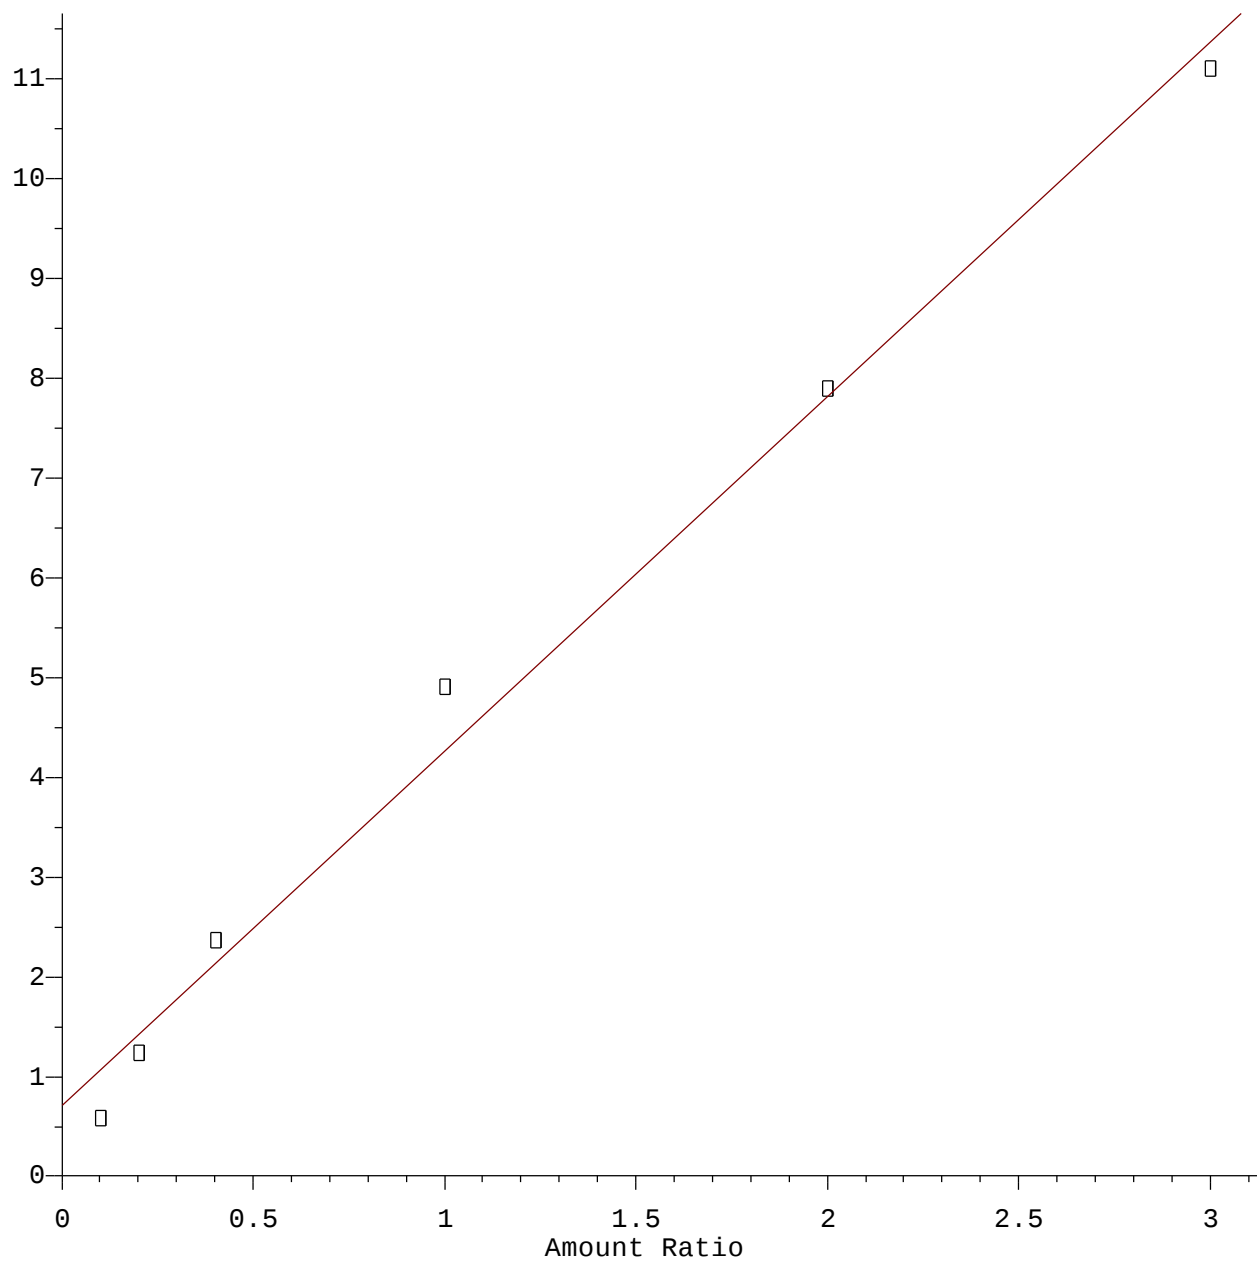

Resp Ratio = 3.55e+000 \* Amt + 7.13e-001  
Coef of Det (r^2) = 0.991 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018

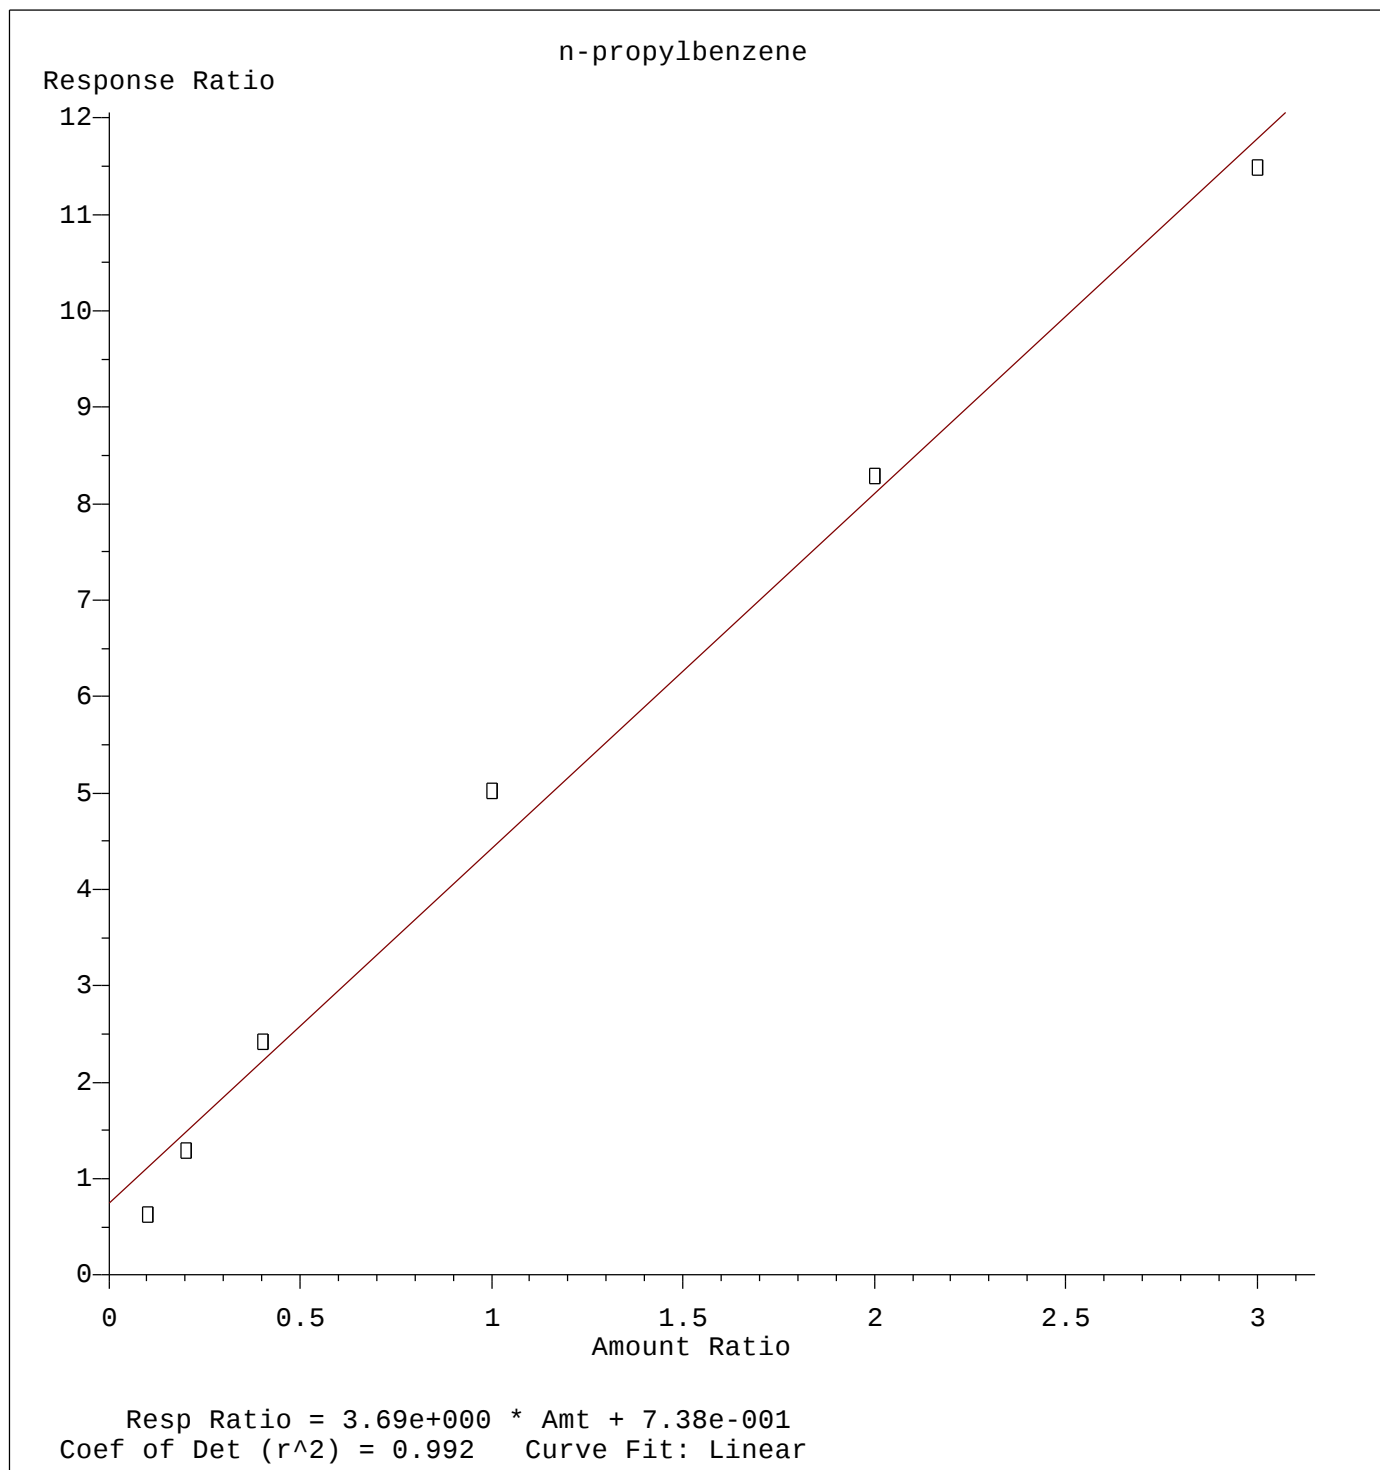

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018


# Methylene Chloride

Response Ratio

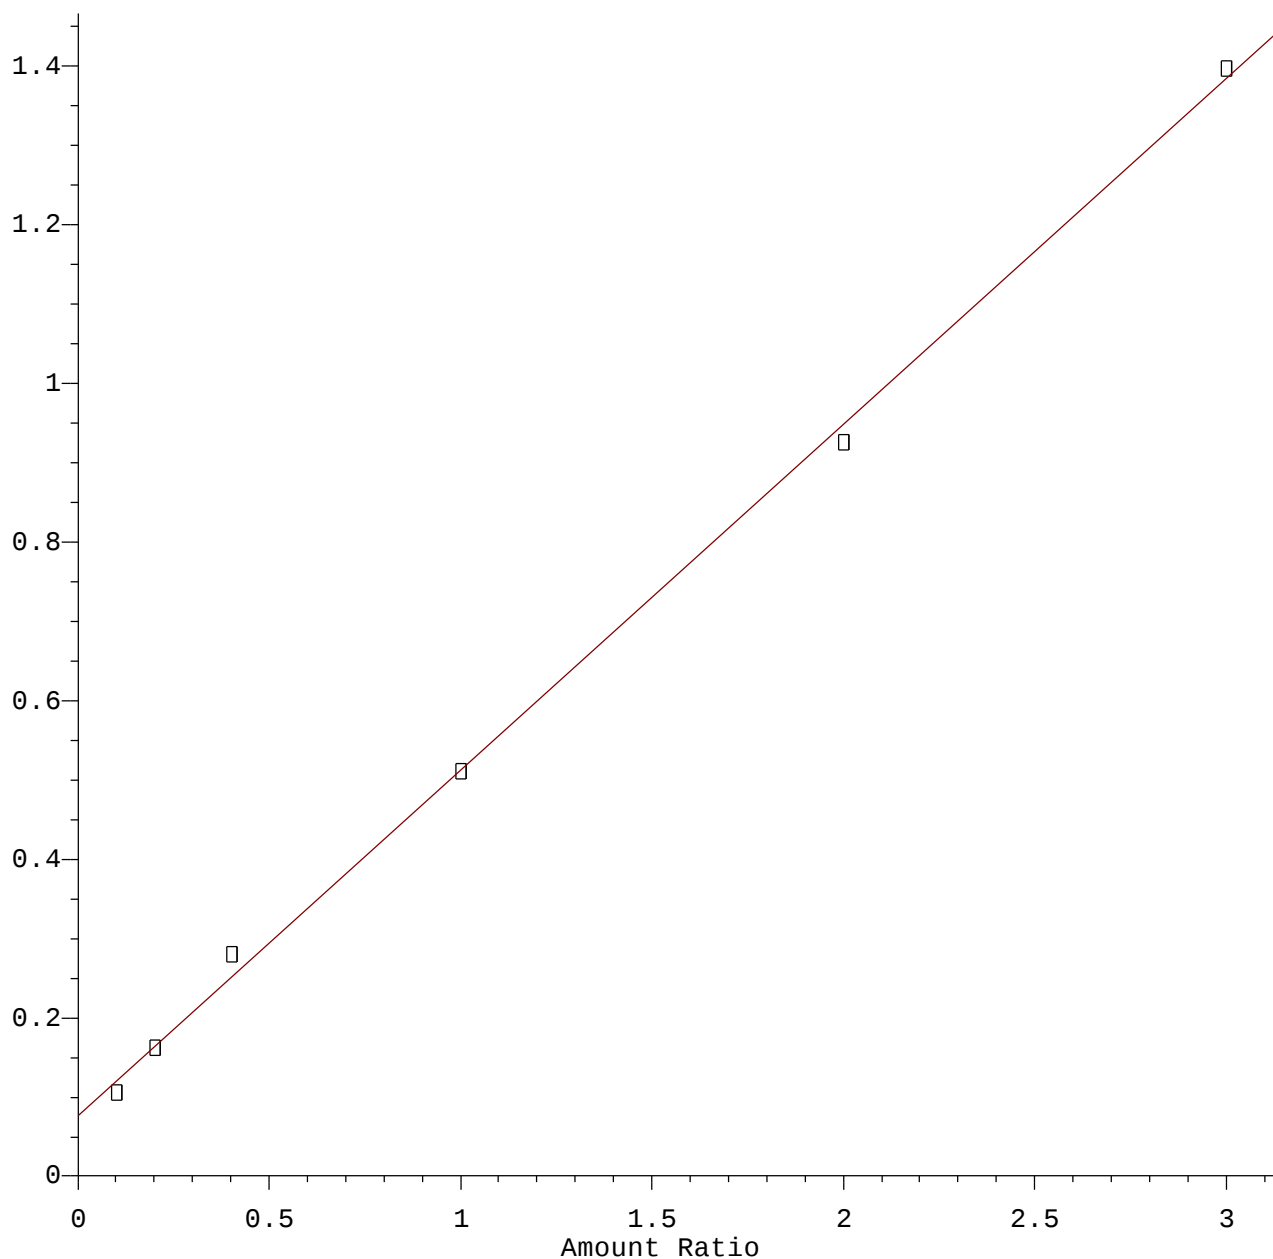


Resp Ratio =  $4.36 \times 10^{-1} \times \text{Amt} + 7.61 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018

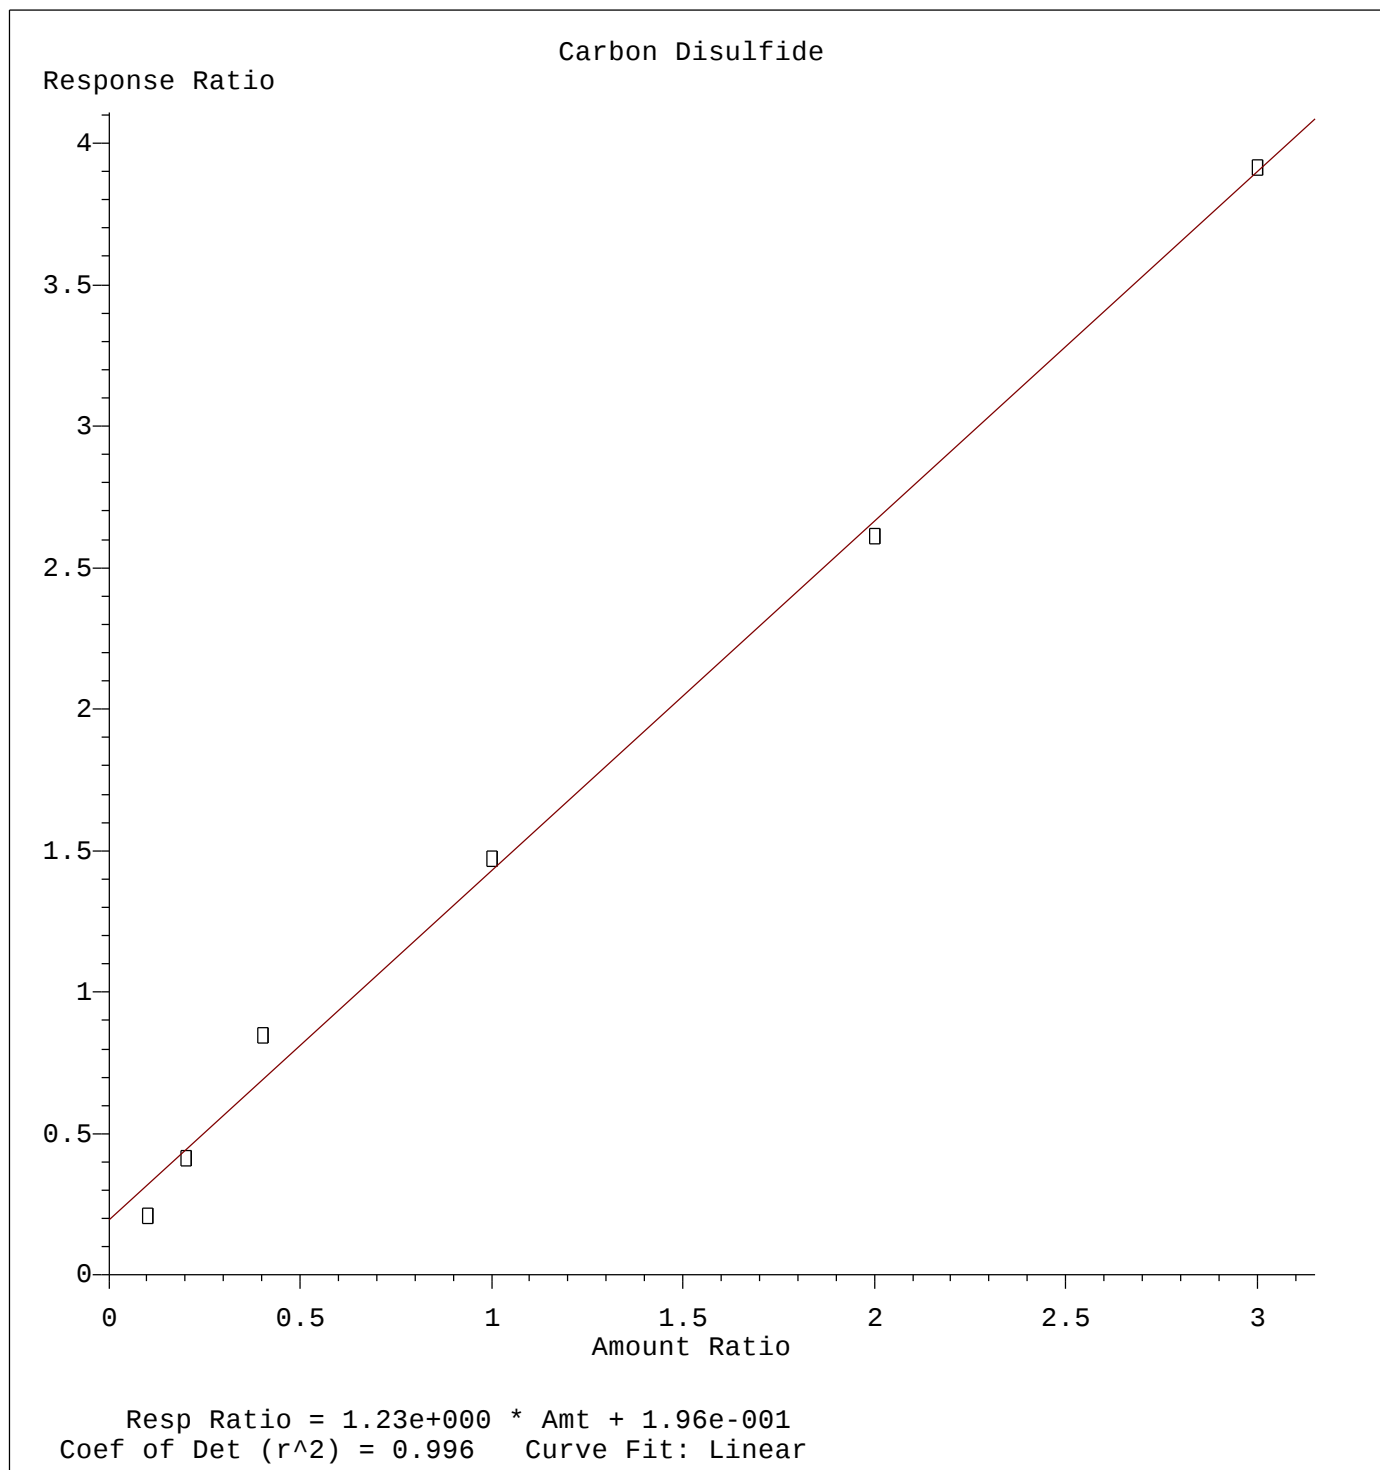


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018

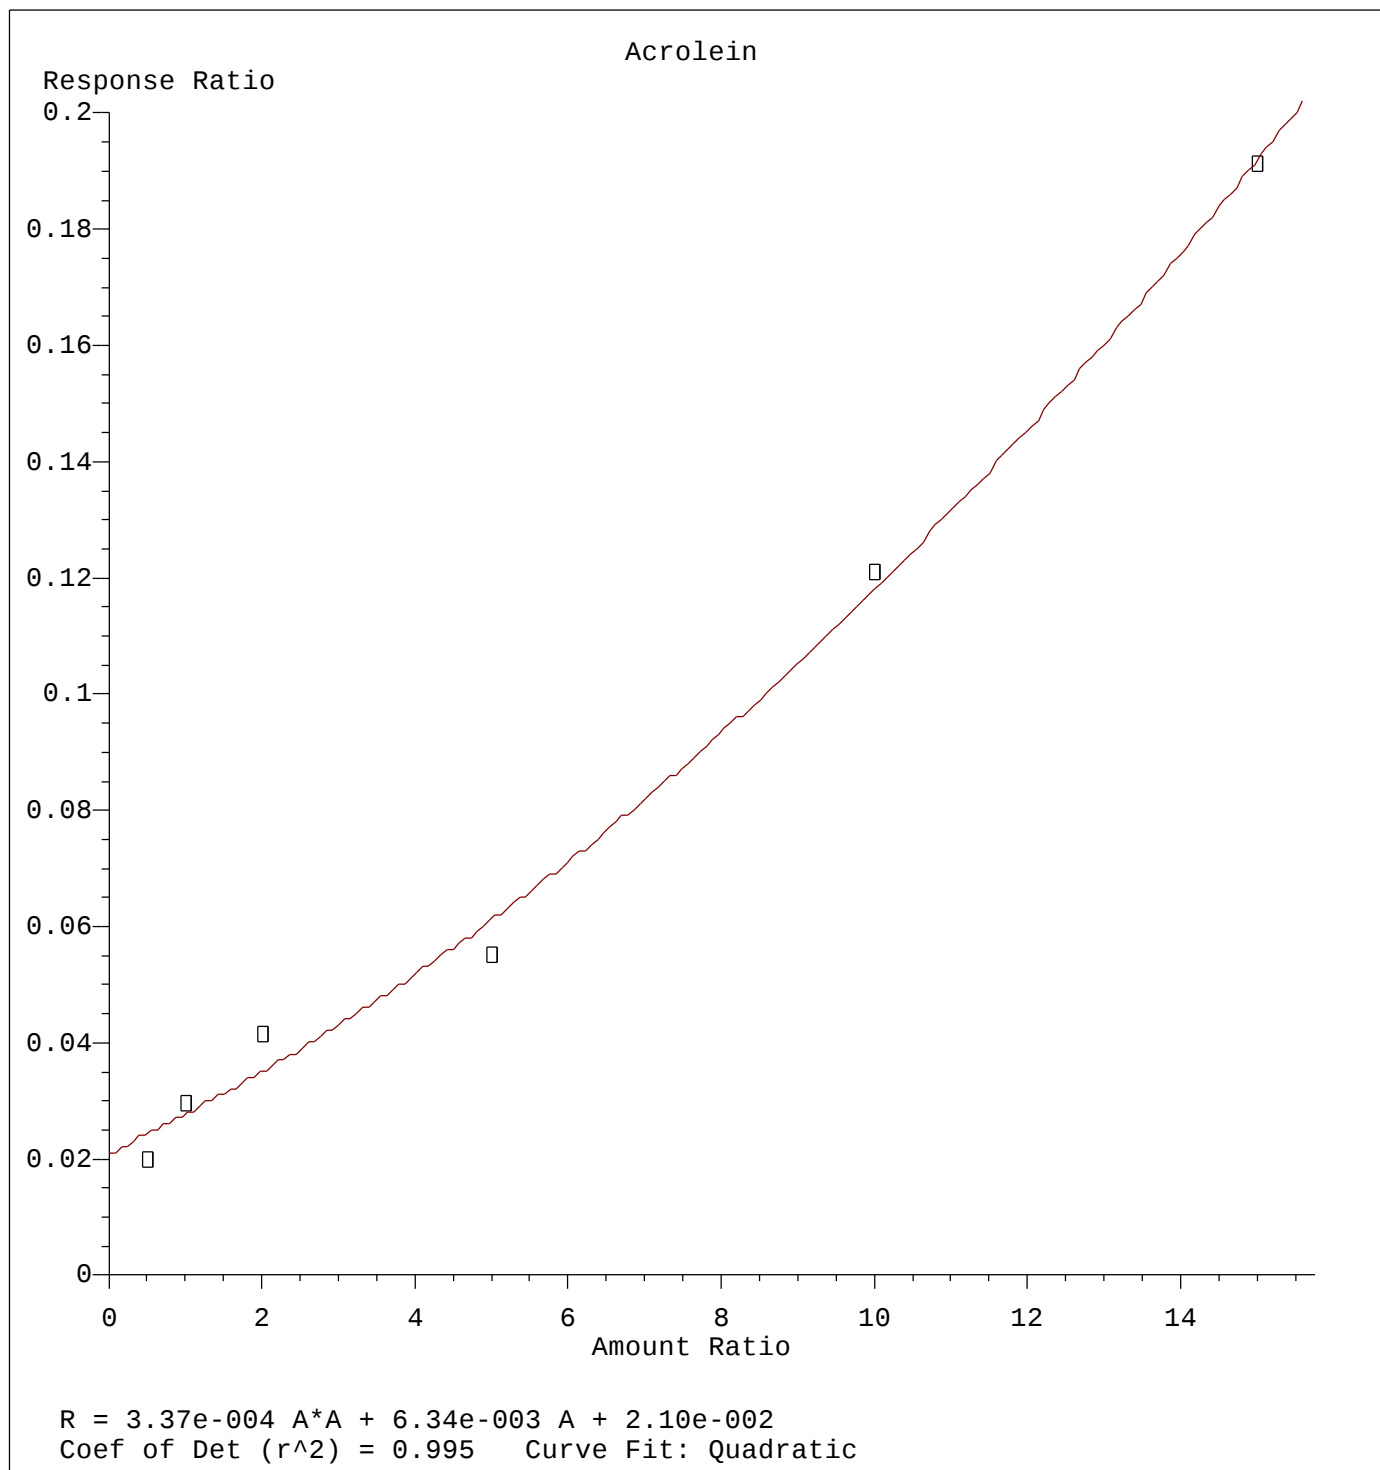

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018

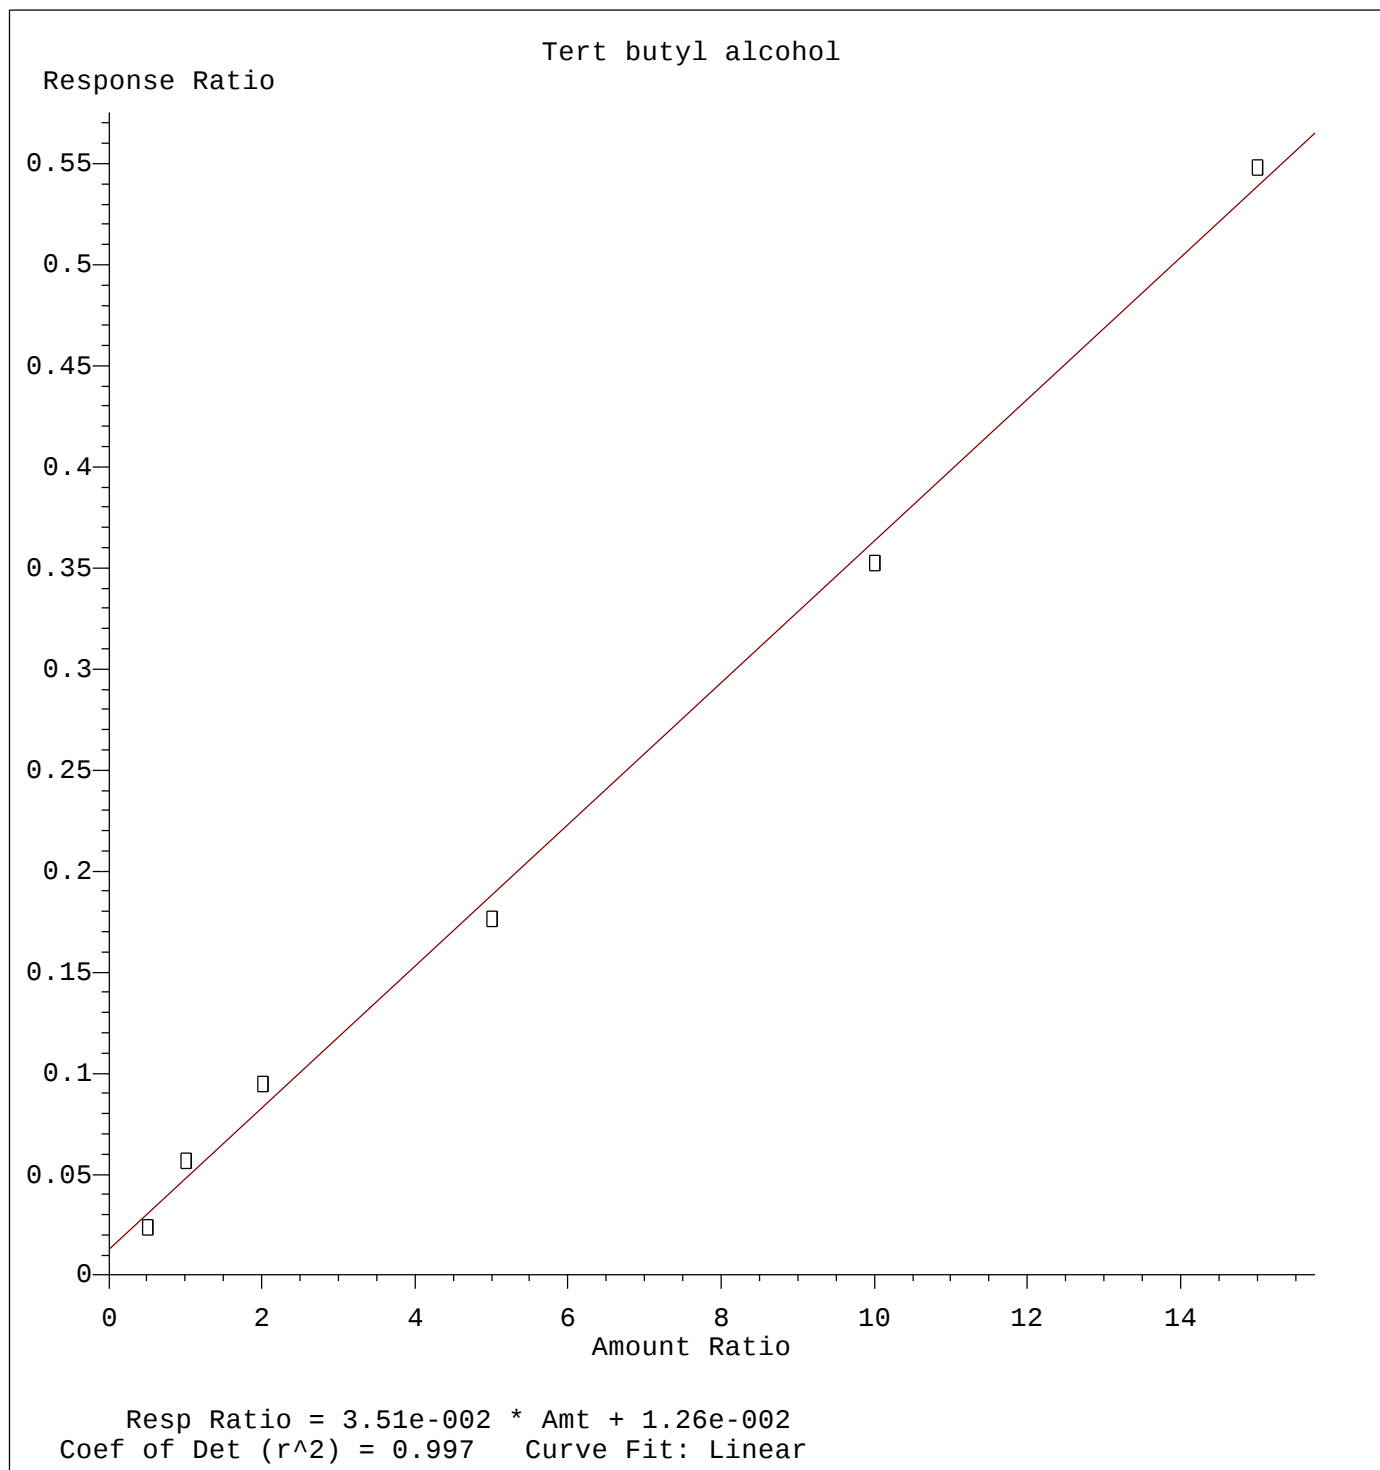

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018

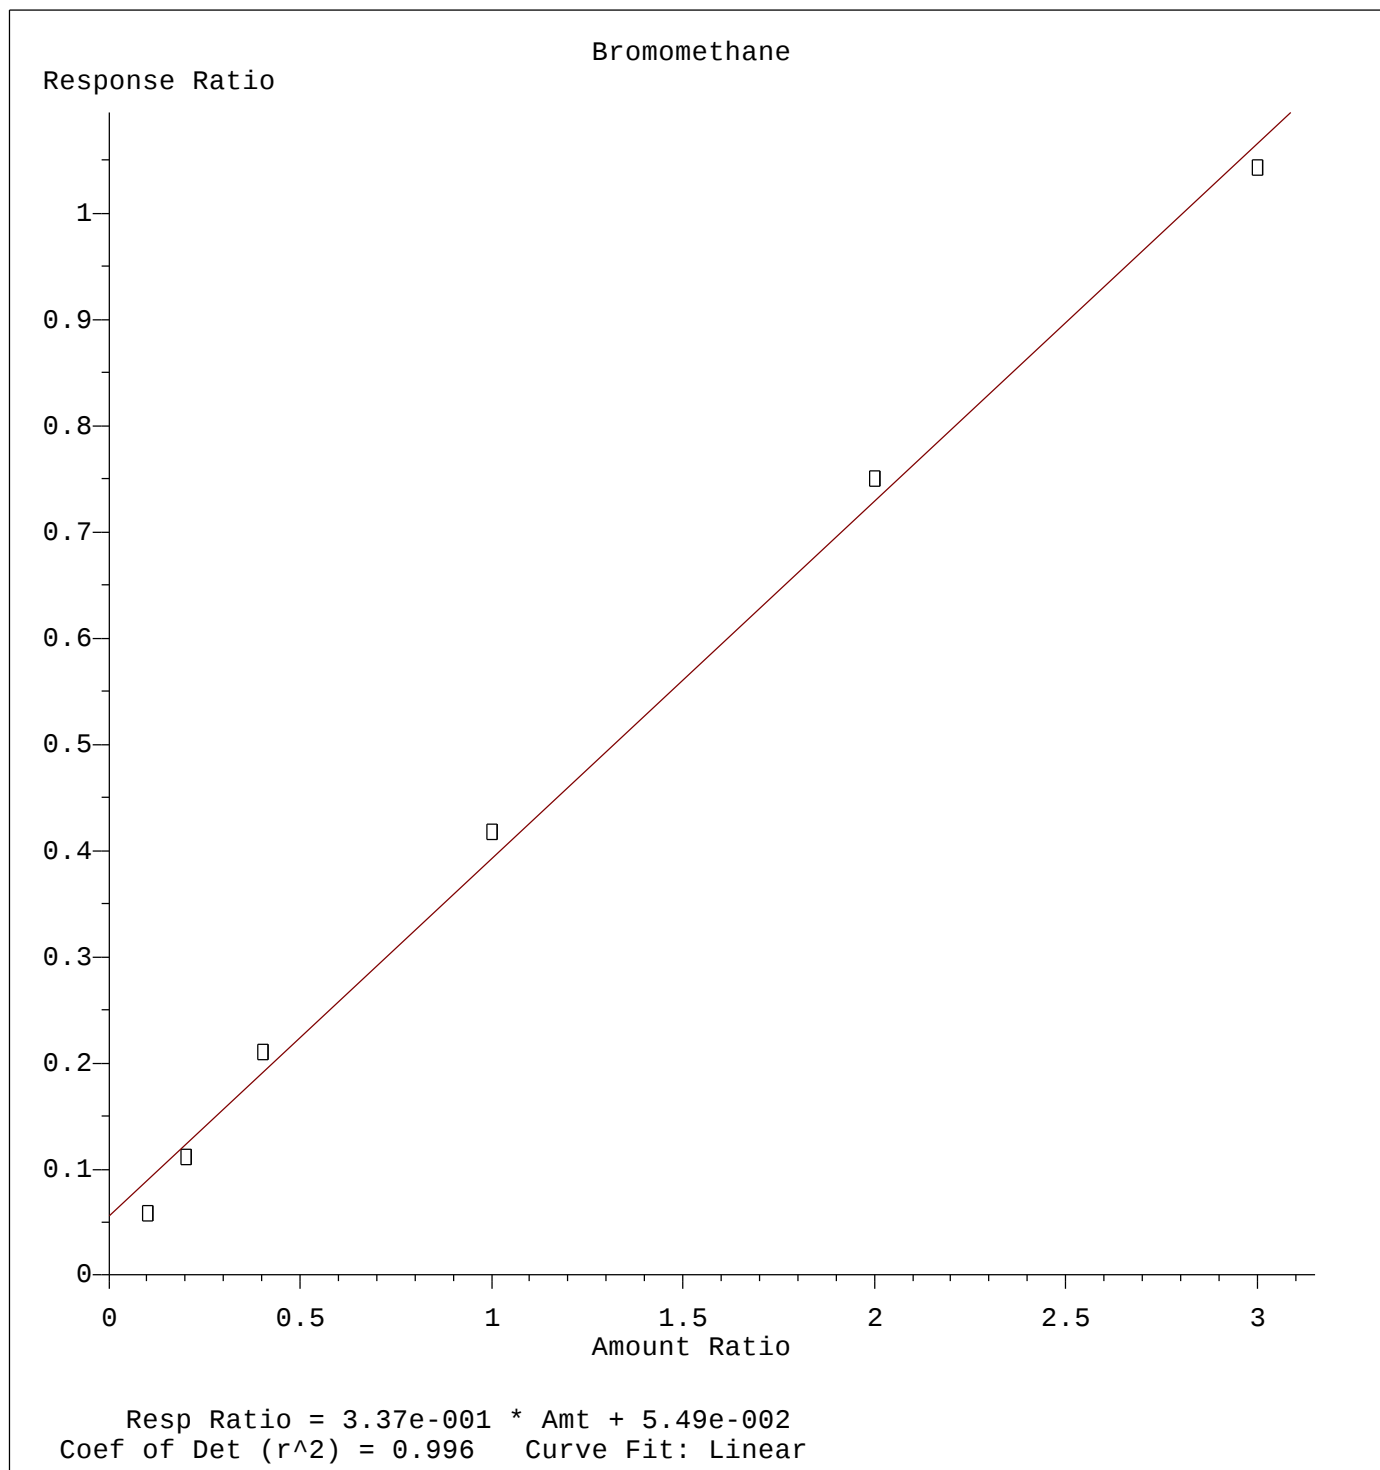

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_F\METHODS\82F091918S.M  
Calibration Table Last Updated: Thu Sep 20 15:16:16 2018