


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA F\DATA\VF091918\
 Data File : VF060276.D
 Acq On : 19 Sep 2018 12:15
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00/5mL/MSVOA F/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F091918S.M
 Title : SW846 8260
 Last Update : Thu Sep 20 02:58:42 2018

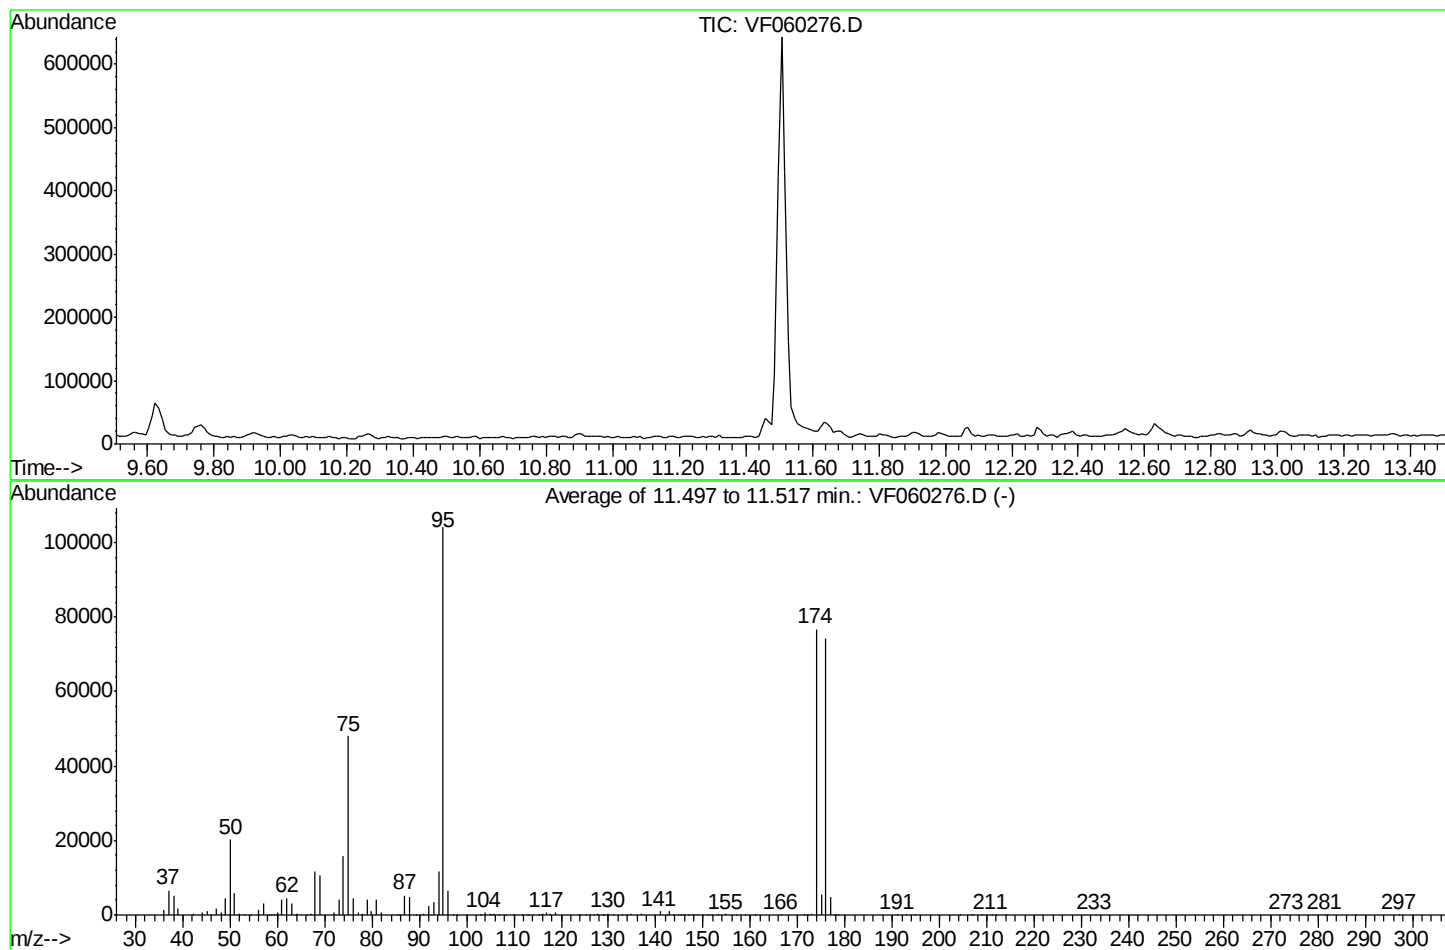

AutoFind: Scans 1102, 1103, 1104; Background Corrected with Scan 1097

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	20276	PASS
75	95	30	60	46.1	48026	PASS
95	95	100	100	100.0	104096	PASS
96	95	5	9	6.2	6410	PASS
173	174	0.00	2	0.4	342	PASS
174	95	50	100	73.8	76786	PASS
175	174	5	9	7.0	5370	PASS
176	174	95	101	96.7	74269	PASS
177	176	5	9	6.5	4799	PASS