


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF092518\
Data File : VF060323.D
Acq On : 25 Sep 2018 12:44
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F091918S.M
Title : SW846 8260
Last Update : Thu Sep 20 02:58:42 2018

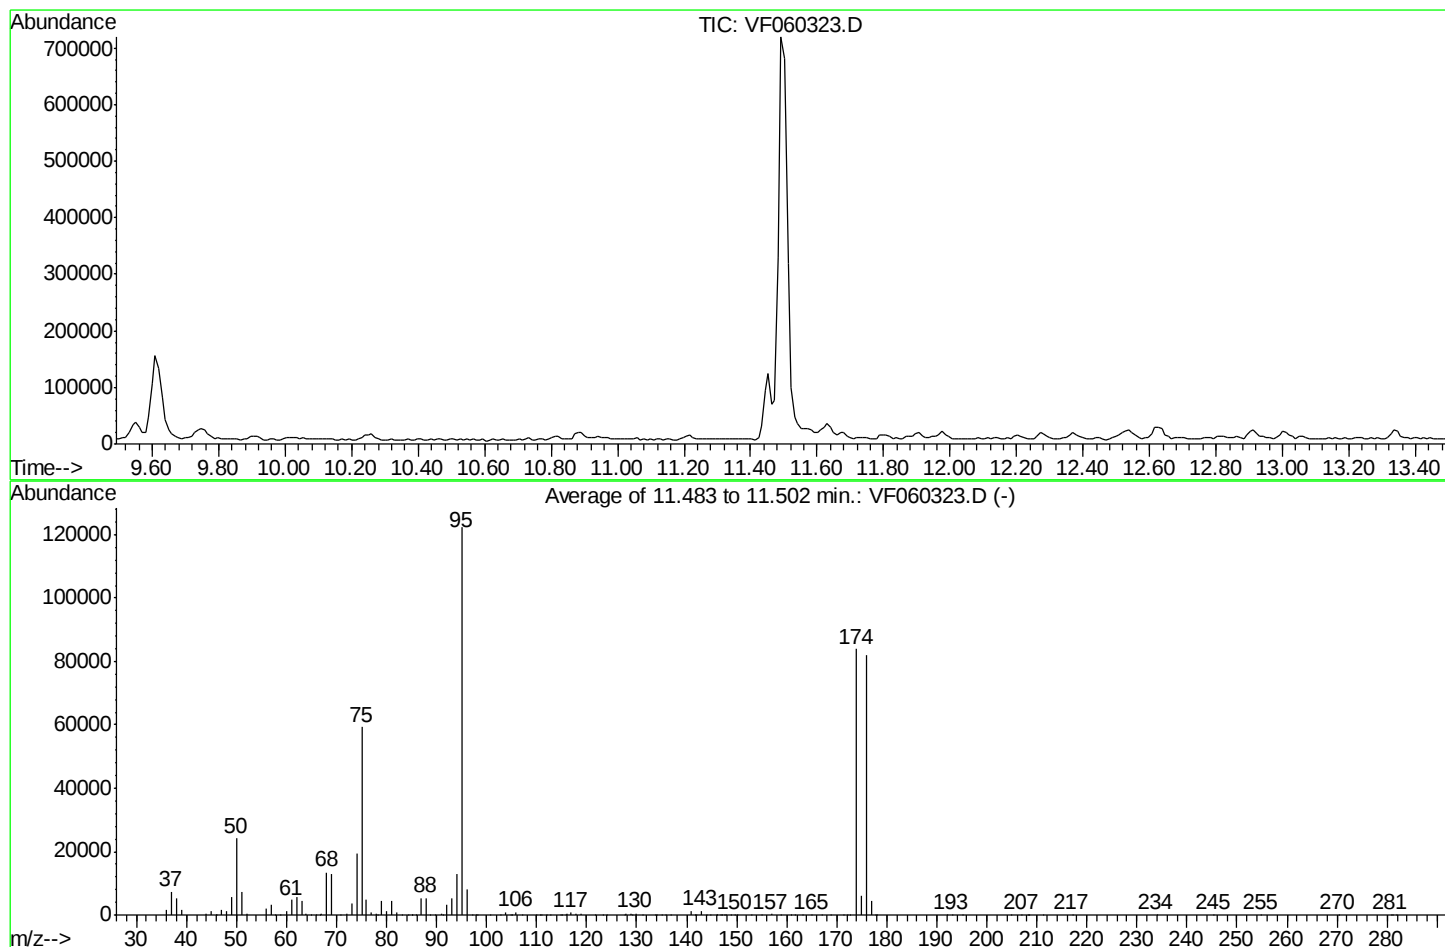

AutoFind: Scans 1101, 1102, 1103; Background Corrected with Scan 1096

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	24074	PASS
75	95	30	60	48.4	59245	PASS
95	95	100	100	100.0	122306	PASS
96	95	5	9	6.5	7890	PASS
173	174	0.00	2	0.2	201	PASS
174	95	50	100	68.6	83861	PASS
175	174	5	9	7.5	6267	PASS
176	174	95	101	97.8	81977	PASS
177	176	5	9	5.5	4535	PASS