


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF092818\
Data File : VF060367.D
Acq On : 28 Sep 2018 13:20
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F091918S.M
Title : SW846 8260
Last Update : Thu Sep 20 02:58:42 2018

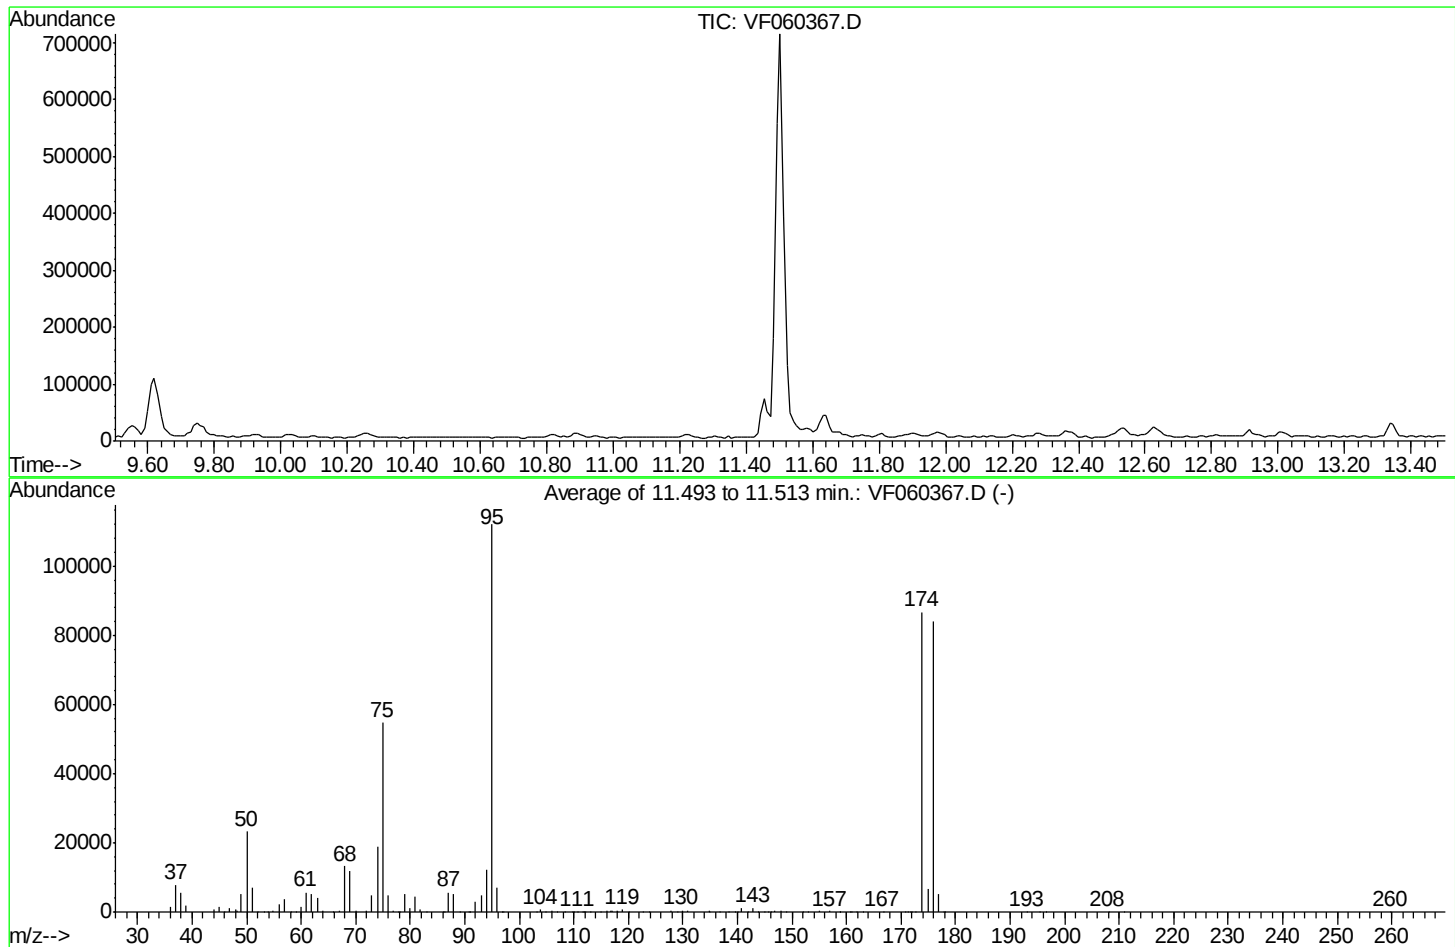

AutoFind: Scans 1102, 1103, 1104; Background Corrected with Scan 1096

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	23203	PASS
75	95	30	60	48.8	54688	PASS
95	95	100	100	100.0	112042	PASS
96	95	5	9	6.2	6940	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.3	86645	PASS
175	174	5	9	7.6	6592	PASS
176	174	95	101	96.9	84002	PASS
177	176	5	9	6.3	5257	PASS