


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF100118\
 Data File : VF060386.D
 Acq On : 1 Oct 2018 16:16
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00/5mL/MSVOA F/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100118S.M
 Title : SW846 8260
 Last Update : Tue Oct 02 11:42:56 2018

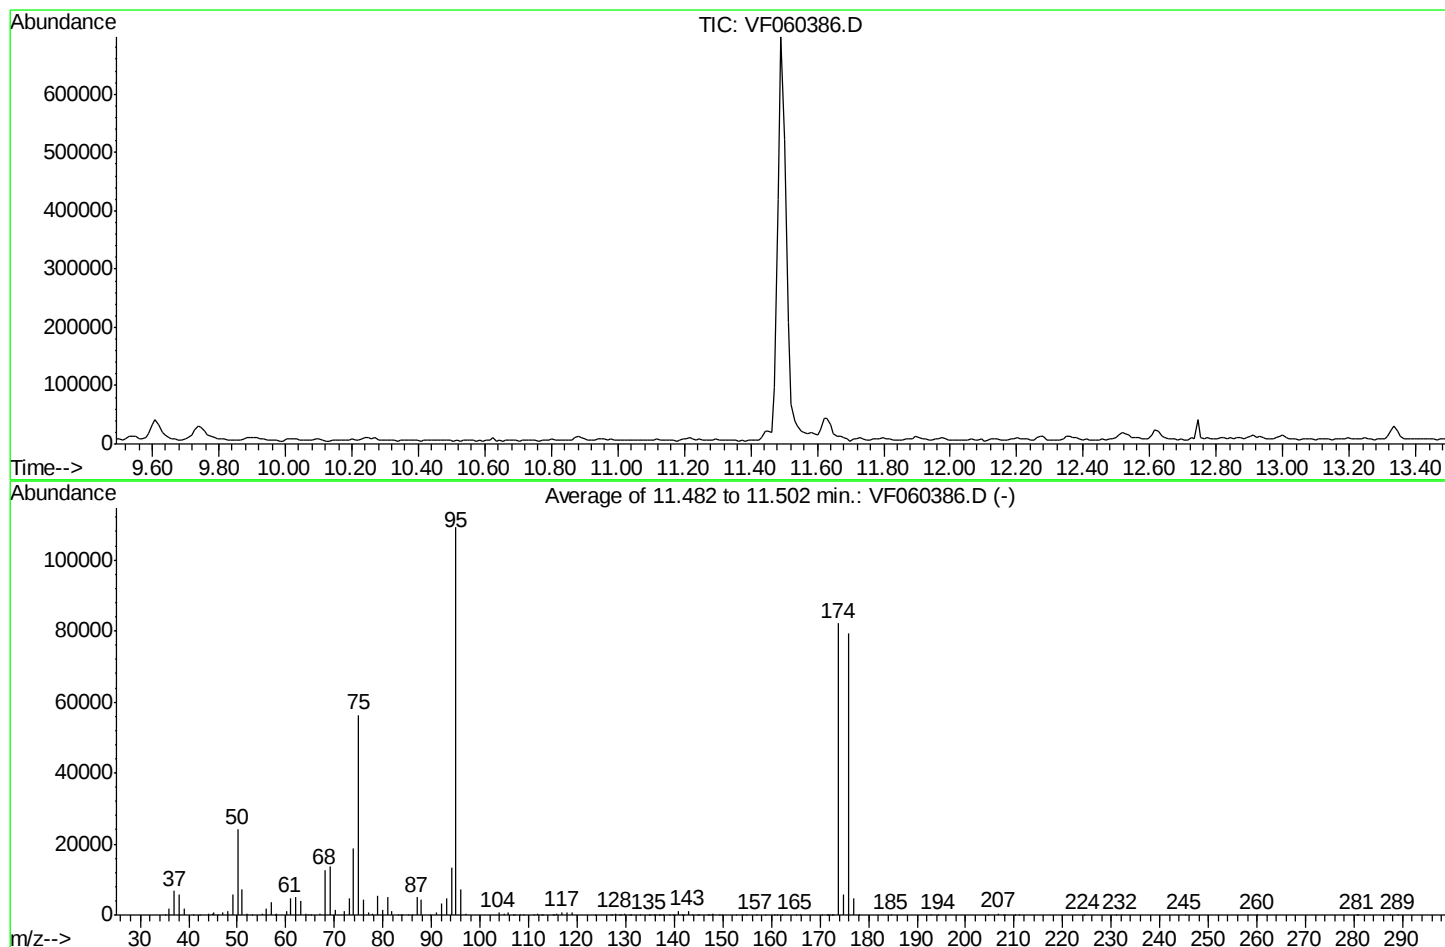

AutoFind: Scans 1101, 1102, 1103; Background Corrected with Scan 1096

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	24000	PASS
75	95	30	60	51.6	56309	PASS
95	95	100	100	100.0	109186	PASS
96	95	5	9	6.5	7108	PASS
173	174	0.00	2	0.2	151	PASS
174	95	50	100	75.2	82117	PASS
175	174	5	9	7.1	5821	PASS
176	174	95	101	96.7	79429	PASS
177	176	5	9	6.1	4865	PASS