


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF100218\
 Data File : VF060395.D
 Acq On : 2 Oct 2018 9:47
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00/5mL/MSVOA F/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100118S.M
 Title : SW846 8260
 Last Update : Tue Oct 02 11:42:56 2018

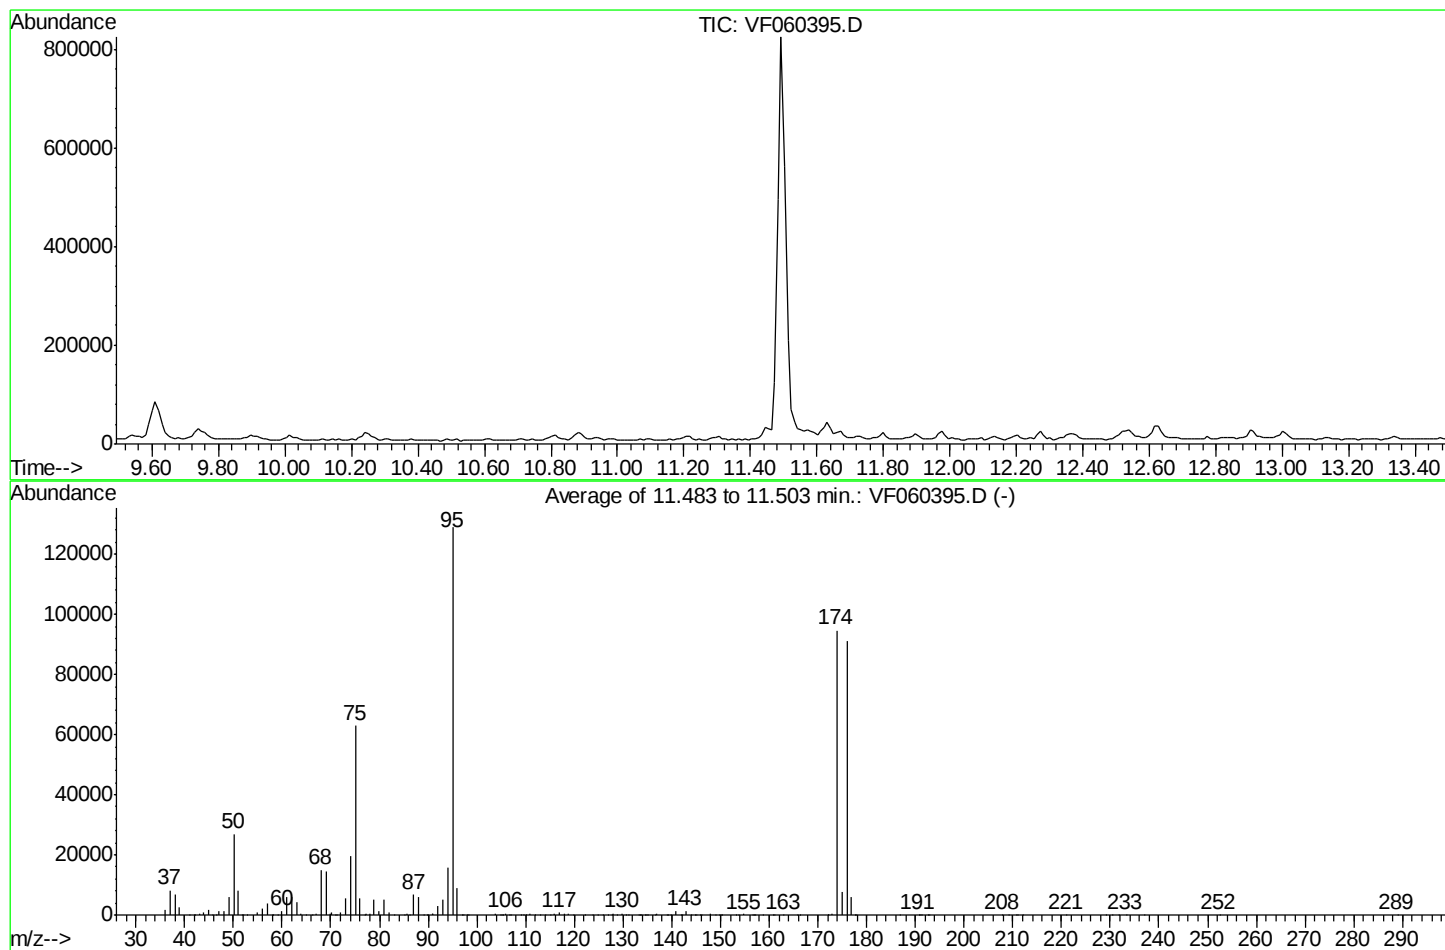

AutoFind: Scans 1101, 1102, 1103; Background Corrected with Scan 1092

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	26858	PASS
75	95	30	60	48.8	62946	PASS
95	95	100	100	100.0	128946	PASS
96	95	5	9	6.9	8914	PASS
173	174	0.00	2	0.4	421	PASS
174	95	50	100	73.4	94706	PASS
175	174	5	9	7.9	7491	PASS
176	174	95	101	96.4	91288	PASS
177	176	5	9	6.7	6138	PASS