


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF100418\
Data File : VF060436.D
Acq On : 4 Oct 2018 13:15
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 11:42:56 2018

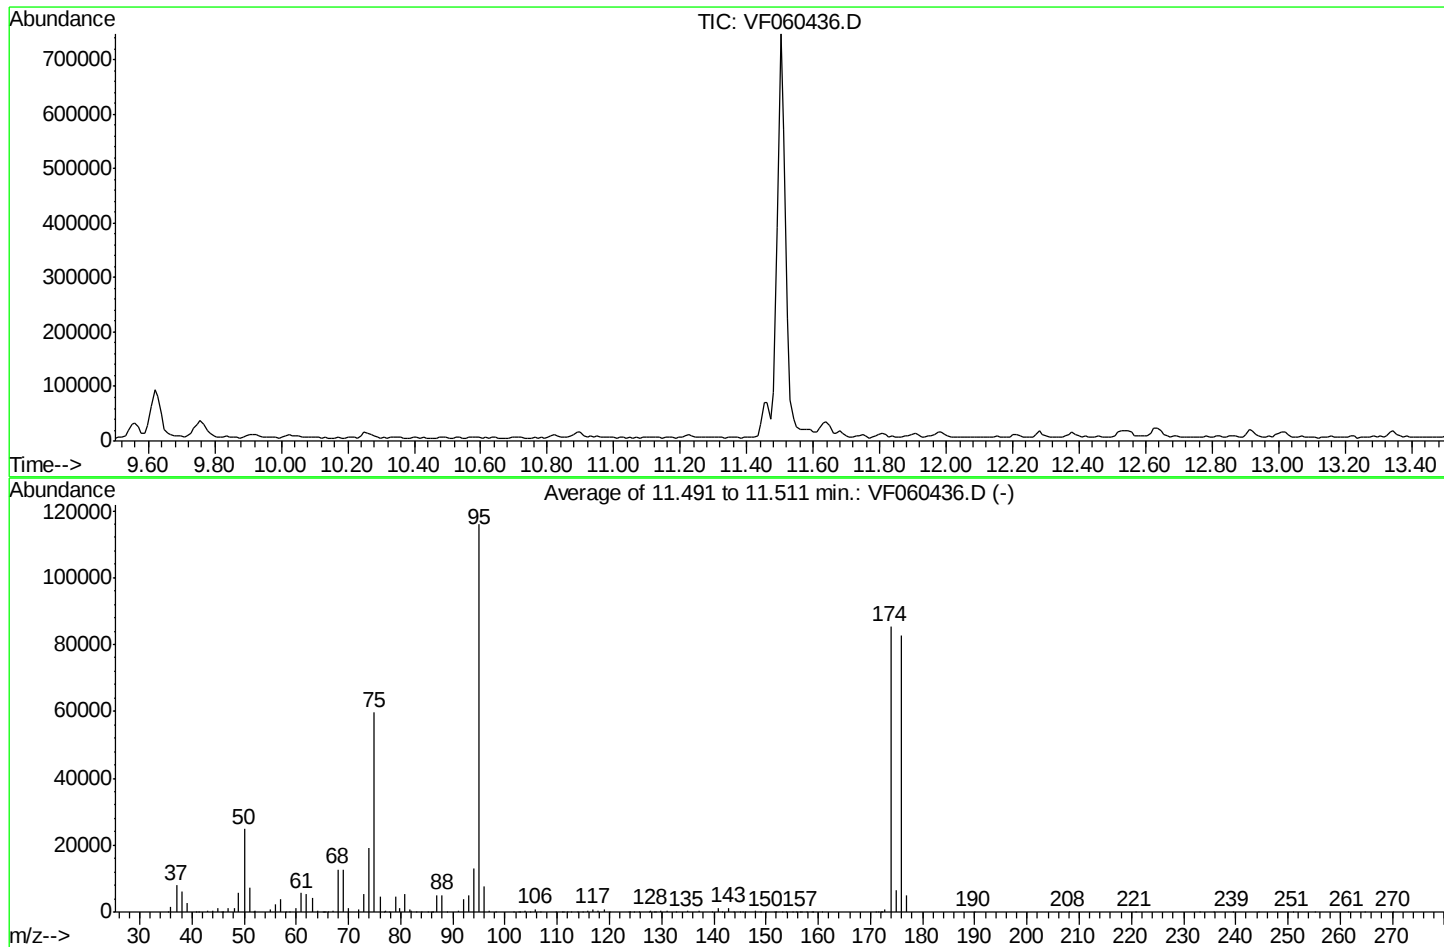

AutoFind: Scans 1102, 1103, 1104; Background Corrected with Scan 1096

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	24805	PASS
75	95	30	60	51.4	59560	PASS
95	95	100	100	100.0	115936	PASS
96	95	5	9	6.7	7749	PASS
173	174	0.00	2	0.9	739	PASS
174	95	50	100	73.5	85189	PASS
175	174	5	9	7.6	6456	PASS
176	174	95	101	97.1	82728	PASS
177	176	5	9	6.1	5029	PASS