


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF100518\
 Data File : VF060458.D
 Acq On : 5 Oct 2018 15:31
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00/5mL/MSVOA F/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100118S.M
 Title : SW846 8260
 Last Update : Tue Oct 02 11:42:56 2018

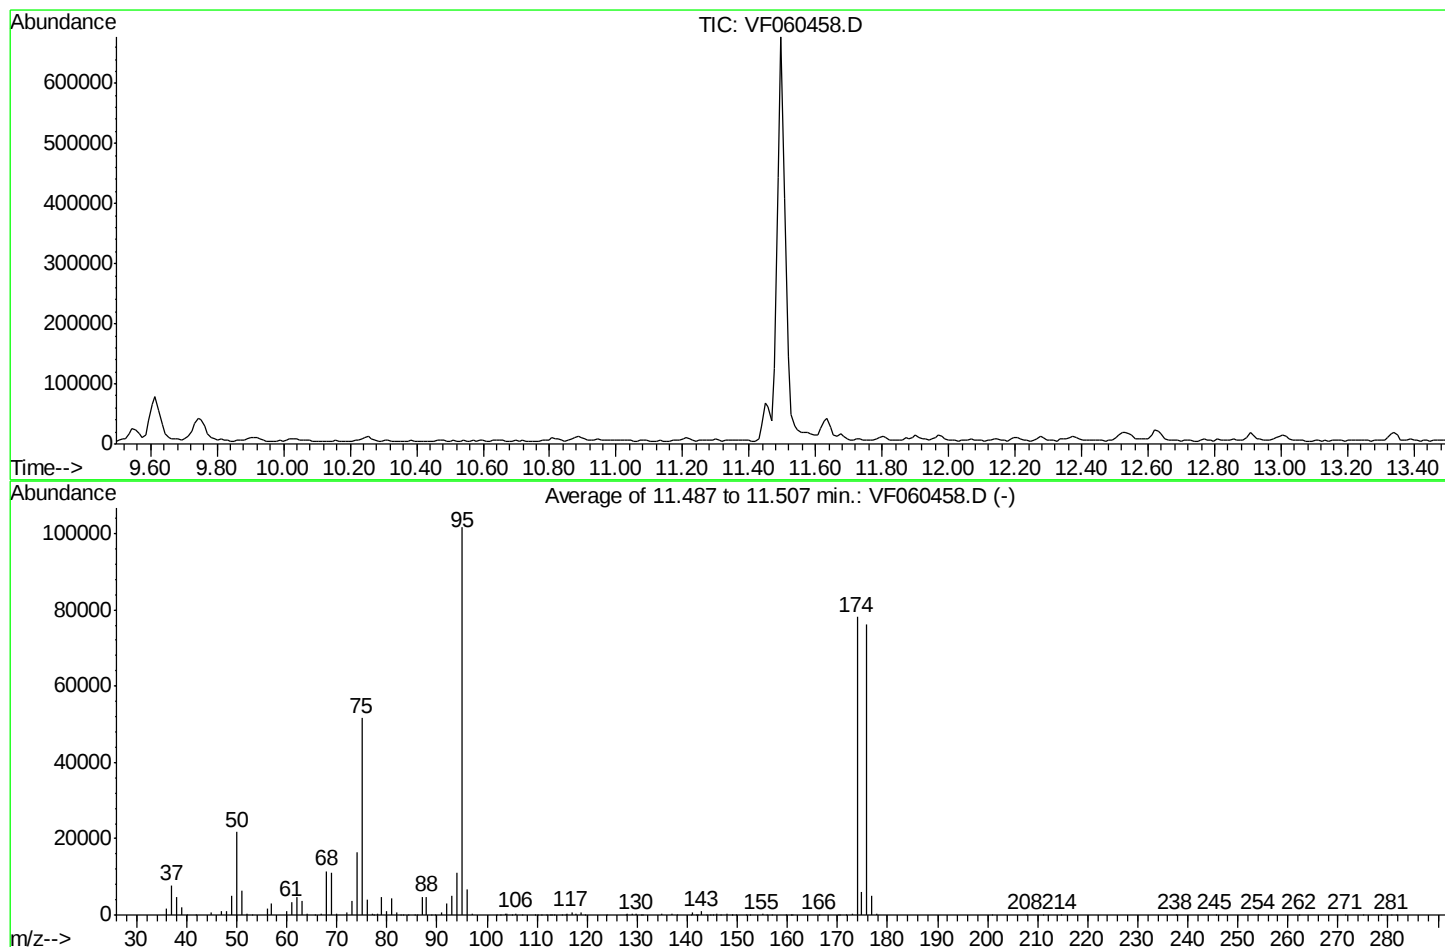

AutoFind: Scans 1101, 1102, 1103; Background Corrected with Scan 1096

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	21774	PASS
75	95	30	60	50.7	51552	PASS
95	95	100	100	100.0	101621	PASS
96	95	5	9	6.7	6828	PASS
173	174	0.00	2	0.6	487	PASS
174	95	50	100	76.8	78085	PASS
175	174	5	9	7.7	5996	PASS
176	174	95	101	97.4	76029	PASS
177	176	5	9	6.5	4954	PASS