


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_F\DATA\VF100818\
Data File : VF060477.D
Acq On : 8 Oct 2018 9:28
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA_F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 11:42:56 2018

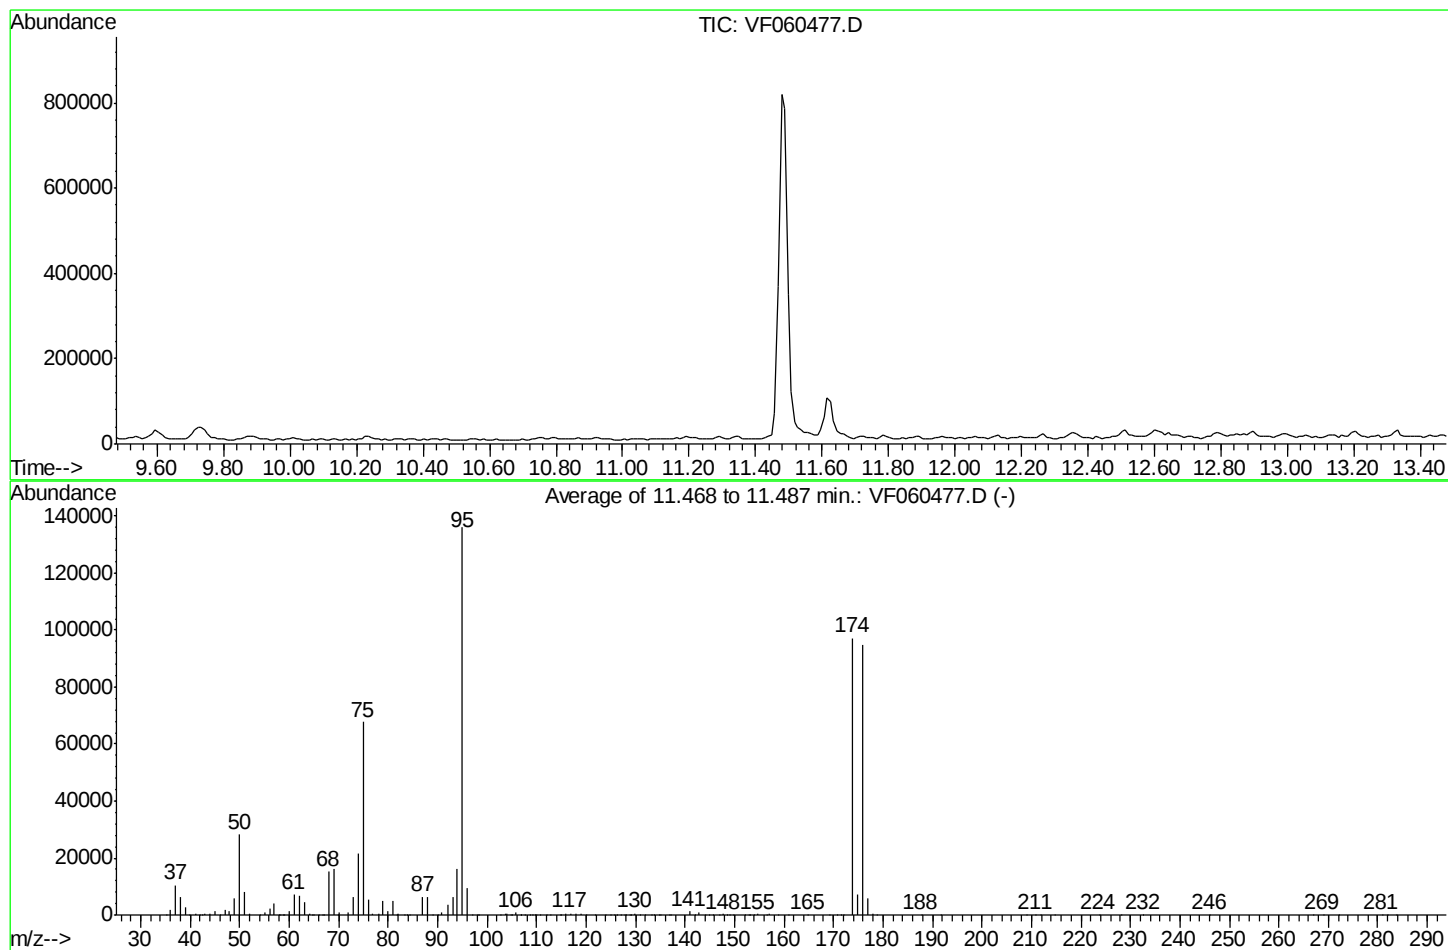

AutoFind: Scans 1099, 1100, 1101; Background Corrected with Scan 1091

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	28171	PASS
75	95	30	60	49.8	67797	PASS
95	95	100	100	100.0	136072	PASS
96	95	5	9	6.9	9420	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.3	97056	PASS
175	174	5	9	7.6	7372	PASS
176	174	95	101	97.9	95026	PASS
177	176	5	9	6.2	5900	PASS