



Dichlorodifluoromethane

Response Ratio

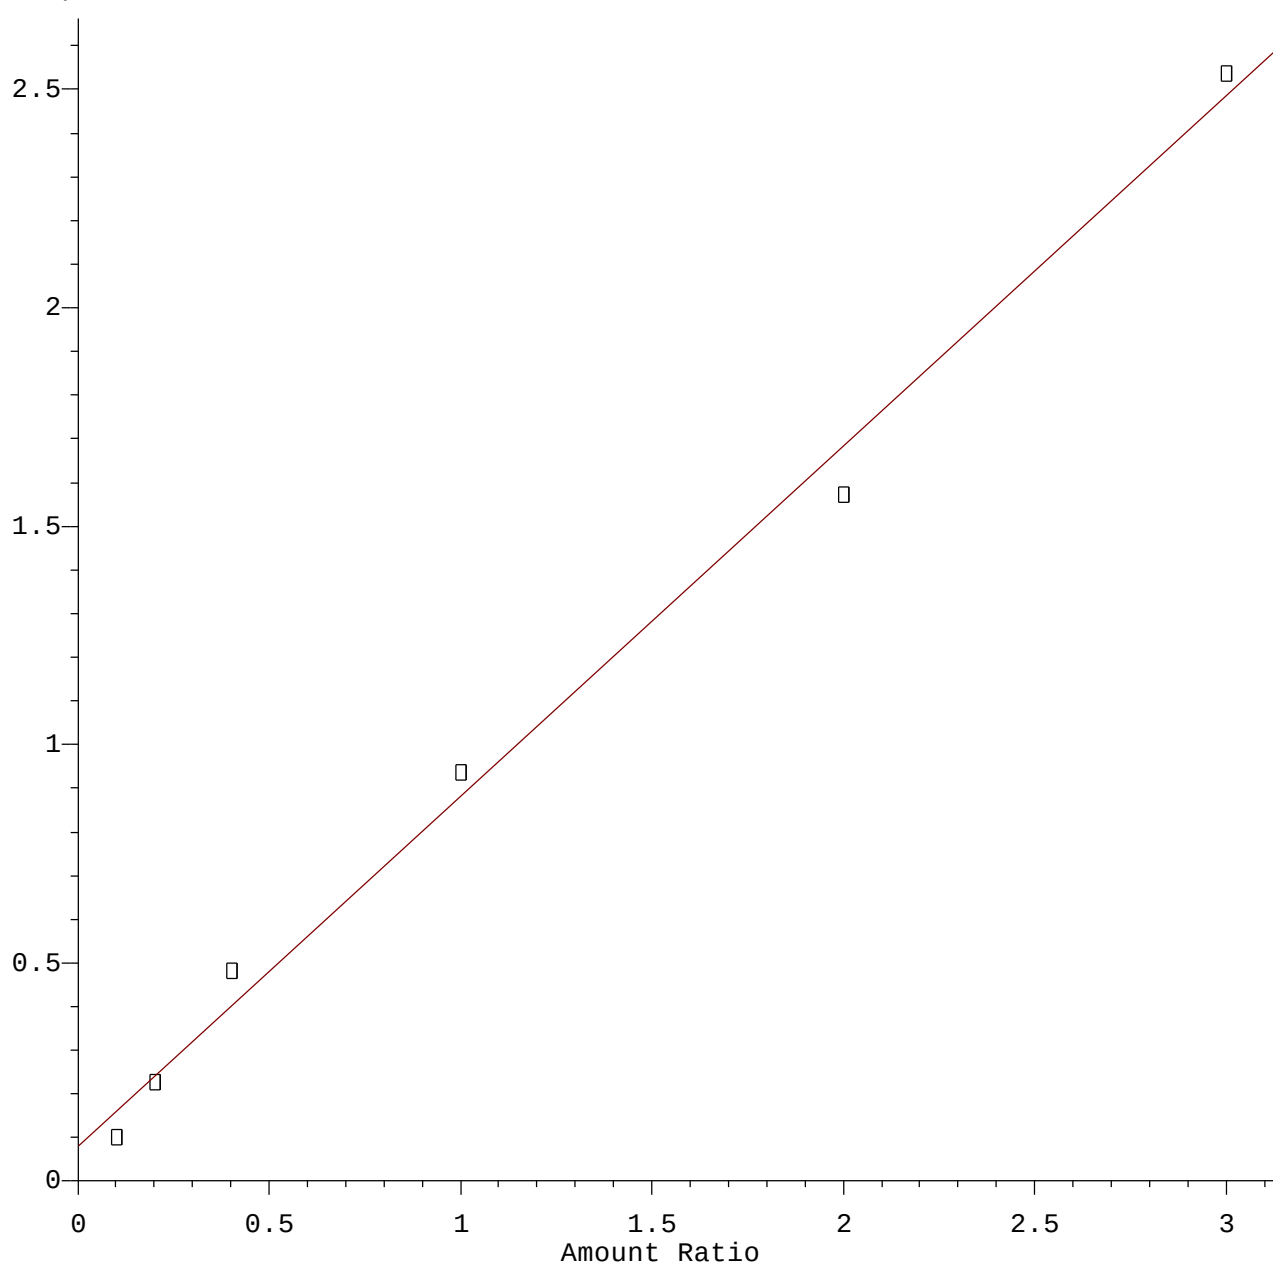


Resp Ratio = $8.03e-001 * \text{Amt} + 7.80e-002$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100918S.M
Calibration Table Last Updated: Wed Oct 10 02:28:46 2018

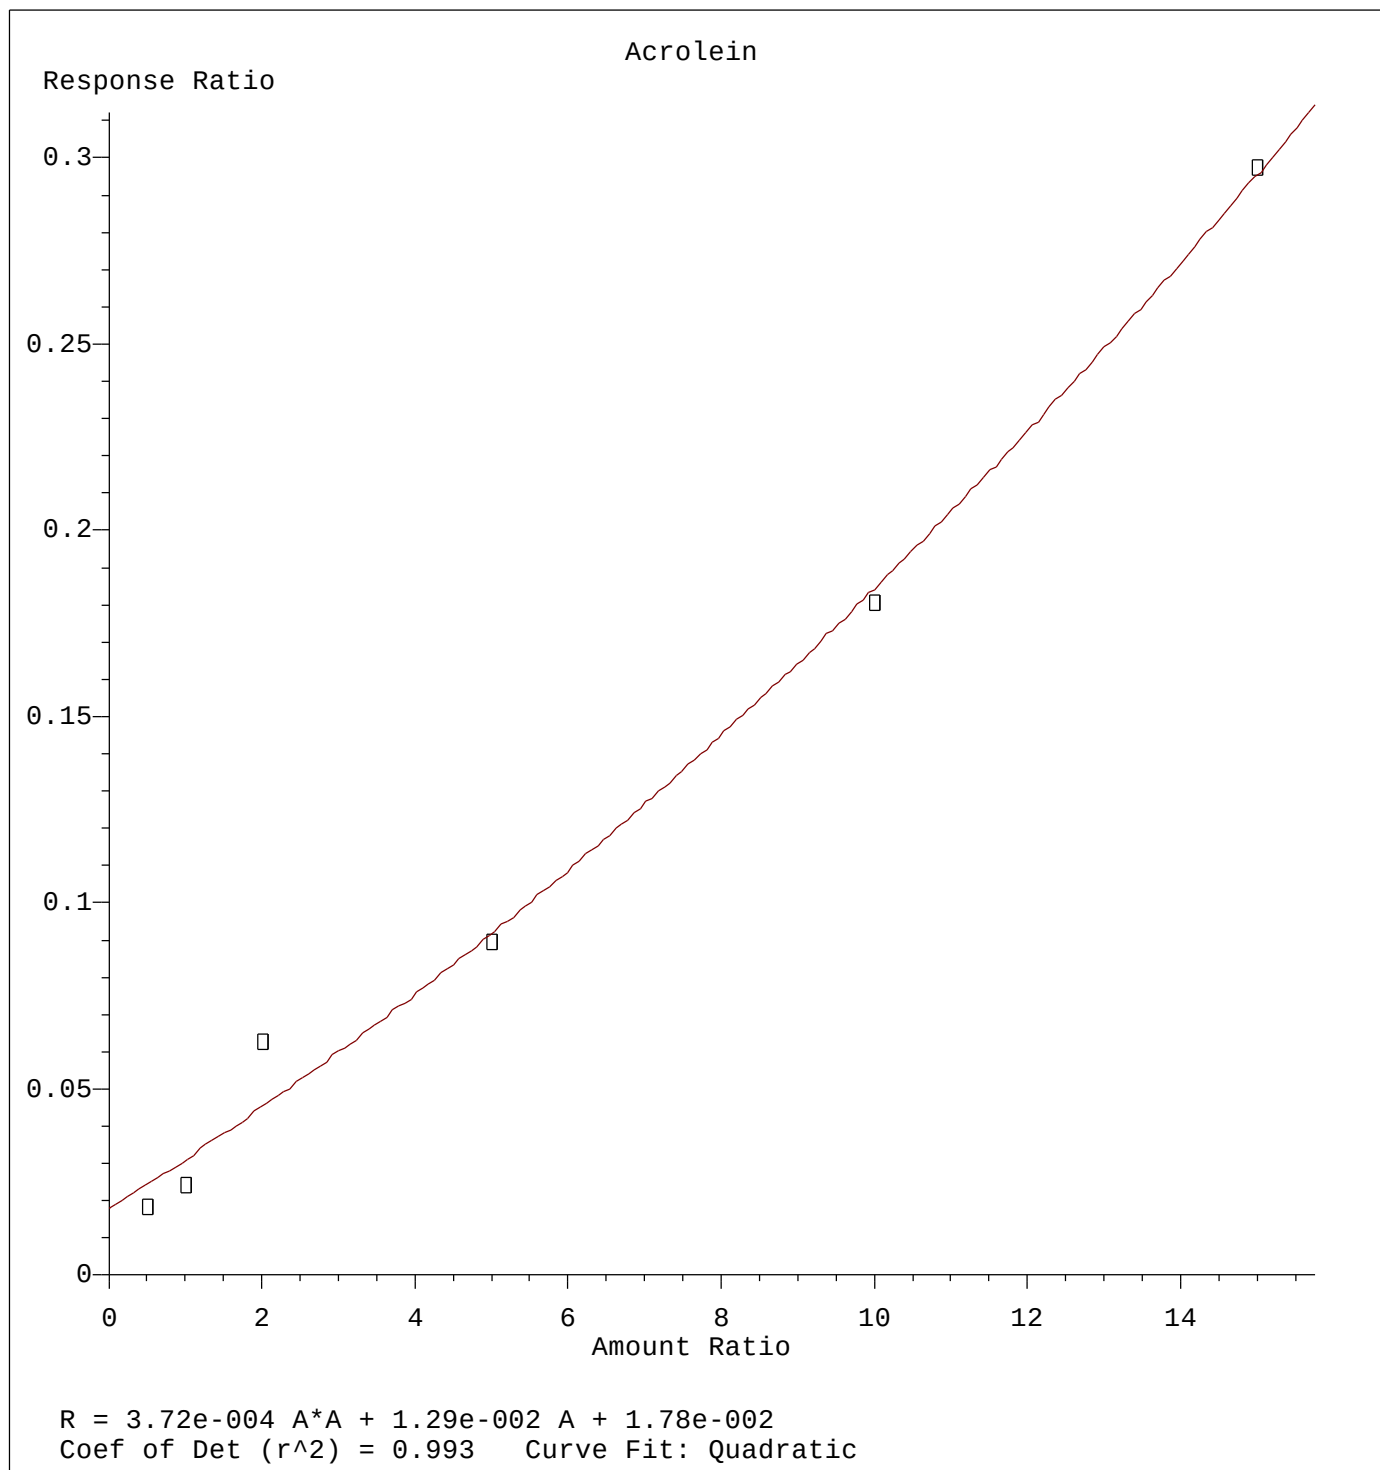


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100918S.M
Calibration Table Last Updated: Wed Oct 10 02:28:46 2018

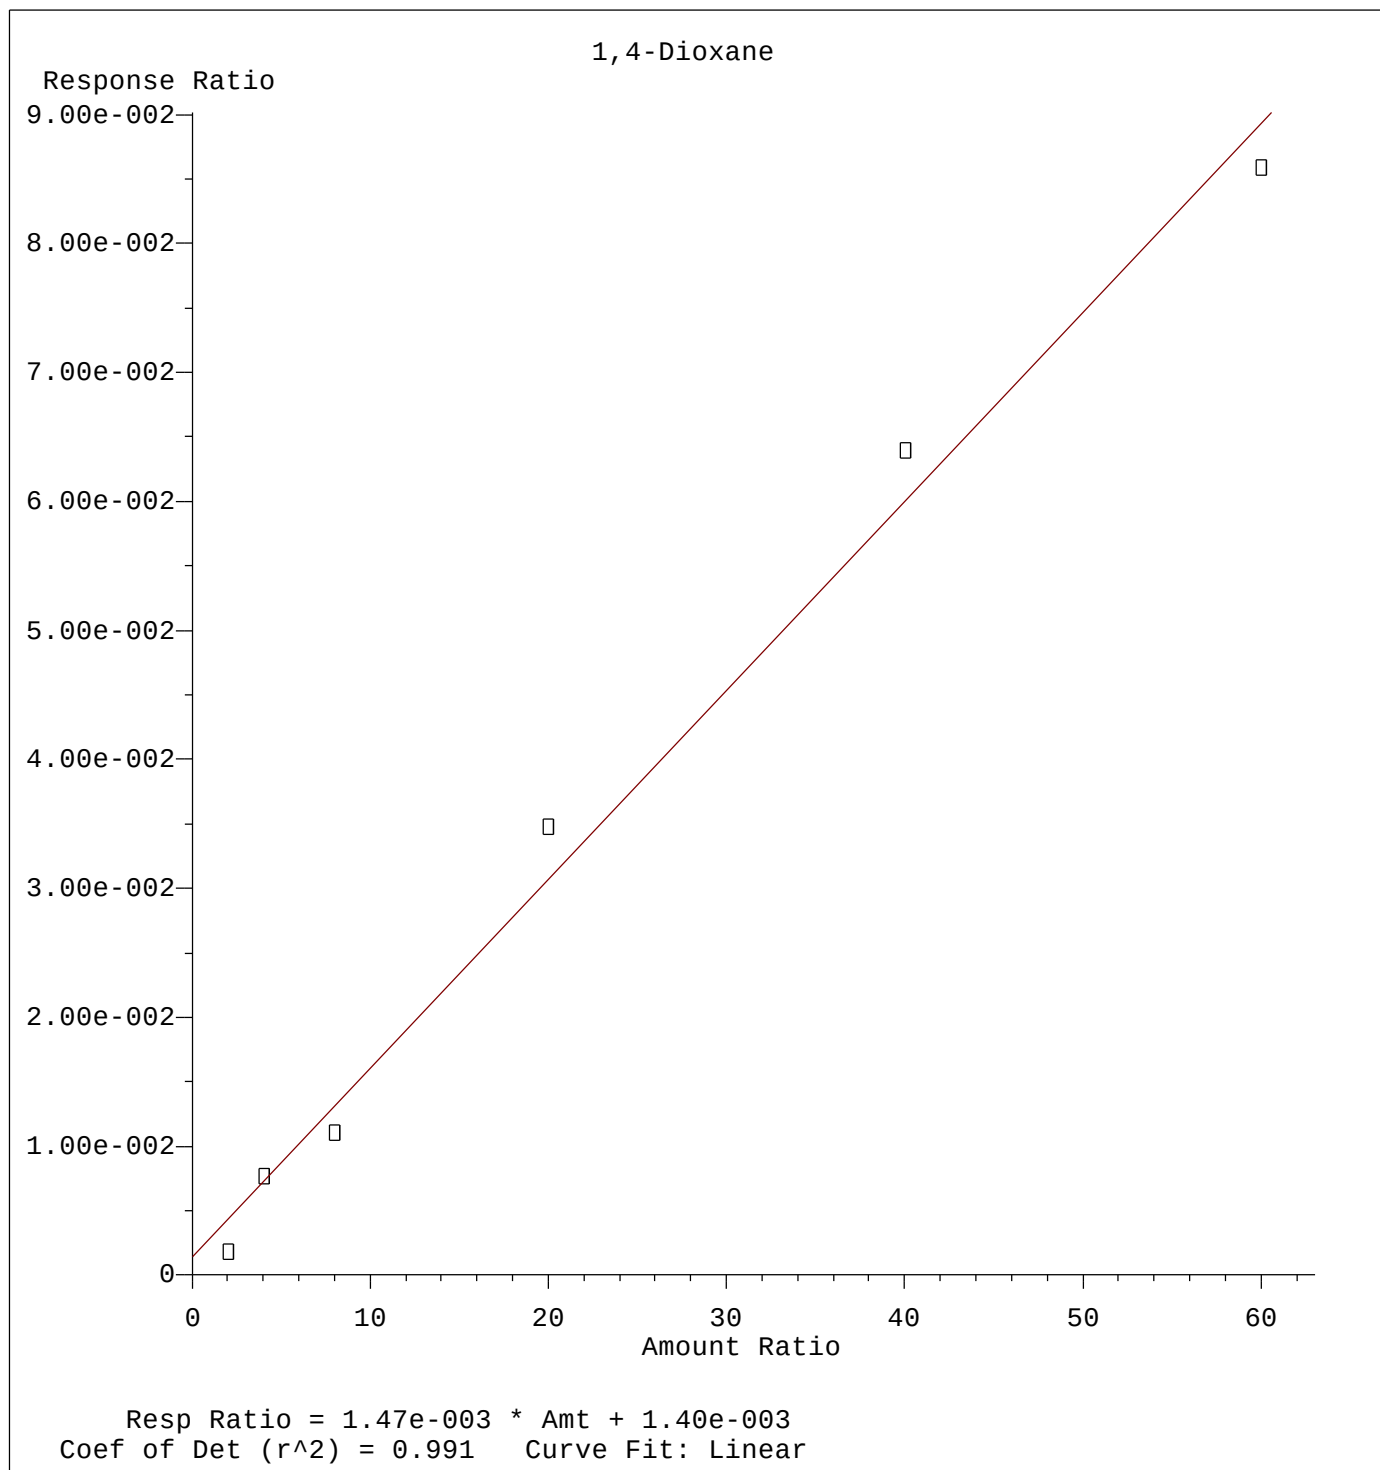

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100918S.M
Calibration Table Last Updated: Wed Oct 10 02:28:46 2018

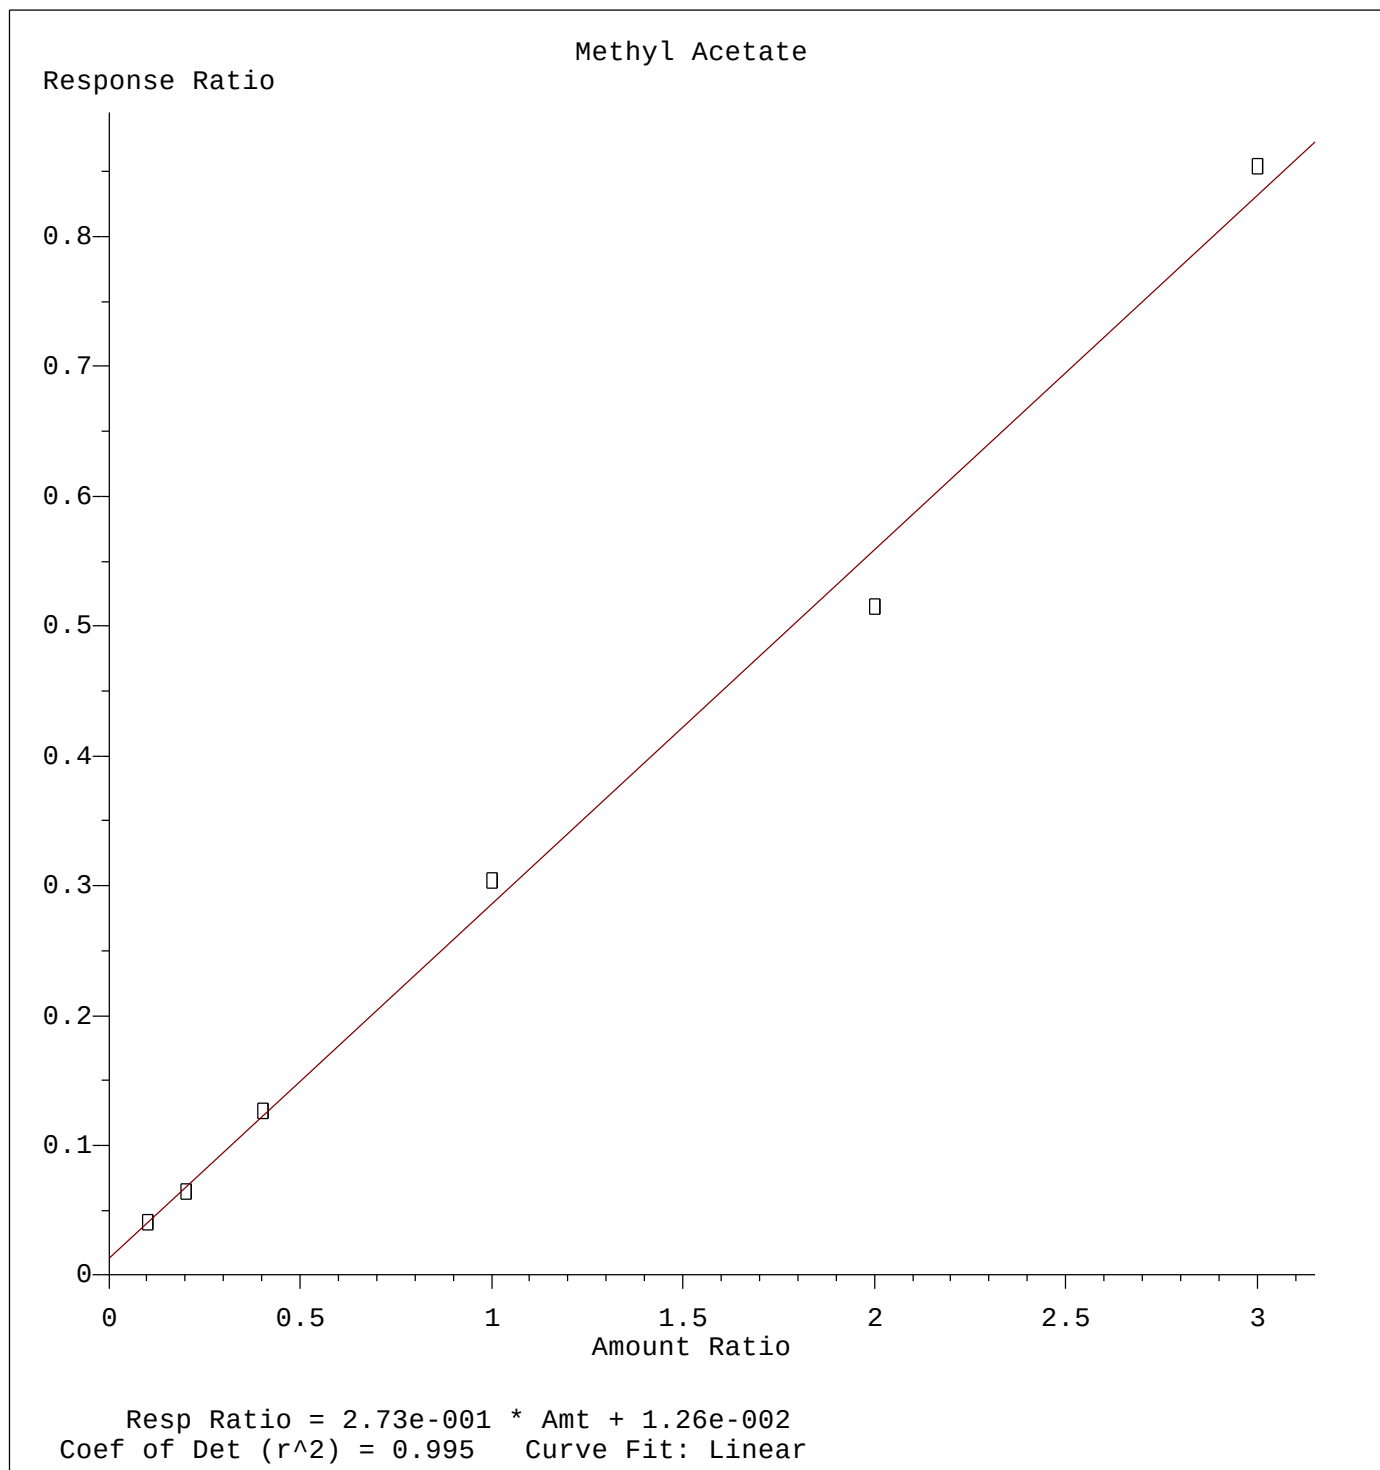

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100918S.M
Calibration Table Last Updated: Wed Oct 10 02:28:46 2018

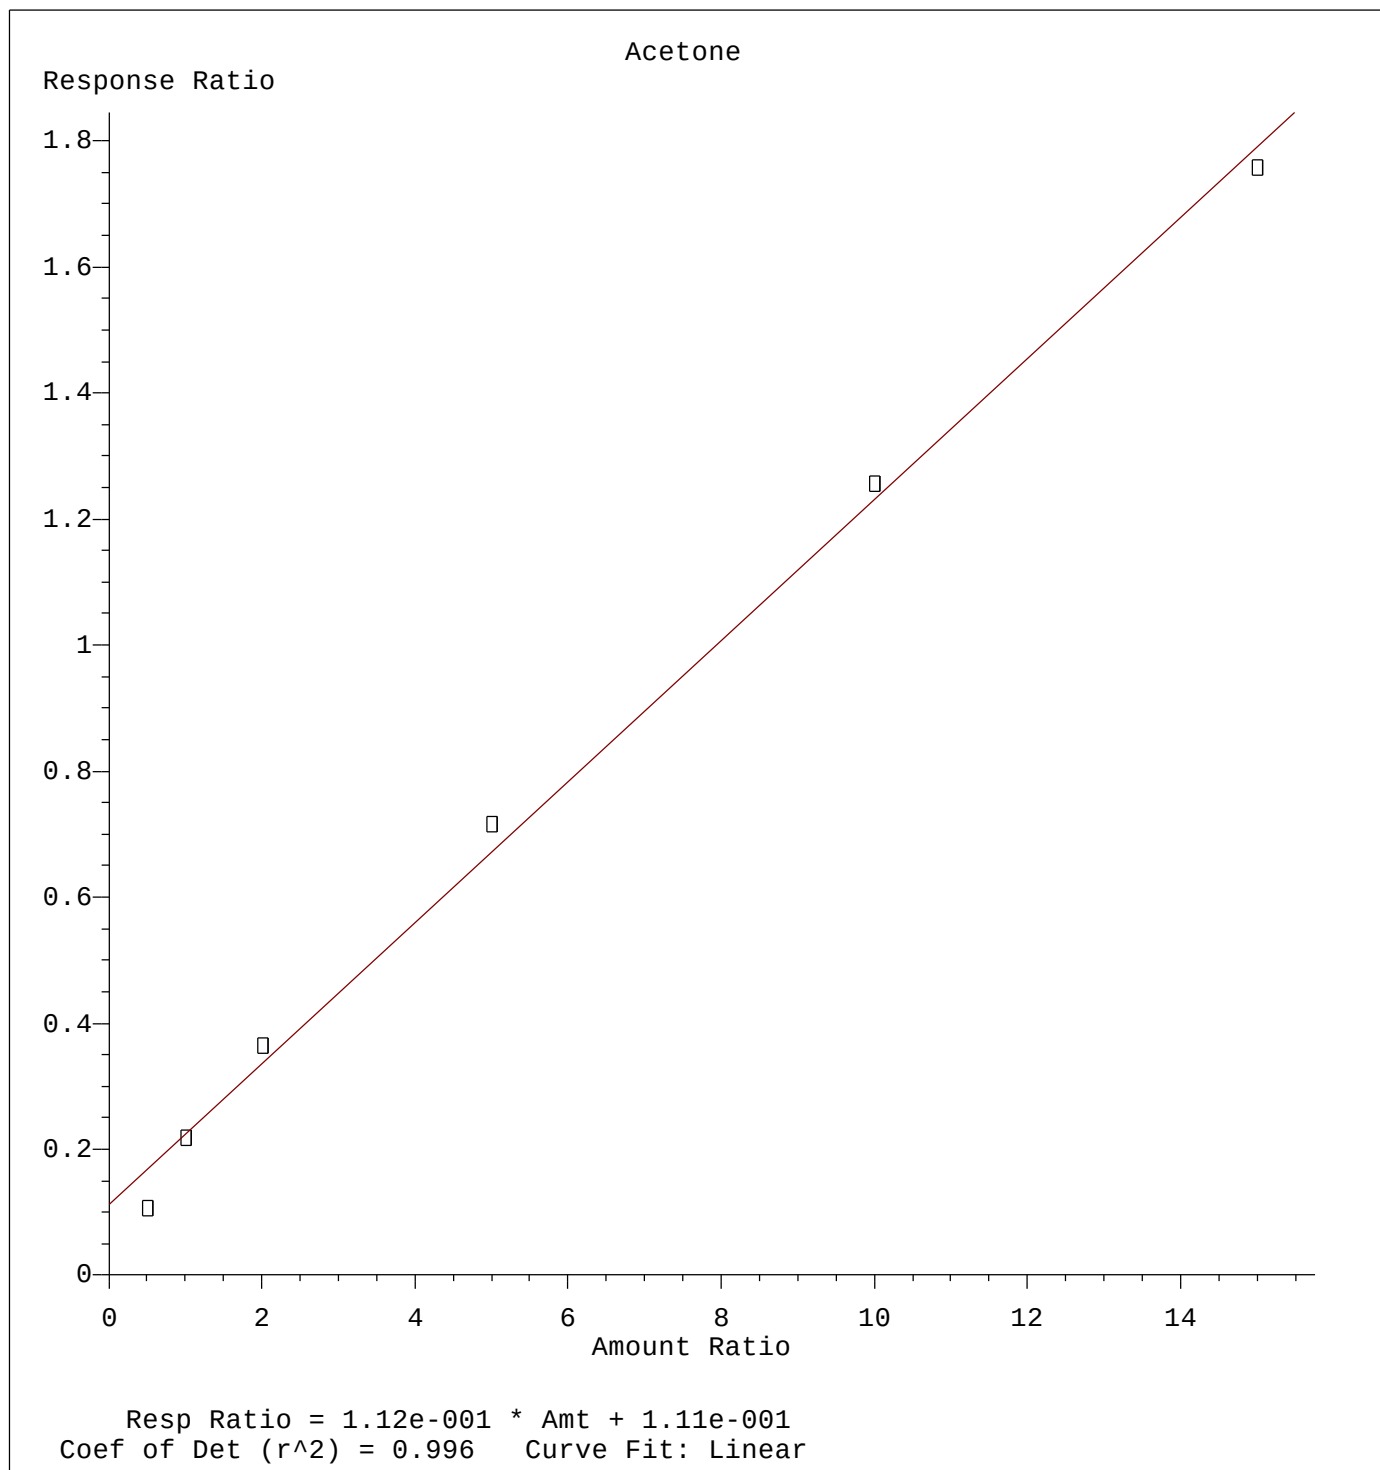

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100918S.M
Calibration Table Last Updated: Wed Oct 10 02:28:46 2018