


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF100918\
Data File : VF060489.D
Acq On : 9 Oct 2018 13:40
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F100918S.M
Title : SW846 8260
Last Update : Wed Oct 10 02:28:46 2018

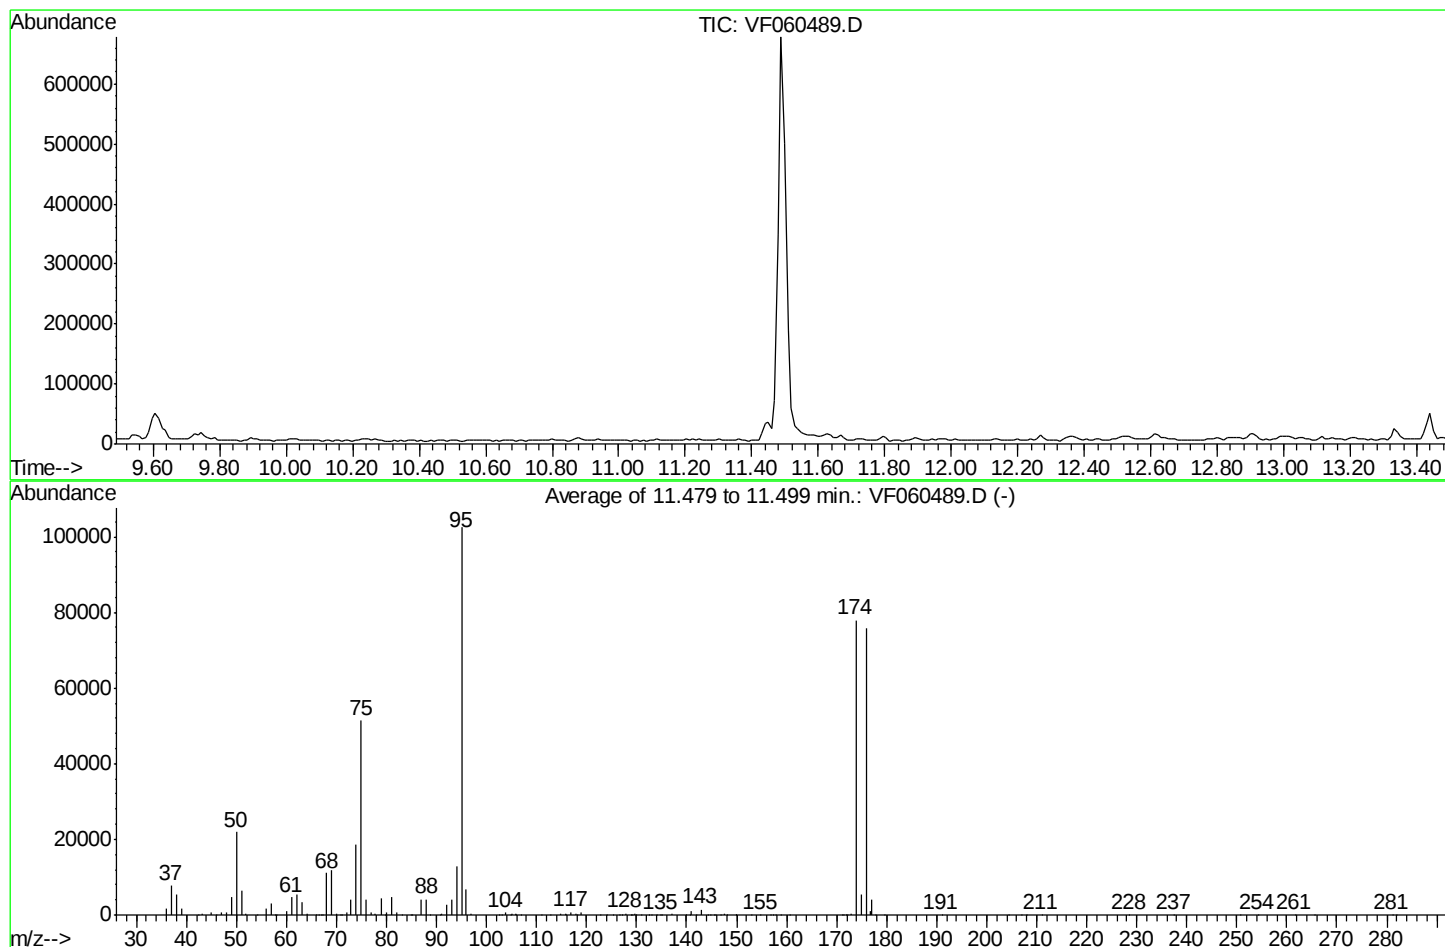

AutoFind: Scans 1100, 1101, 1102; Background Corrected with Scan 1095

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	21949	PASS
75	95	30	60	50.2	51410	PASS
95	95	100	100	100.0	102482	PASS
96	95	5	9	6.6	6727	PASS
173	174	0.00	2	0.3	219	PASS
174	95	50	100	76.0	77914	PASS
175	174	5	9	6.8	5313	PASS
176	174	95	101	97.5	75978	PASS
177	176	5	9	5.4	4079	PASS