



Dichlorodifluoromethane

Response Ratio

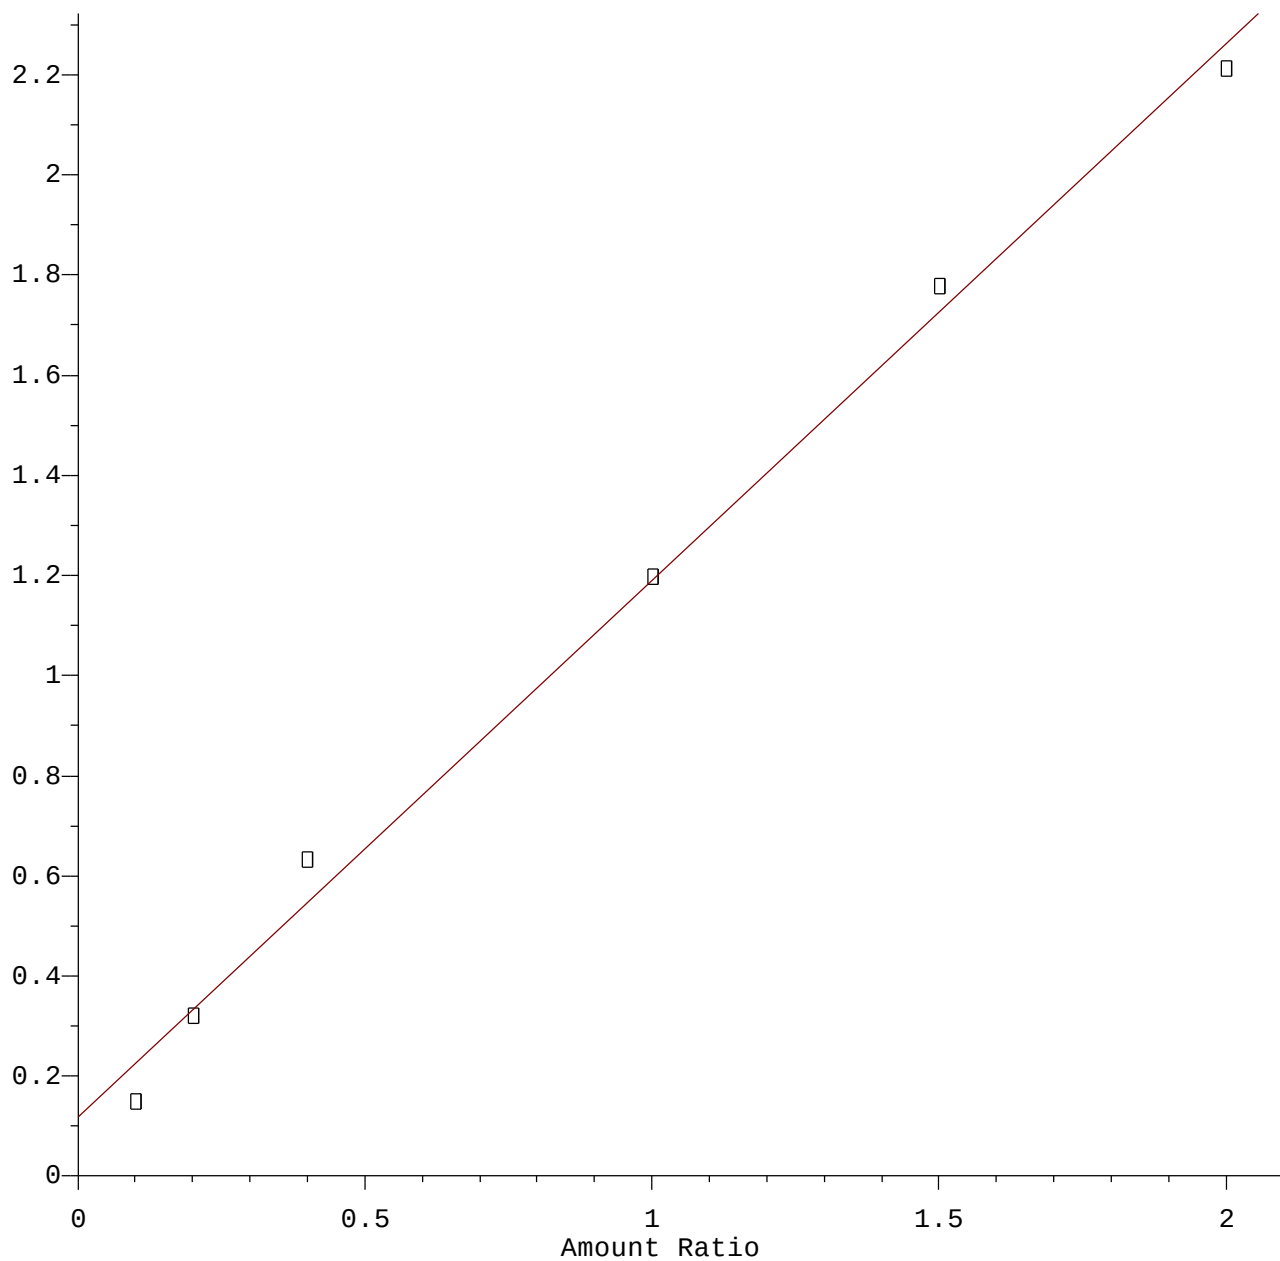

Resp Ratio = 1.07e+000 * Amt + 1.18e-001
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Calibration Table Last Updated: Fri Oct 26 02:17:41 2018

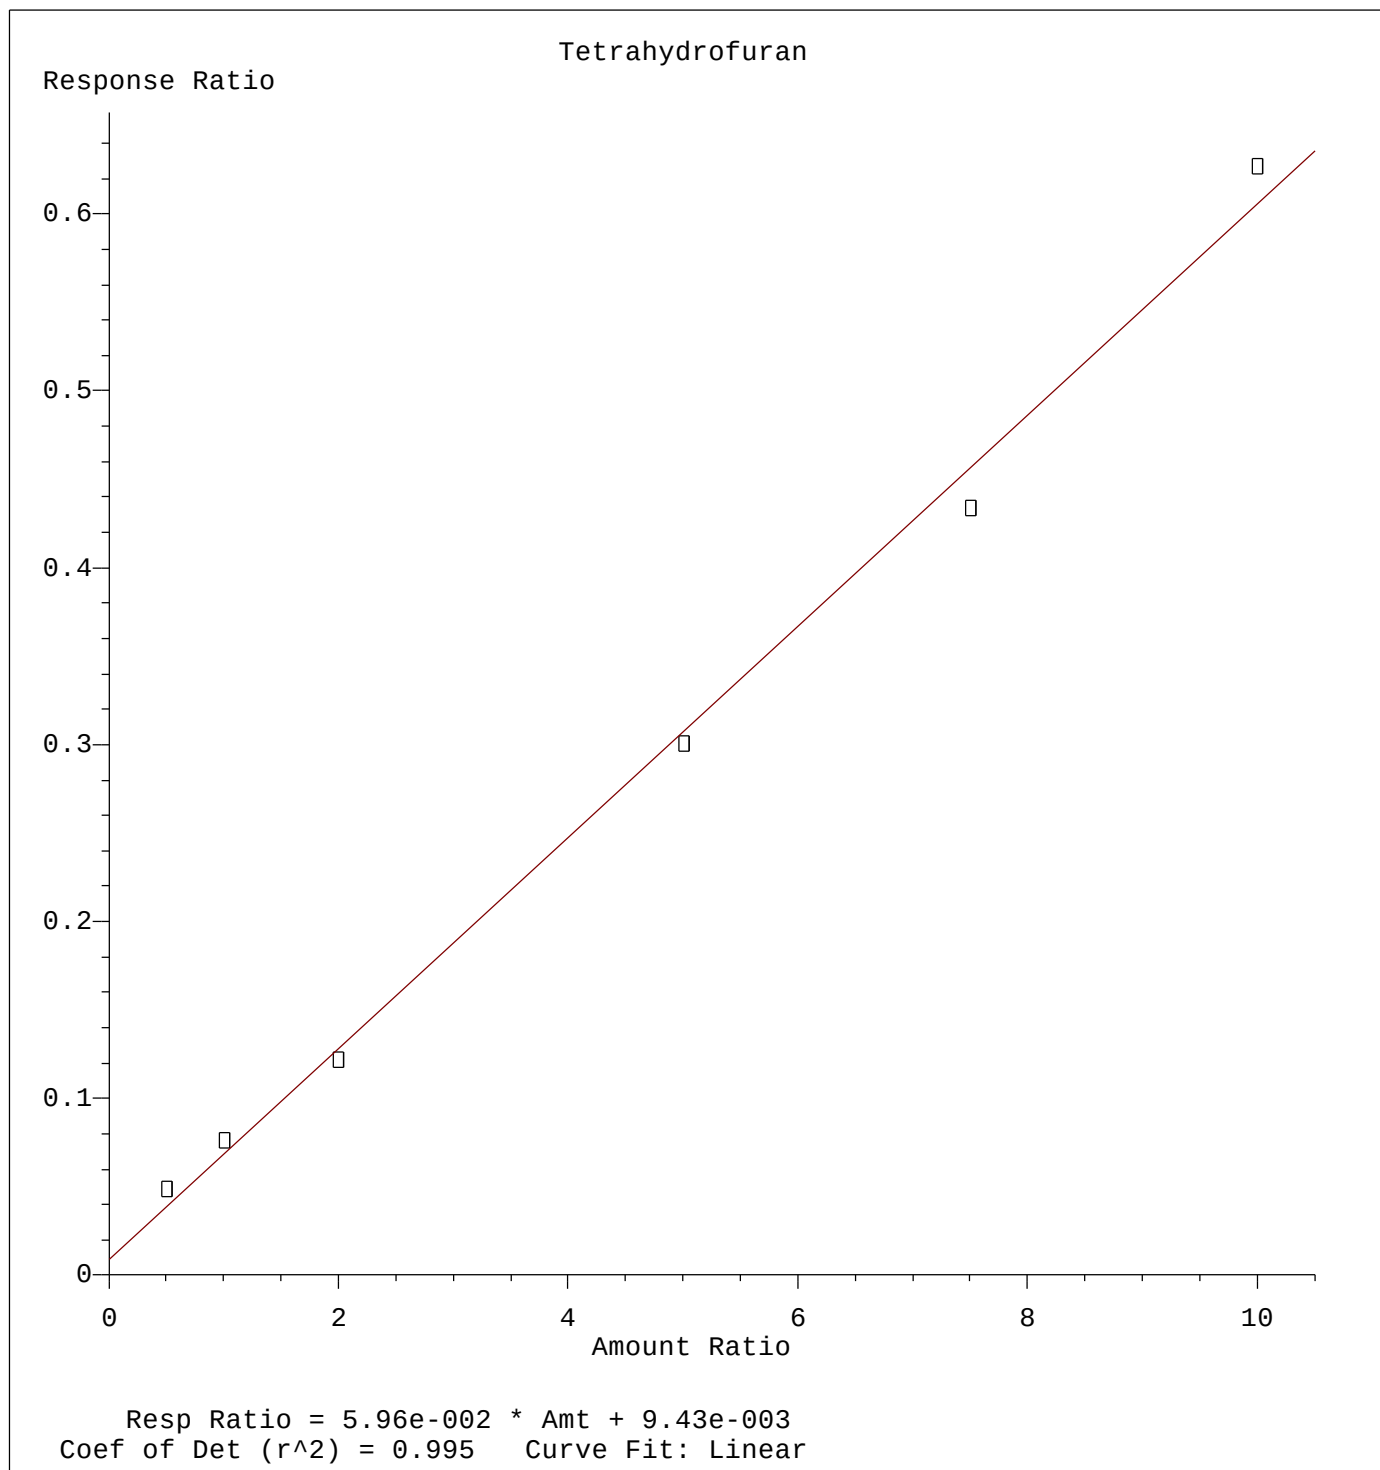

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Calibration Table Last Updated: Fri Oct 26 02:17:41 2018


Methylene Chloride

Response Ratio

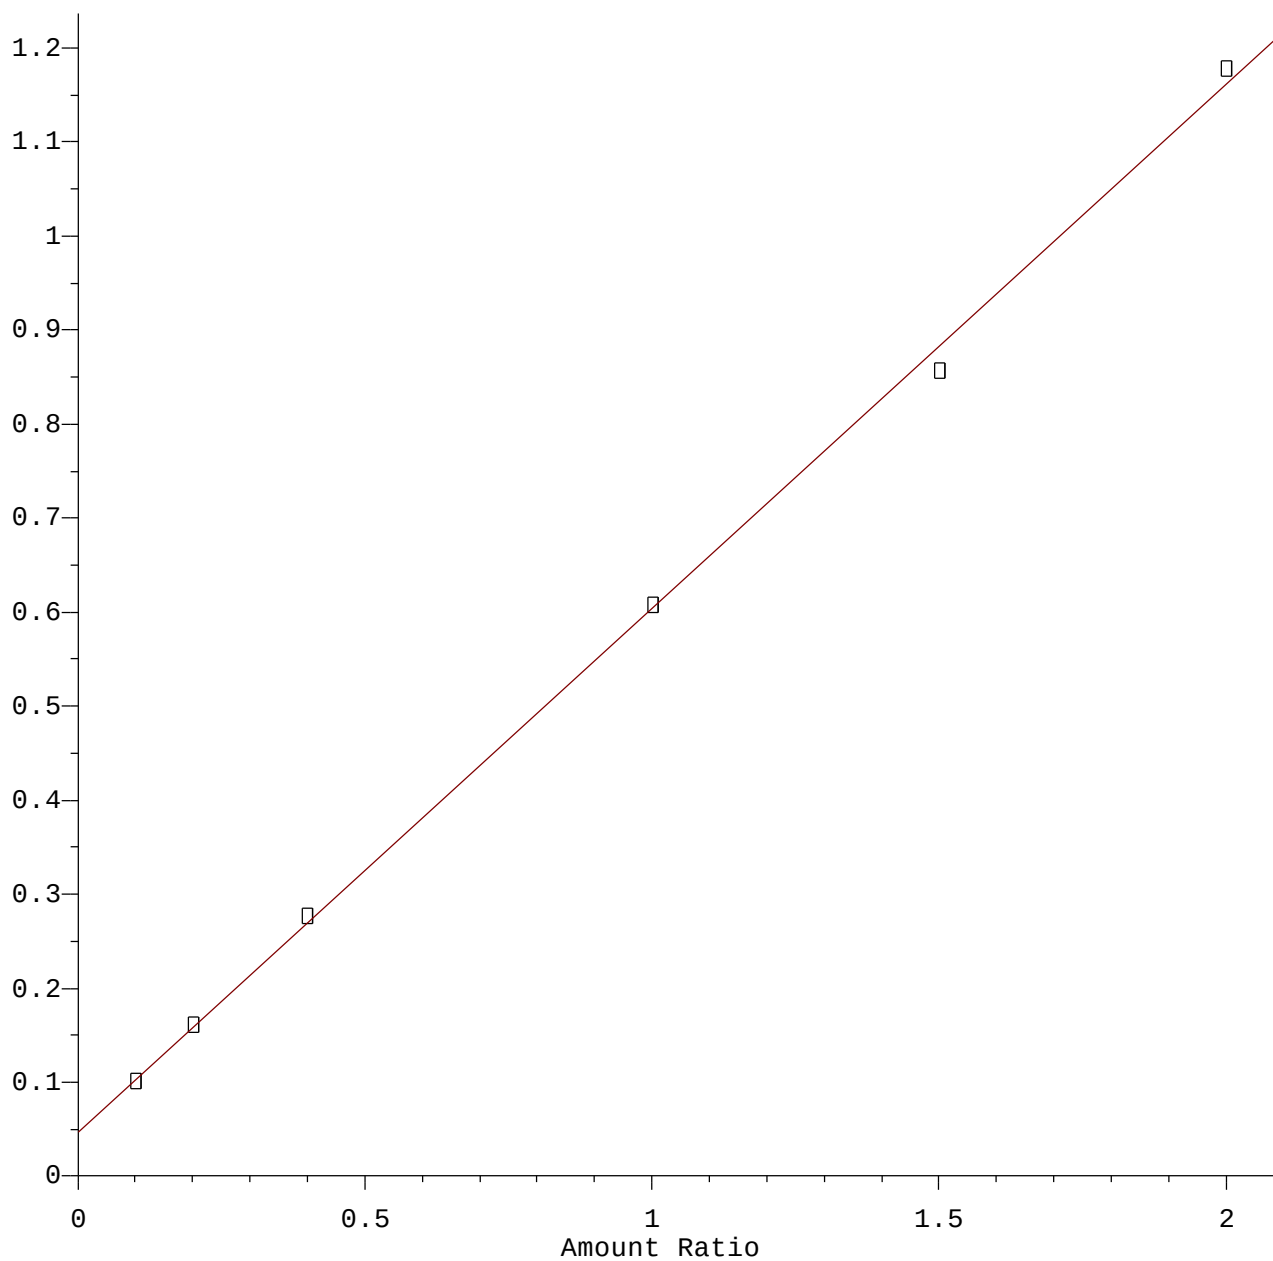


Resp Ratio = $5.57 \times 10^{-1} \times \text{Amt} + 4.68 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Calibration Table Last Updated: Fri Oct 26 02:17:41 2018

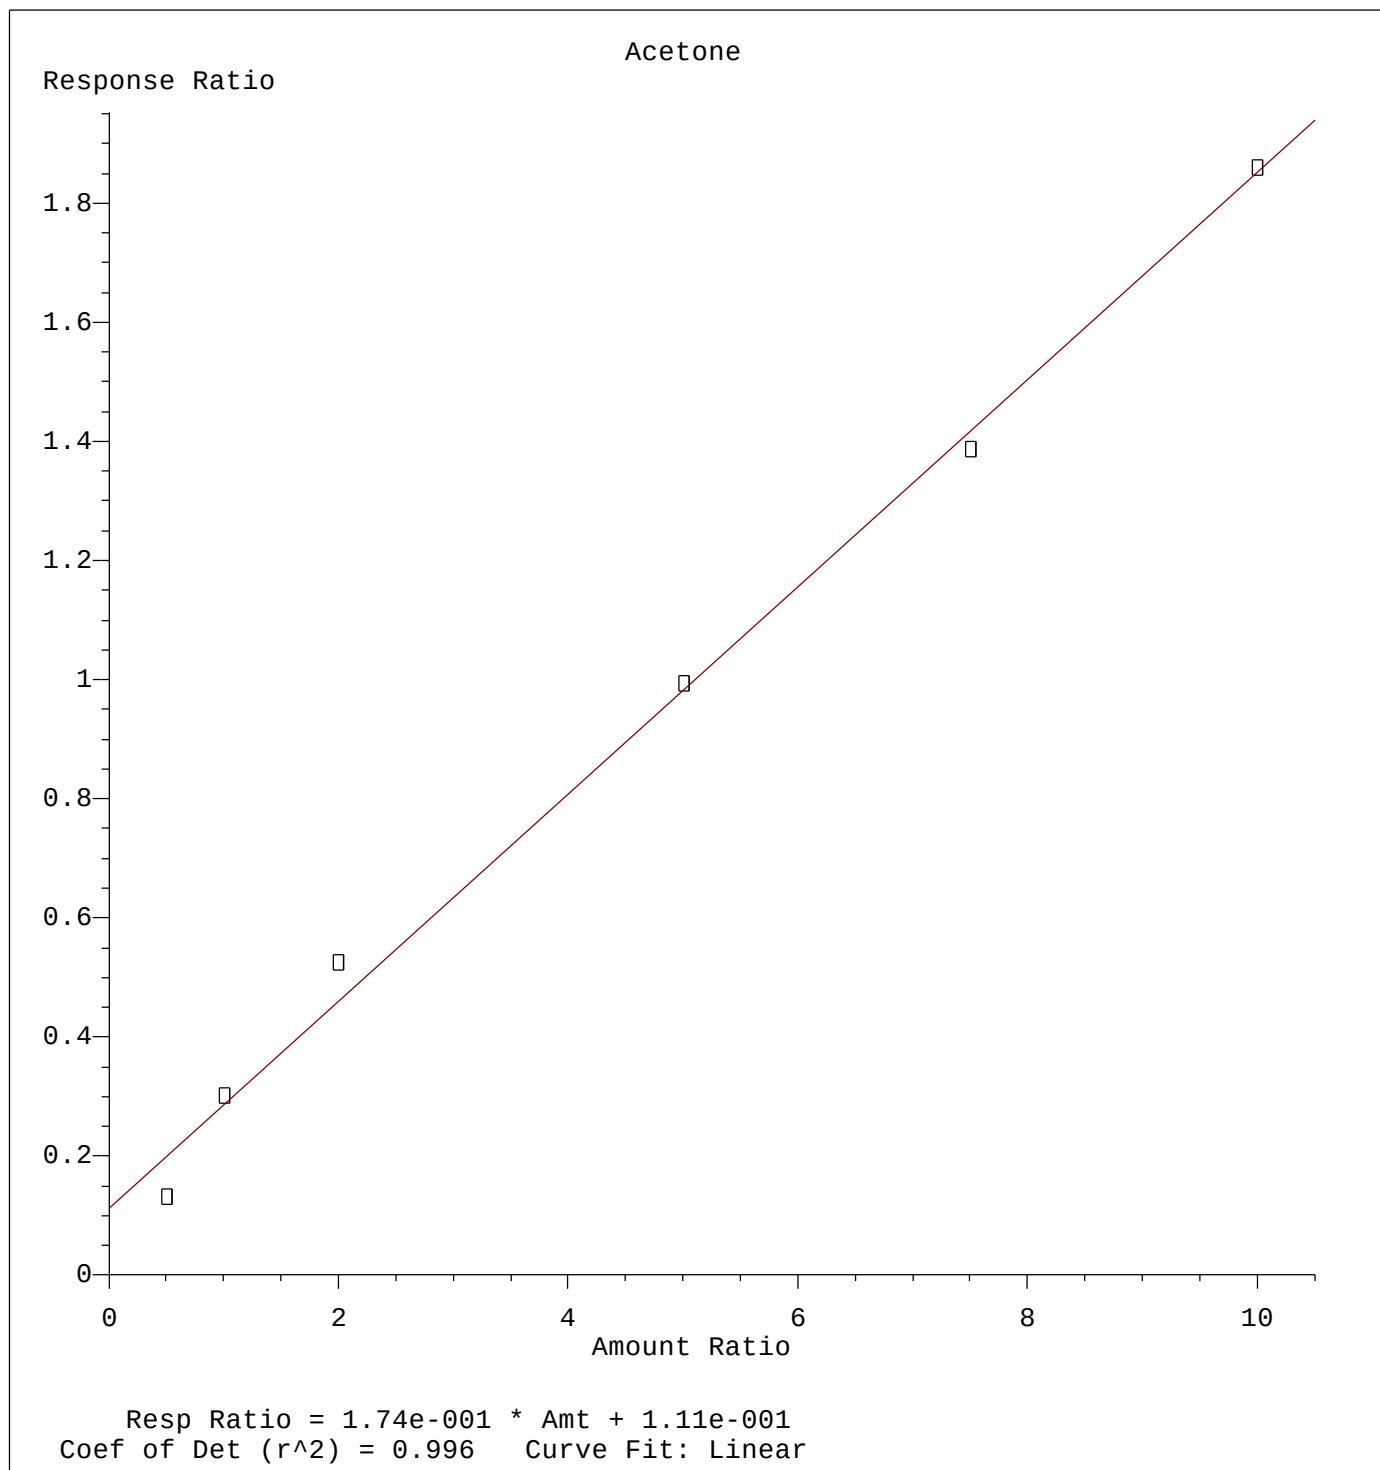


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Calibration Table Last Updated: Fri Oct 26 02:17:41 2018

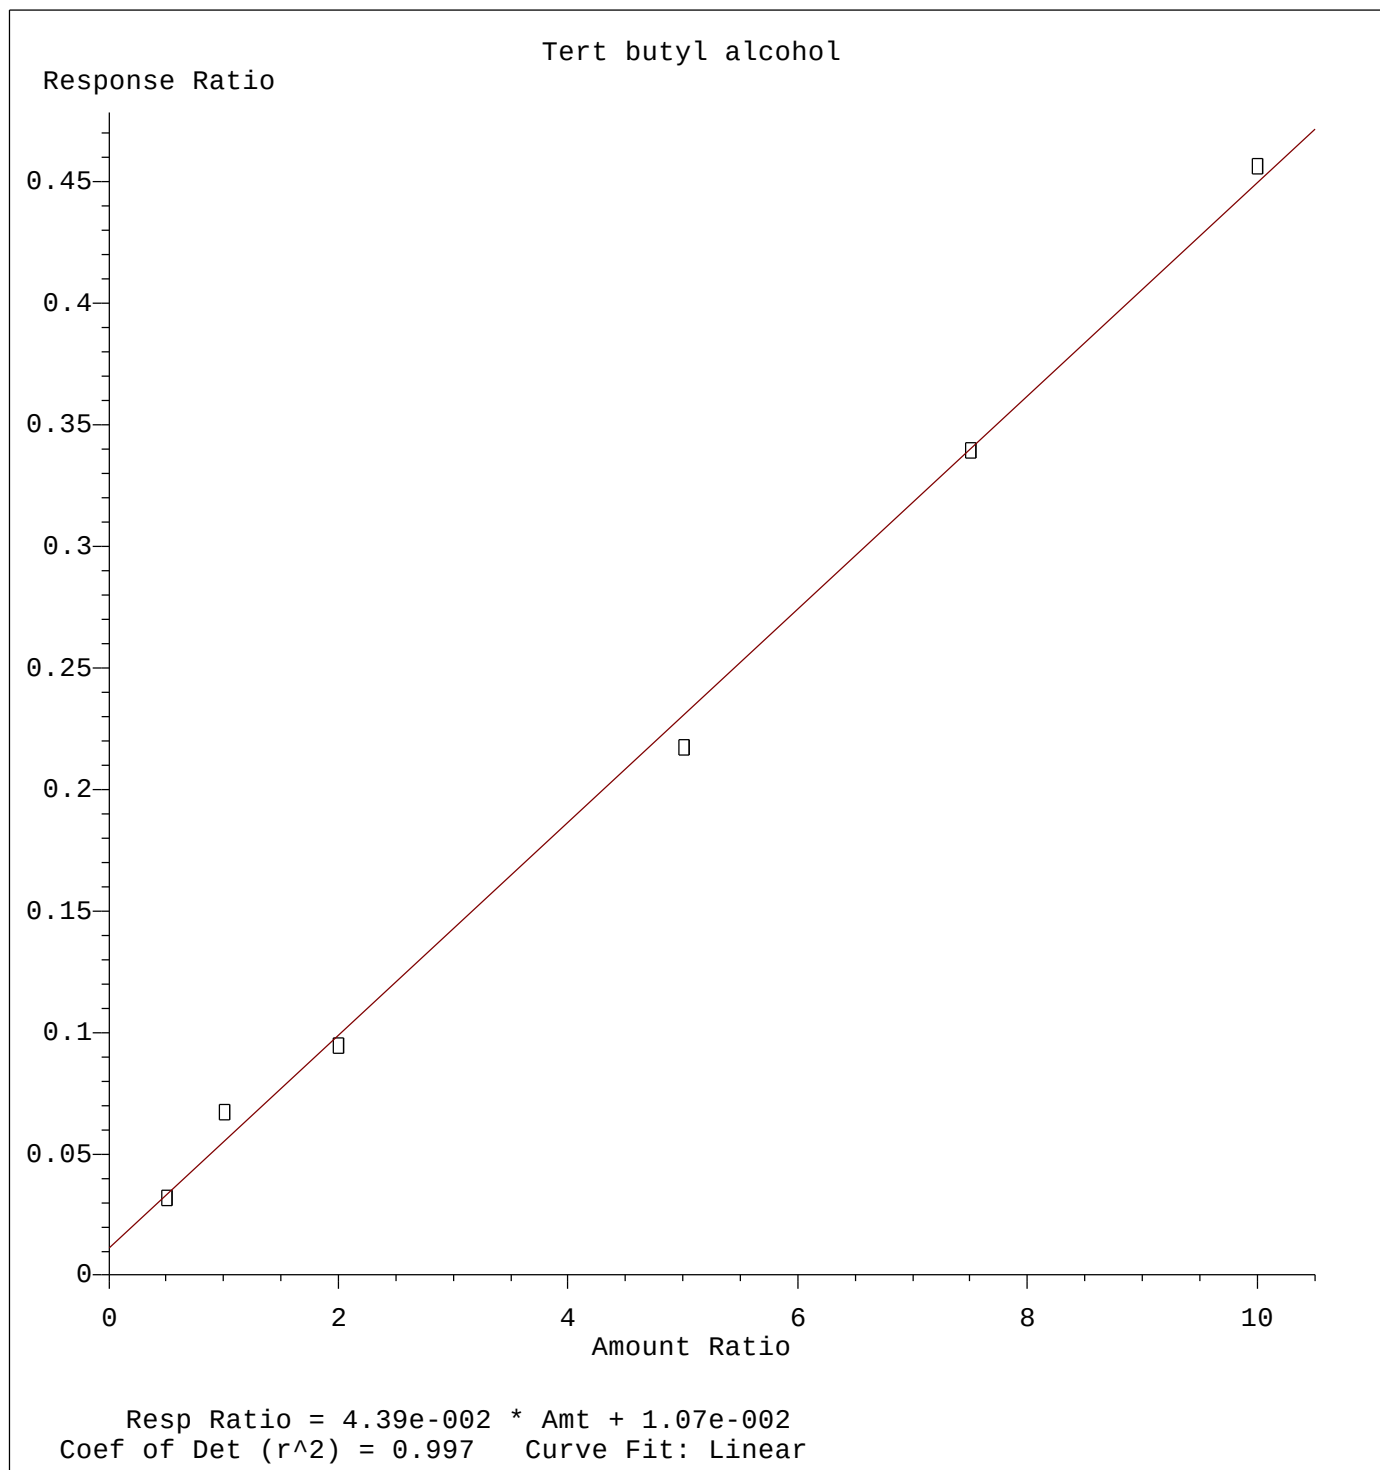

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Calibration Table Last Updated: Fri Oct 26 02:17:41 2018


2-Hexanone

Response Ratio

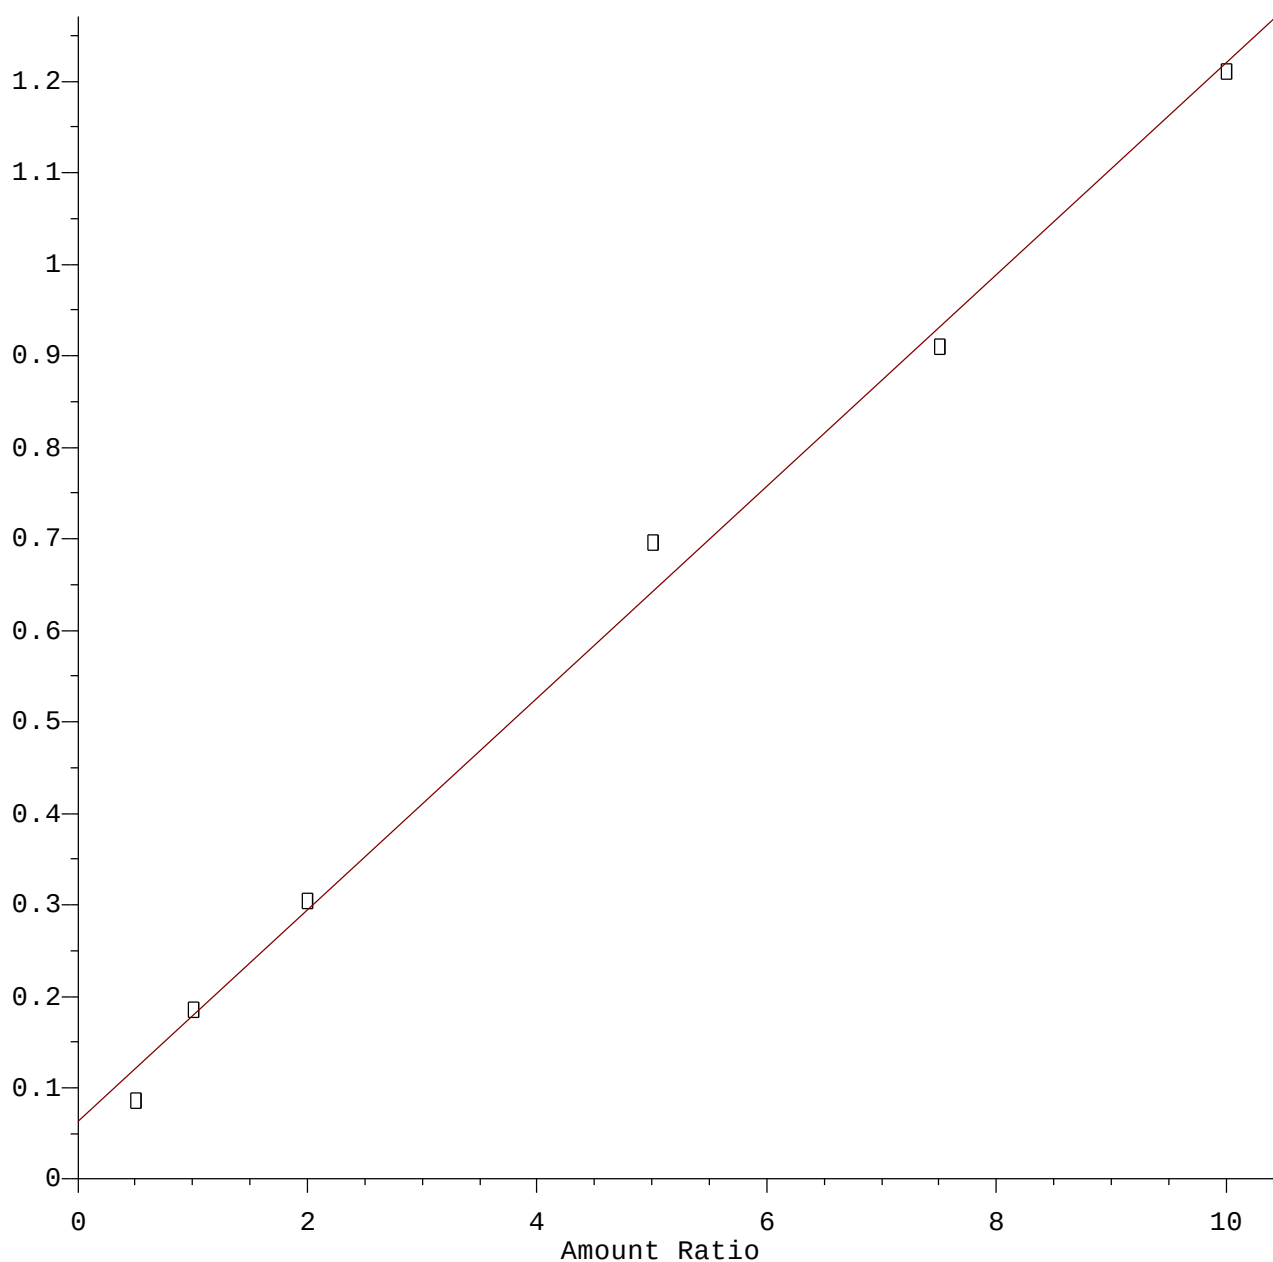

Resp Ratio = $1.16 \times 10^{-1} \times \text{Amt} + 6.30 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Calibration Table Last Updated: Fri Oct 26 02:17:41 2018

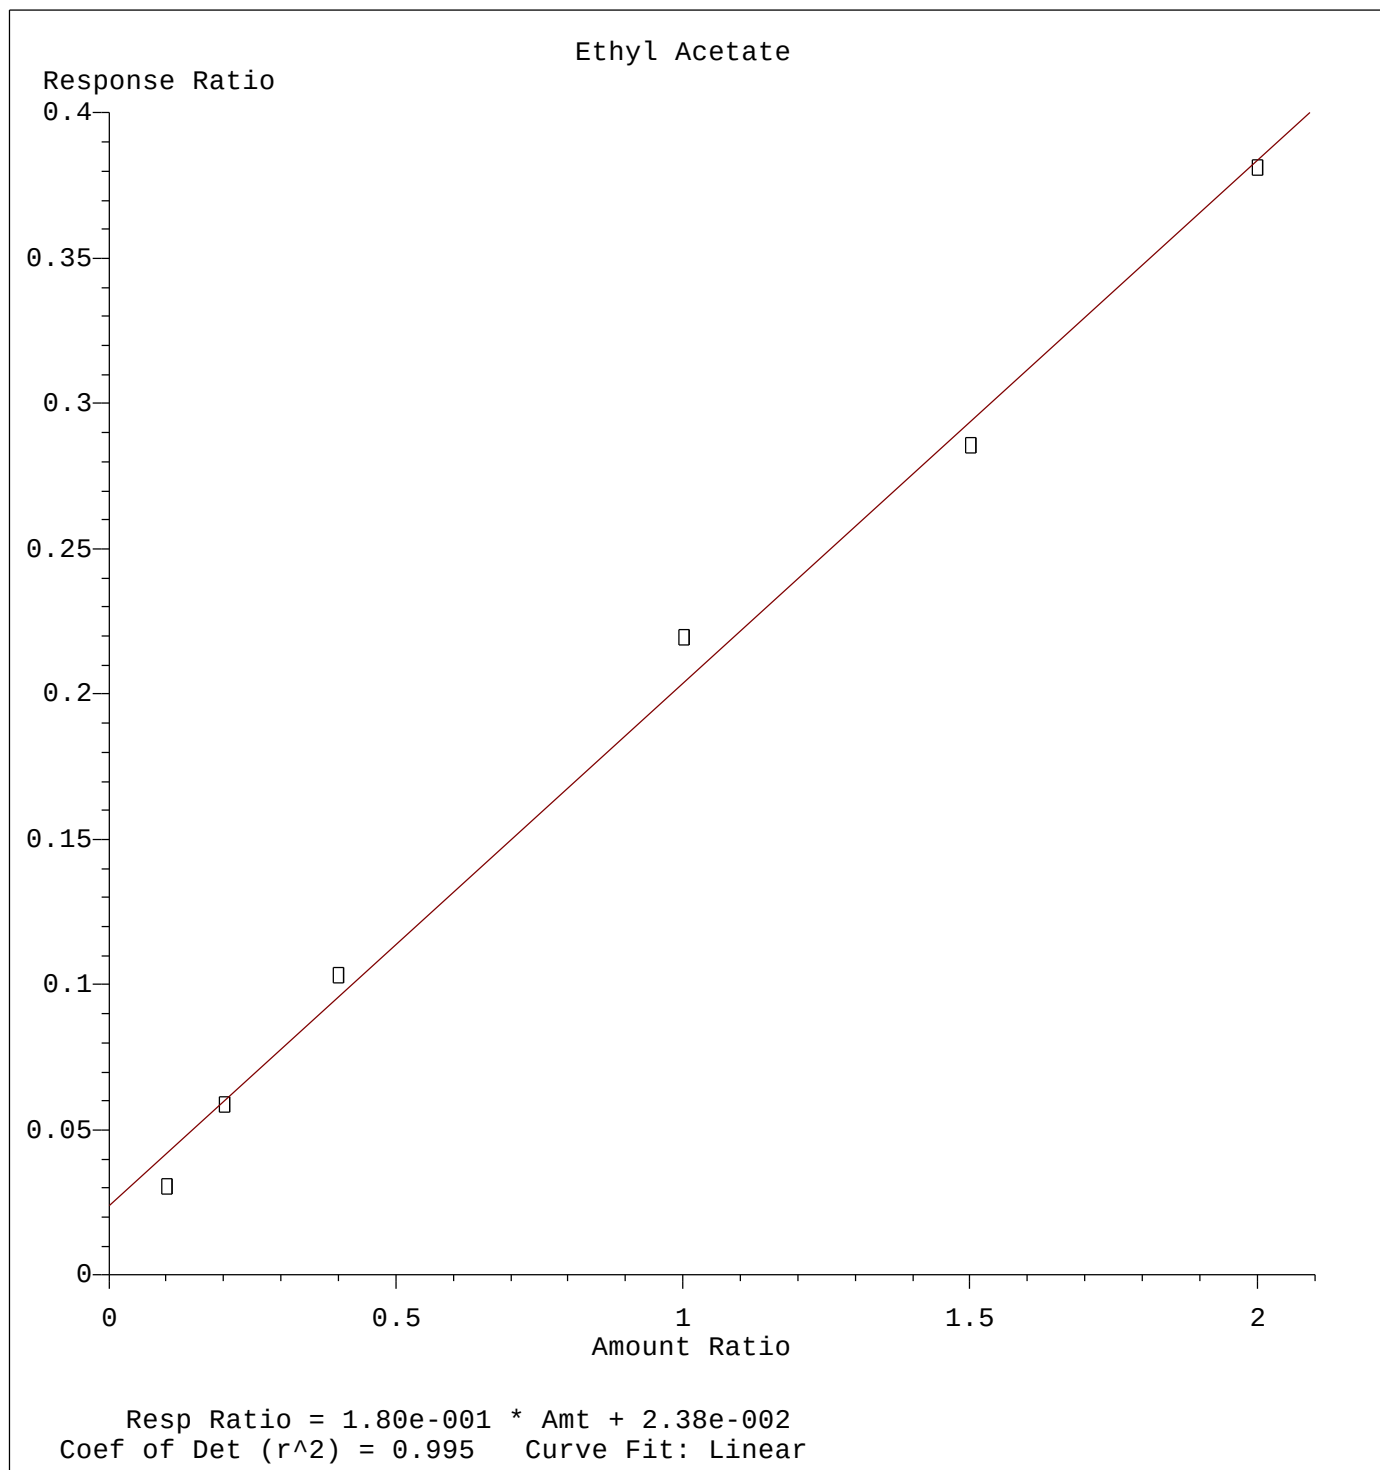

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Calibration Table Last Updated: Fri Oct 26 02:17:41 2018