


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF102518\
Data File : VF060504.D
Acq On : 25 Oct 2018 13:01
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Title : SW846 8260
Last Update : Fri Oct 26 02:17:41 2018

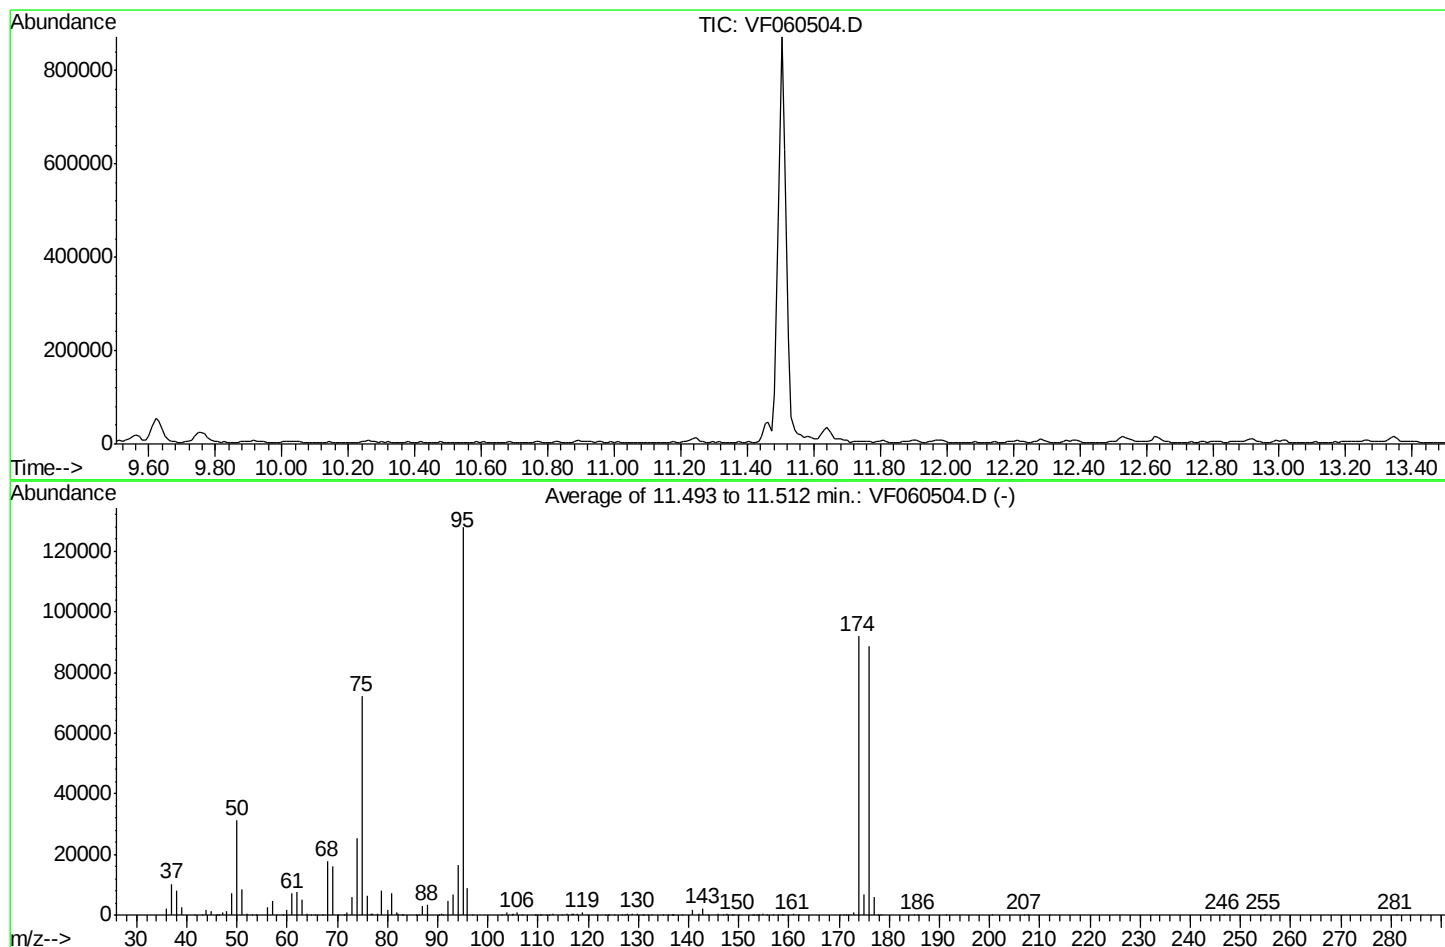

AutoFind: Scans 1102, 1103, 1104; Background Corrected with Scan 1097

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	31210	PASS
75	95	30	60	56.3	72057	PASS
95	95	100	100	100.0	127906	PASS
96	95	5	9	7.1	9086	PASS
173	174	0.00	2	0.7	662	PASS
174	95	50	100	71.9	91997	PASS
175	174	5	9	7.4	6837	PASS
176	174	95	101	96.3	88592	PASS
177	176	5	9	6.7	5902	PASS