


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF102618\
Data File : VF060513.D
Acq On : 26 Oct 2018 9:45
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA F/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102518S.M
Title : SW846 8260
Last Update : Fri Oct 26 02:17:41 2018

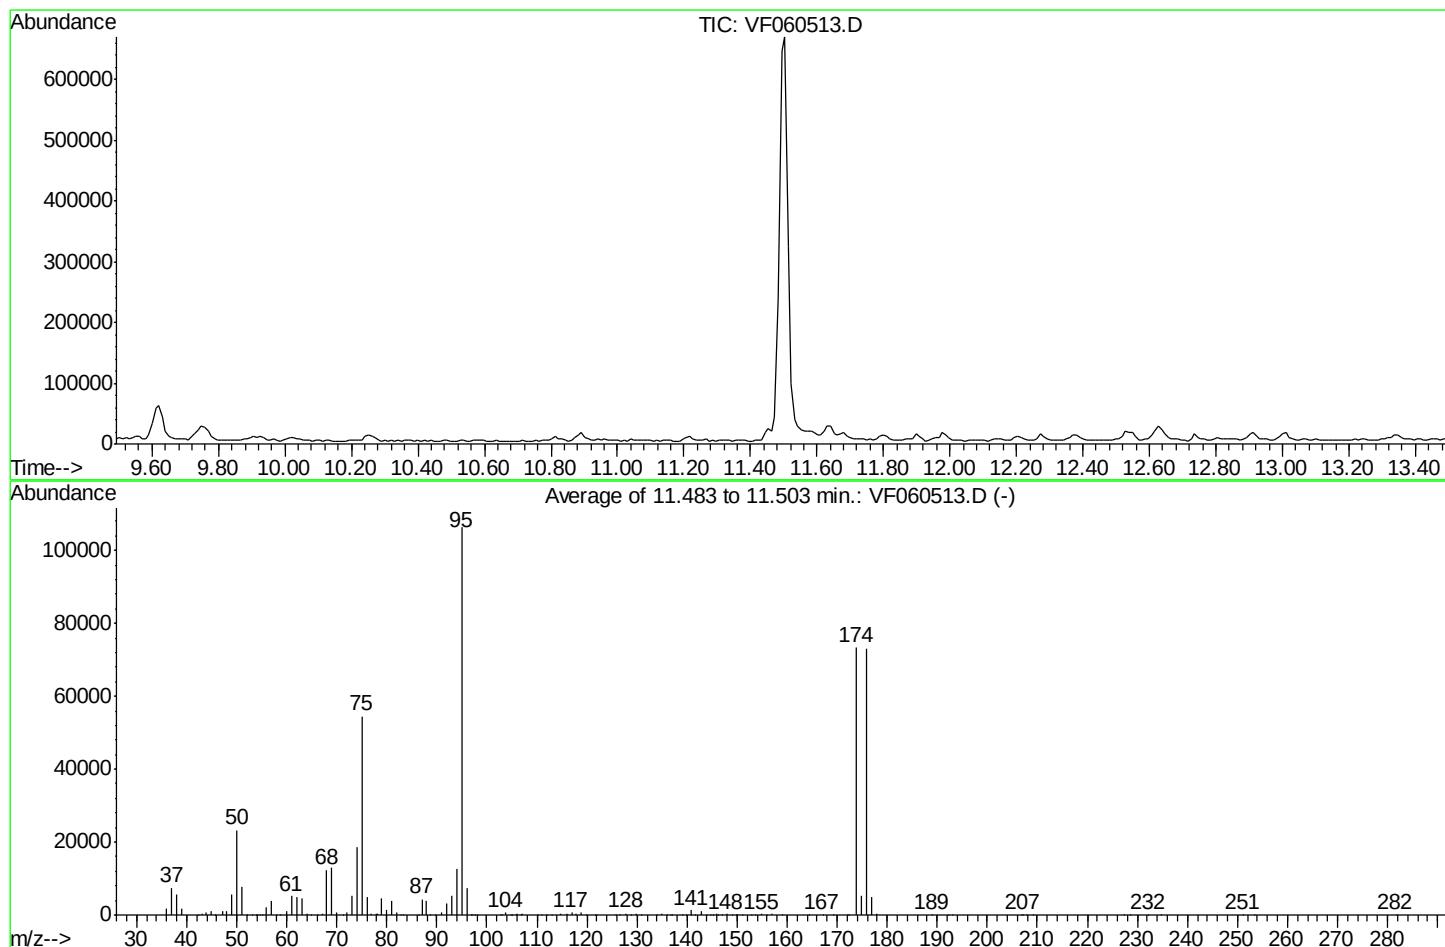

AutoFind: Scans 1101, 1102, 1103; Background Corrected with Scan 1096

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	23230	PASS
75	95	30	60	51.3	54533	PASS
95	95	100	100	100.0	106322	PASS
96	95	5	9	7.0	7438	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	68.9	73288	PASS
175	174	5	9	7.3	5329	PASS
176	174	95	101	99.7	73074	PASS
177	176	5	9	6.7	4909	PASS