


Data Path : Z:\voasrv\HPCHEM1\MSVOA_F\Data\VF103018\
 Data File : VF060539.D
 Acq On : 30 Oct 2018 9:38
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00/5mL/MSVOA_F/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F102918S.M
 Title : SW846 8260
 Last Update : Tue Oct 30 05:31:58 2018

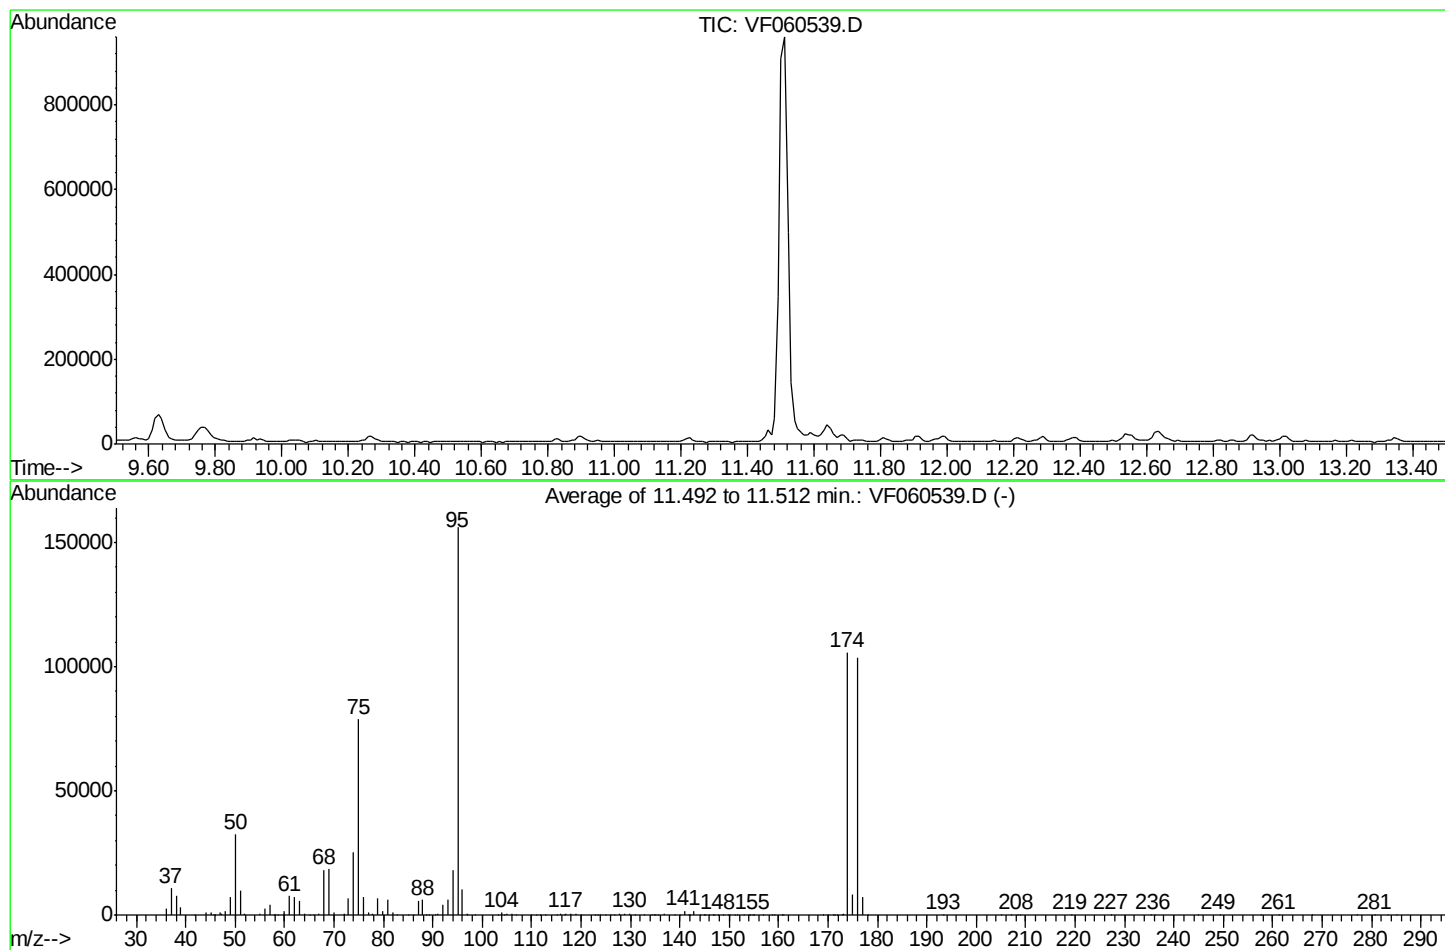

AutoFind: Scans 1102, 1103, 1104; Background Corrected with Scan 1097

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	32445	PASS
75	95	30	60	50.4	78669	PASS
95	95	100	100	100.0	156122	PASS
96	95	5	9	6.5	10119	PASS
173	174	0.00	2	0.5	490	PASS
174	95	50	100	67.6	105464	PASS
175	174	5	9	7.7	8159	PASS
176	174	95	101	98.1	103413	PASS
177	176	5	9	7.2	7458	PASS