


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF110518\
Data File : VF060567.D
Acq On : 5 Nov 2018 11:02
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F110218S.M
Title : SW846 8260
Last Update : Sat Nov 03 05:29:31 2018

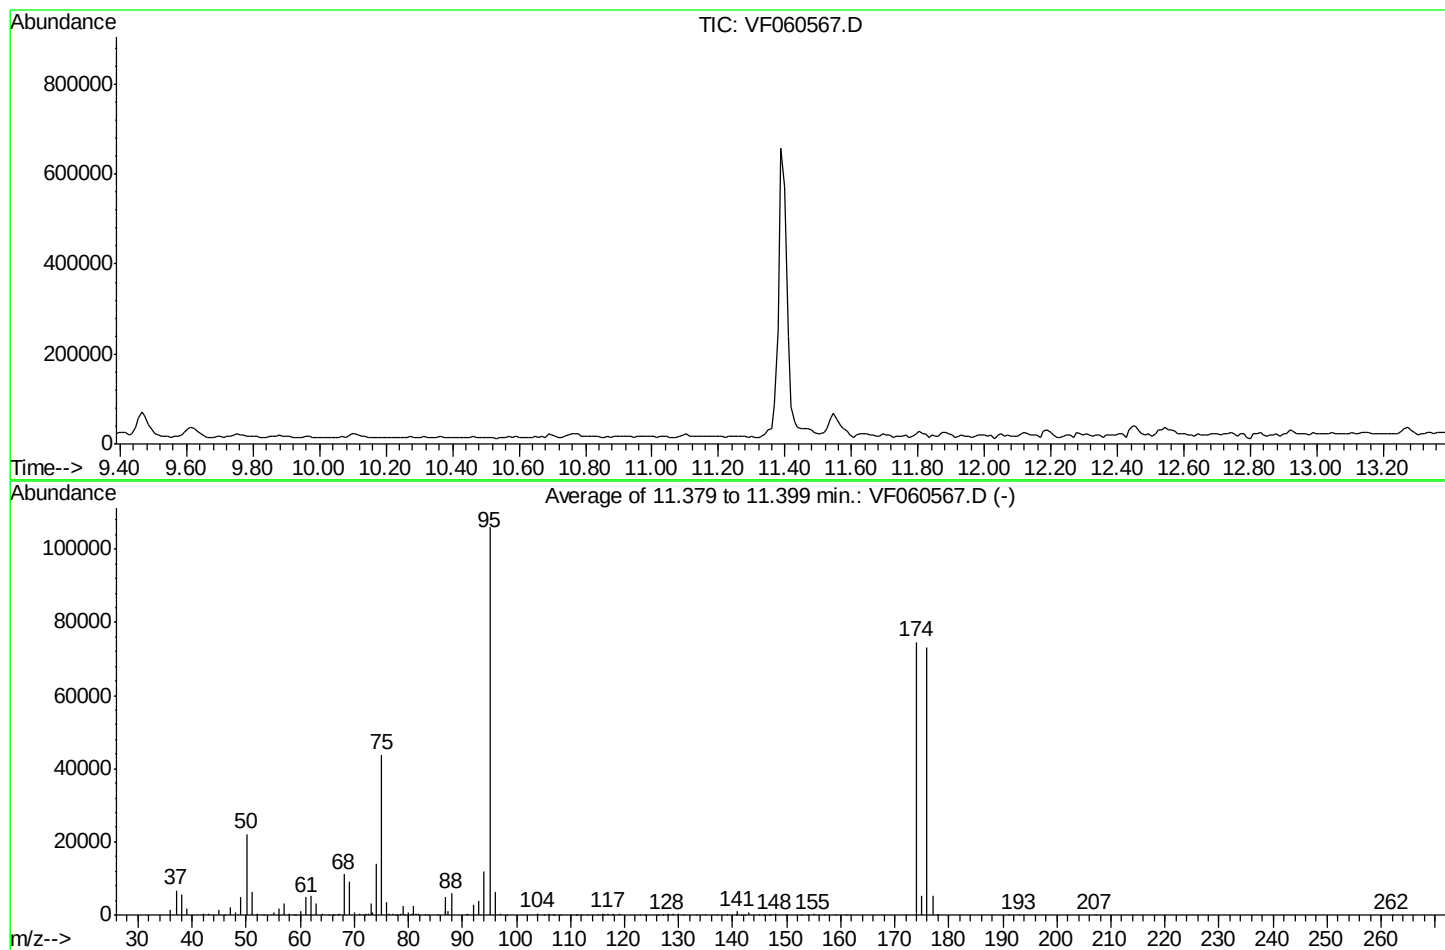

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1083

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	22136	PASS
75	95	30	60	41.3	43811	PASS
95	95	100	100	100.0	105994	PASS
96	95	5	9	5.8	6187	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.5	74714	PASS
175	174	5	9	7.1	5280	PASS
176	174	95	101	97.9	73157	PASS
177	176	5	9	7.1	5208	PASS