


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF110518\
Data File : VF060589.D
Acq On : 5 Nov 2018 23:32
Operator : VA/AP
Sample : BFB
Misc : 5.00/5mL/MSVOA-F/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F110218S.M
Title : SW846 8260
Last Update : Sat Nov 03 05:29:31 2018

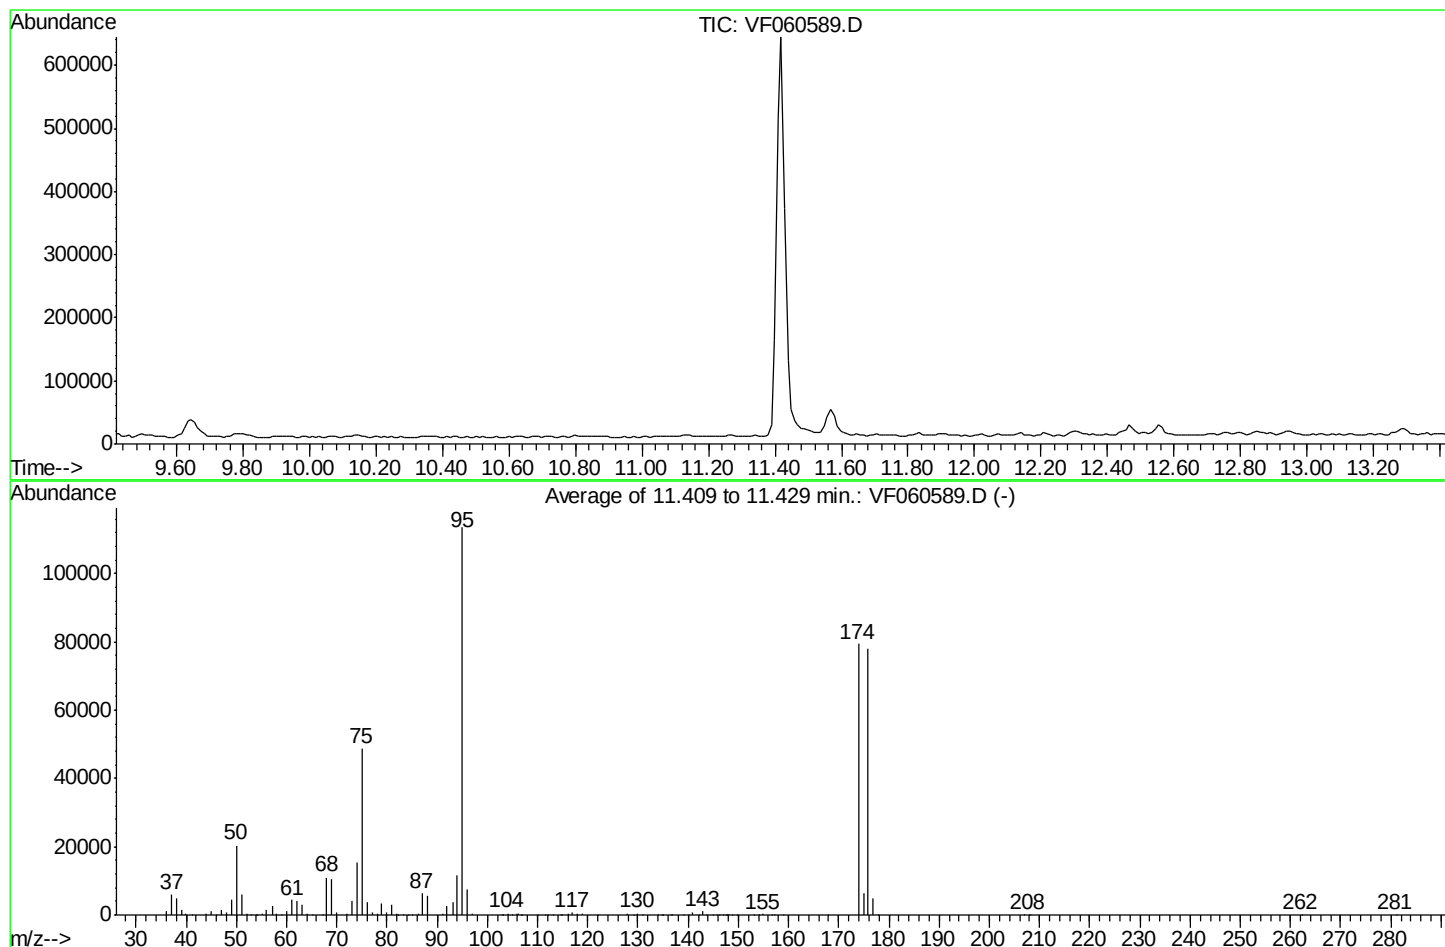

AutoFind: Scans 1093, 1094, 1095; Background Corrected with Scan 1088

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	20301	PASS
75	95	30	60	42.8	48616	PASS
95	95	100	100	100.0	113509	PASS
96	95	5	9	6.6	7531	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.9	79354	PASS
175	174	5	9	8.1	6388	PASS
176	174	95	101	98.4	78112	PASS
177	176	5	9	6.3	4938	PASS