


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF110618\
Data File : VF060609.D
Acq On : 6 Nov 2018 12:09
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F110218S.M
Title : SW846 8260
Last Update : Sat Nov 03 05:29:31 2018

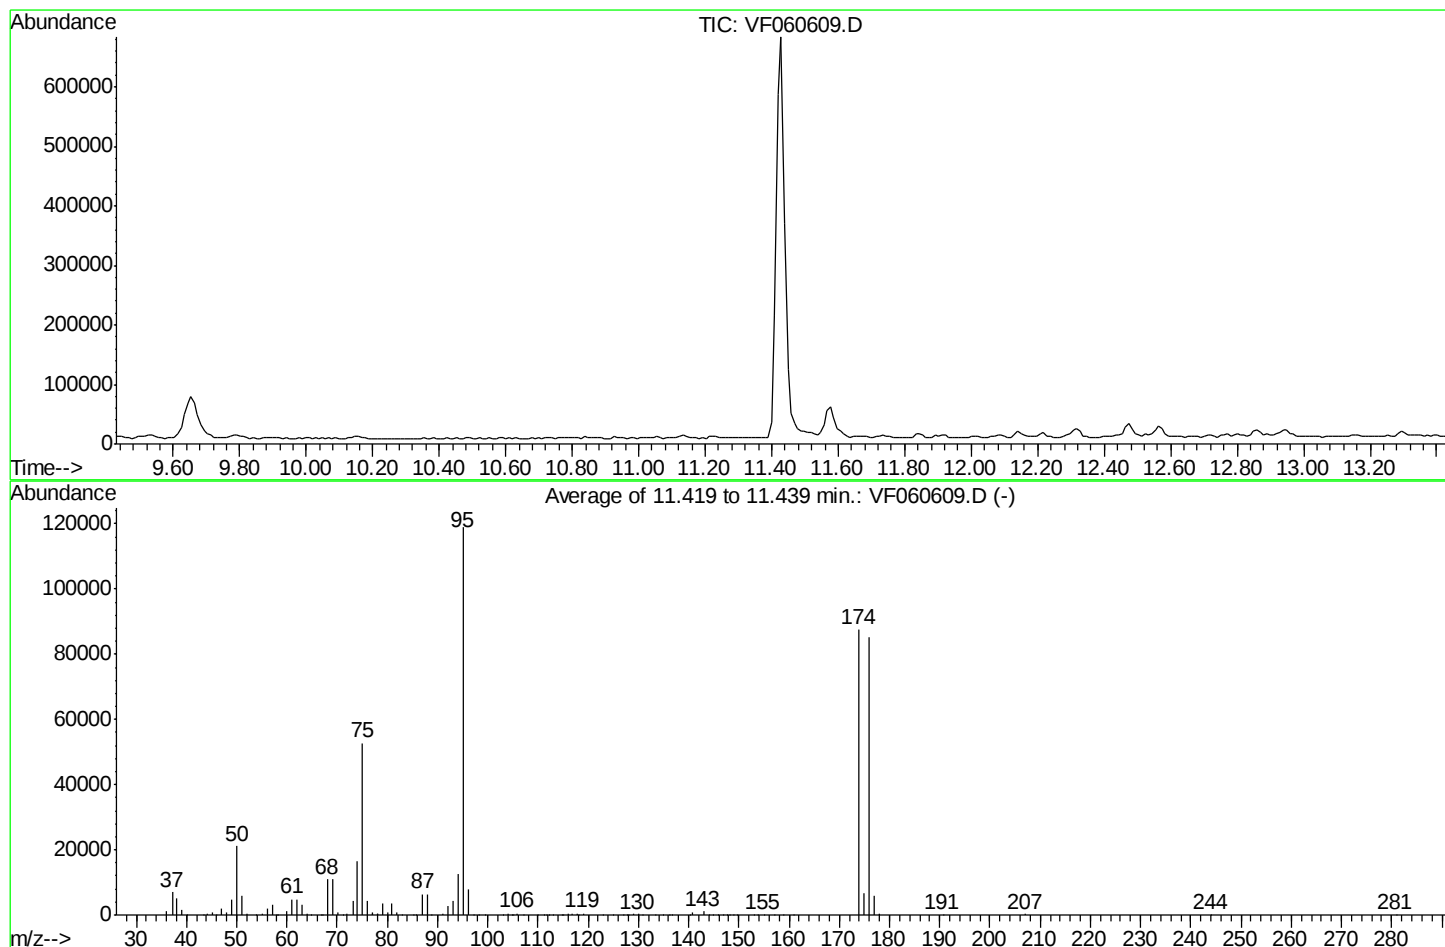

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1085

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	21031	PASS
75	95	30	60	44.4	52800	PASS
95	95	100	100	100.0	118949	PASS
96	95	5	9	6.7	7966	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.5	87437	PASS
175	174	5	9	7.4	6508	PASS
176	174	95	101	97.5	85245	PASS
177	176	5	9	7.0	5965	PASS