


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF110718\
Data File : VF060624.D
Acq On : 7 Nov 2018 10:51
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F110218S.M
Title : SW846 8260
Last Update : Sat Nov 03 05:29:31 2018

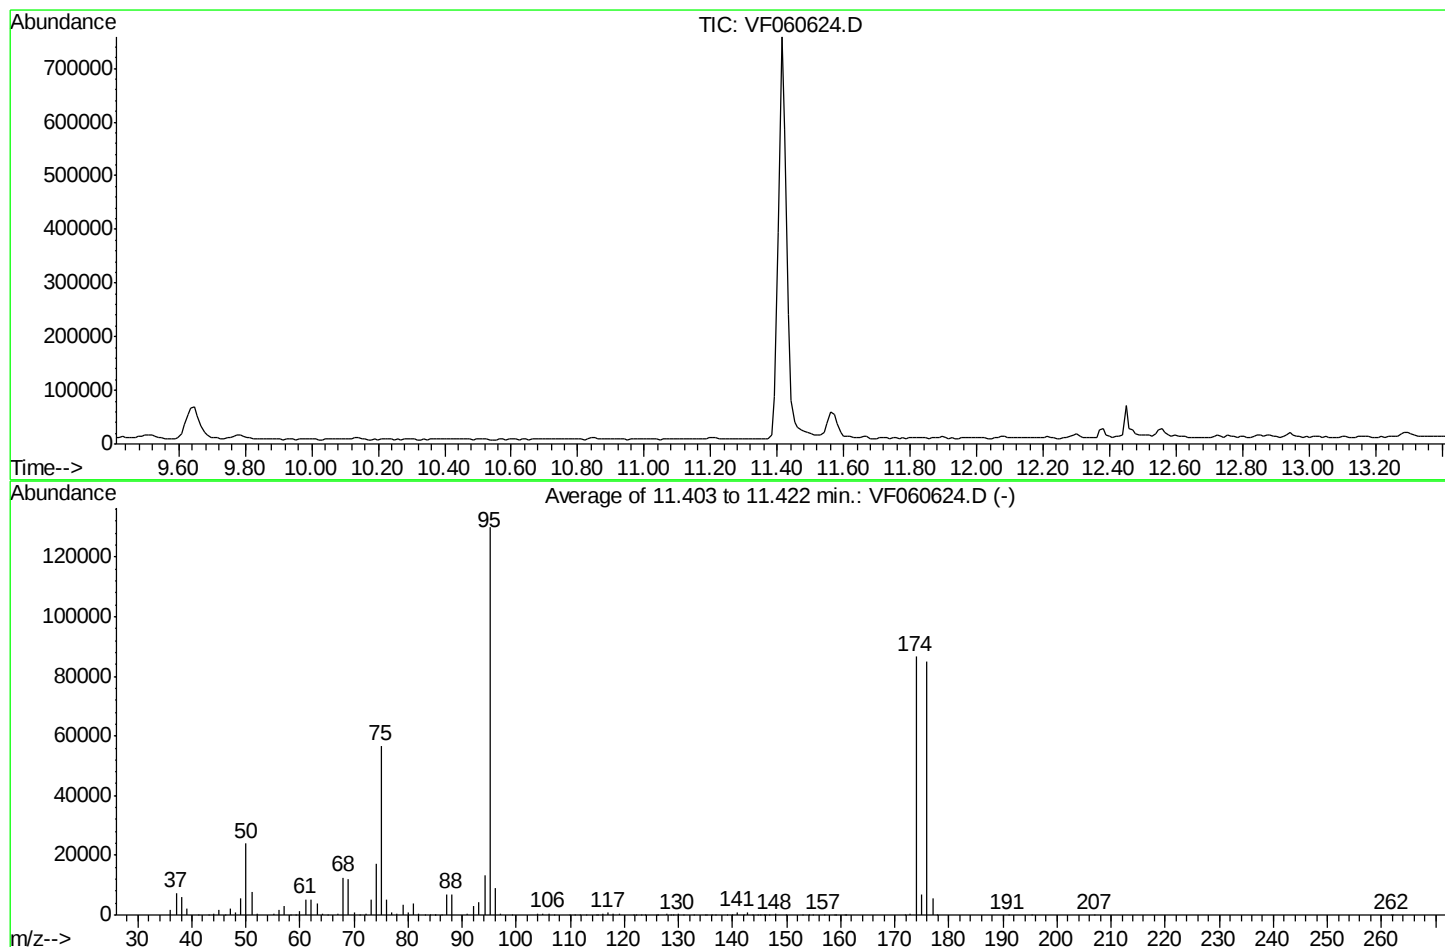

AutoFind: Scans 1092, 1093, 1094; Background Corrected with Scan 1087

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	23856	PASS
75	95	30	60	43.7	56840	PASS
95	95	100	100	100.0	129946	PASS
96	95	5	9	6.8	8839	PASS
173	174	0.00	2	0.3	244	PASS
174	95	50	100	66.6	86584	PASS
175	174	5	9	8.0	6943	PASS
176	174	95	101	97.9	84765	PASS
177	176	5	9	6.6	5621	PASS