


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF110818\
 Data File : VF060645.D
 Acq On : 8 Nov 2018 10:47
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F110218S.M
 Title : SW846 8260
 Last Update : Sat Nov 03 05:29:31 2018

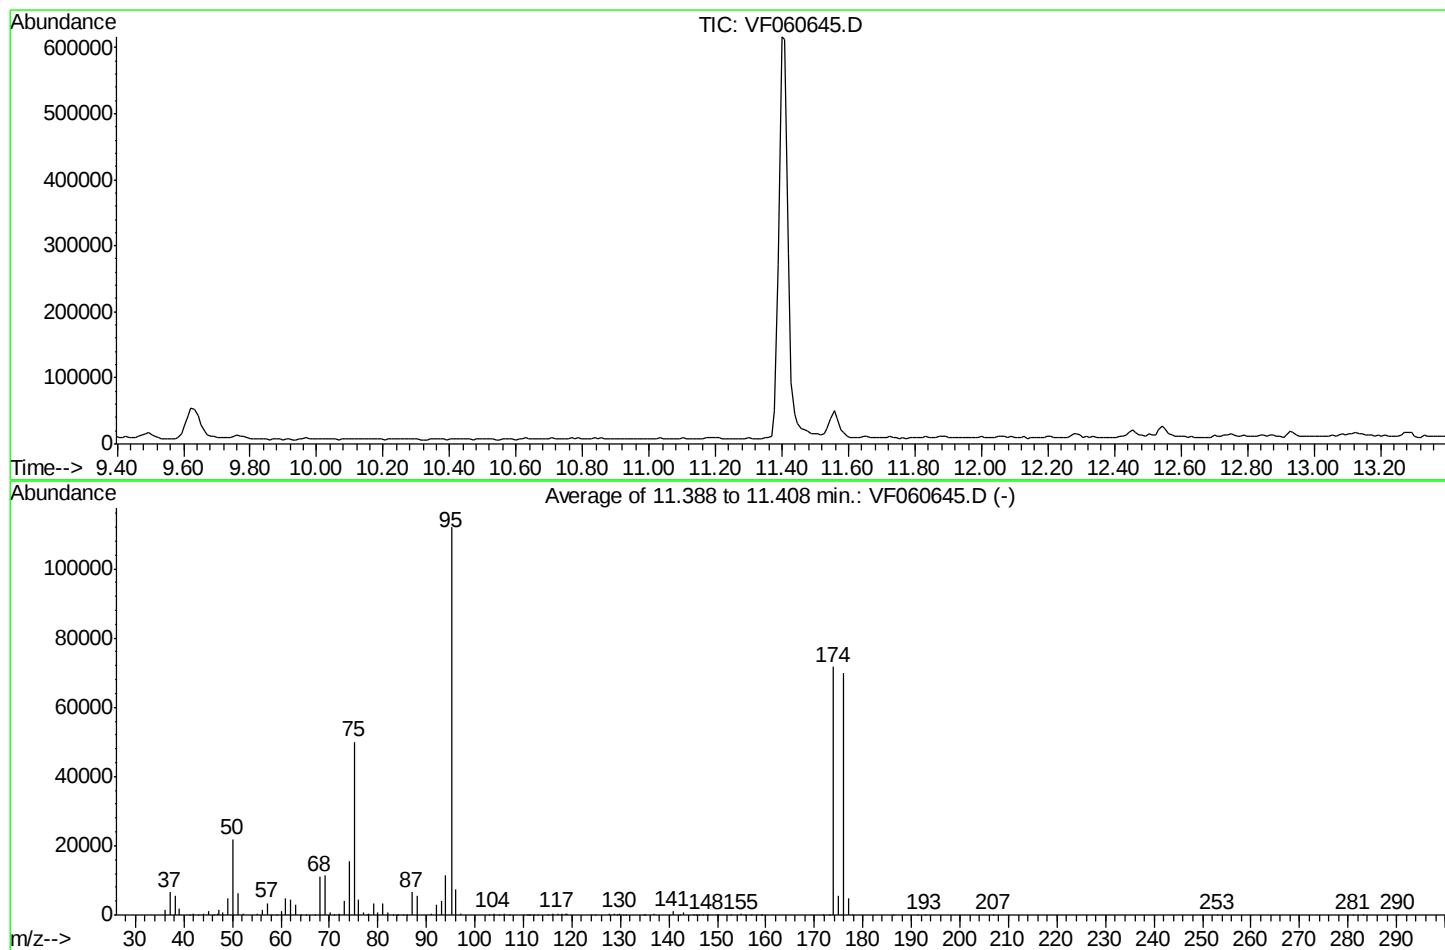

AutoFind: Scans 1091, 1092, 1093; Background Corrected with Scan 1084

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	21730	PASS
75	95	30	60	44.7	50090	PASS
95	95	100	100	100.0	111960	PASS
96	95	5	9	6.7	7530	PASS
173	174	0.00	2	0.1	84	PASS
174	95	50	100	64.0	71602	PASS
175	174	5	9	7.9	5677	PASS
176	174	95	101	97.7	69954	PASS
177	176	5	9	6.9	4842	PASS