


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF111218\
 Data File : VF060688.D
 Acq On : 12 Nov 2018 13:34
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F110218S.M
 Title : SW846 8260
 Last Update : Sat Nov 03 05:29:31 2018

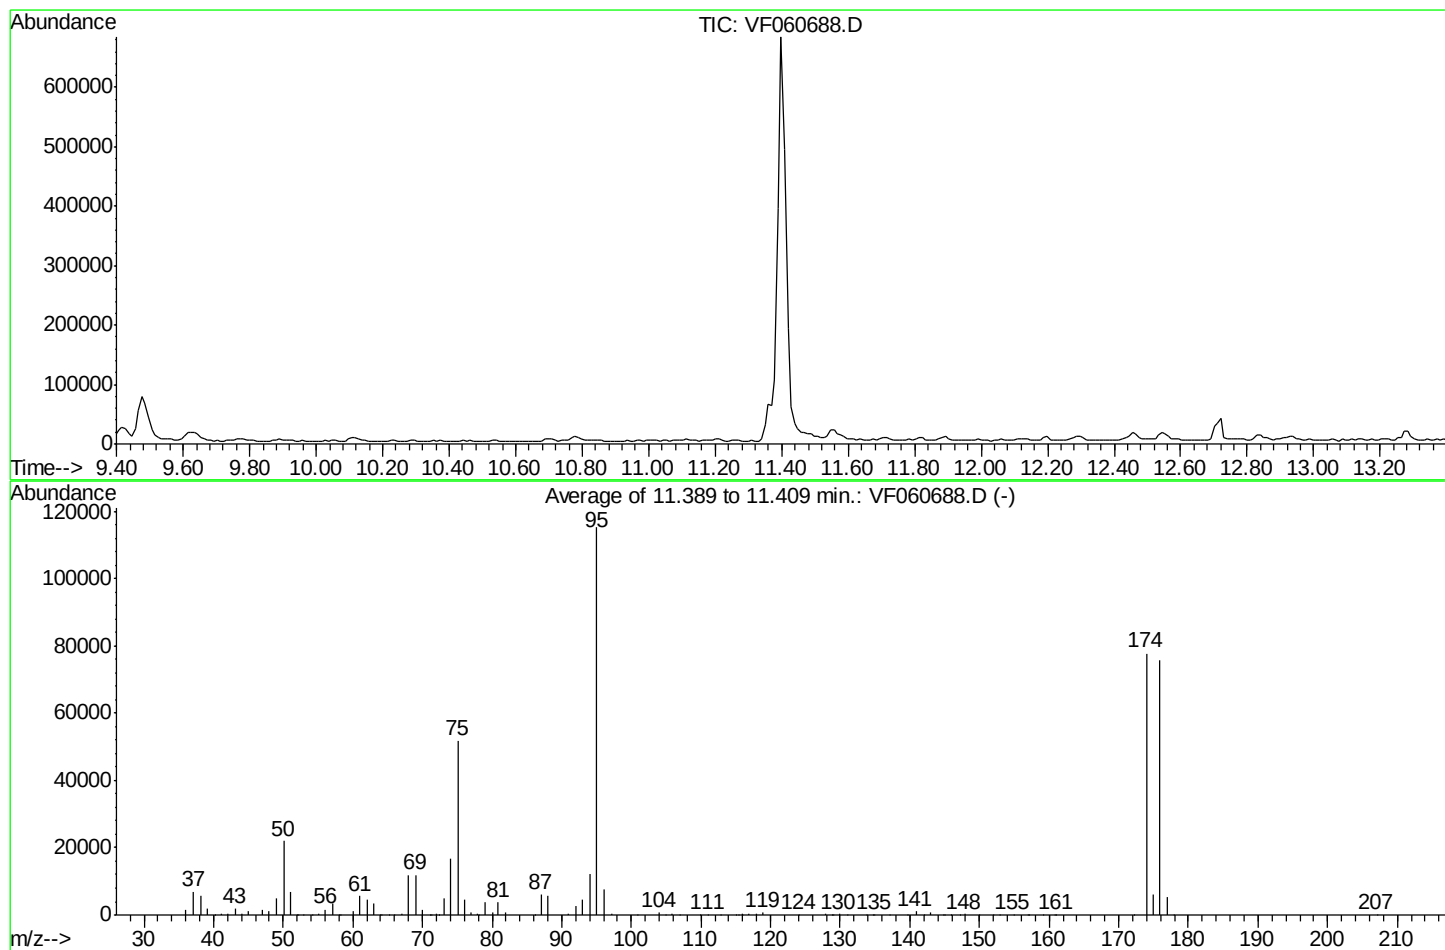

AutoFind: Scans 1091, 1092, 1093; Background Corrected with Scan 1085

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	21920	PASS
75	95	30	60	45.0	51890	PASS
95	95	100	100	100.0	115245	PASS
96	95	5	9	6.7	7722	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.5	77802	PASS
175	174	5	9	7.7	5965	PASS
176	174	95	101	97.2	75597	PASS
177	176	5	9	7.0	5257	PASS