


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF111318\
Data File : VF060706.D
Acq On : 13 Nov 2018 11:03
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F111318S.M
Title : SW846 8260
Last Update : Wed Nov 14 03:11:14 2018

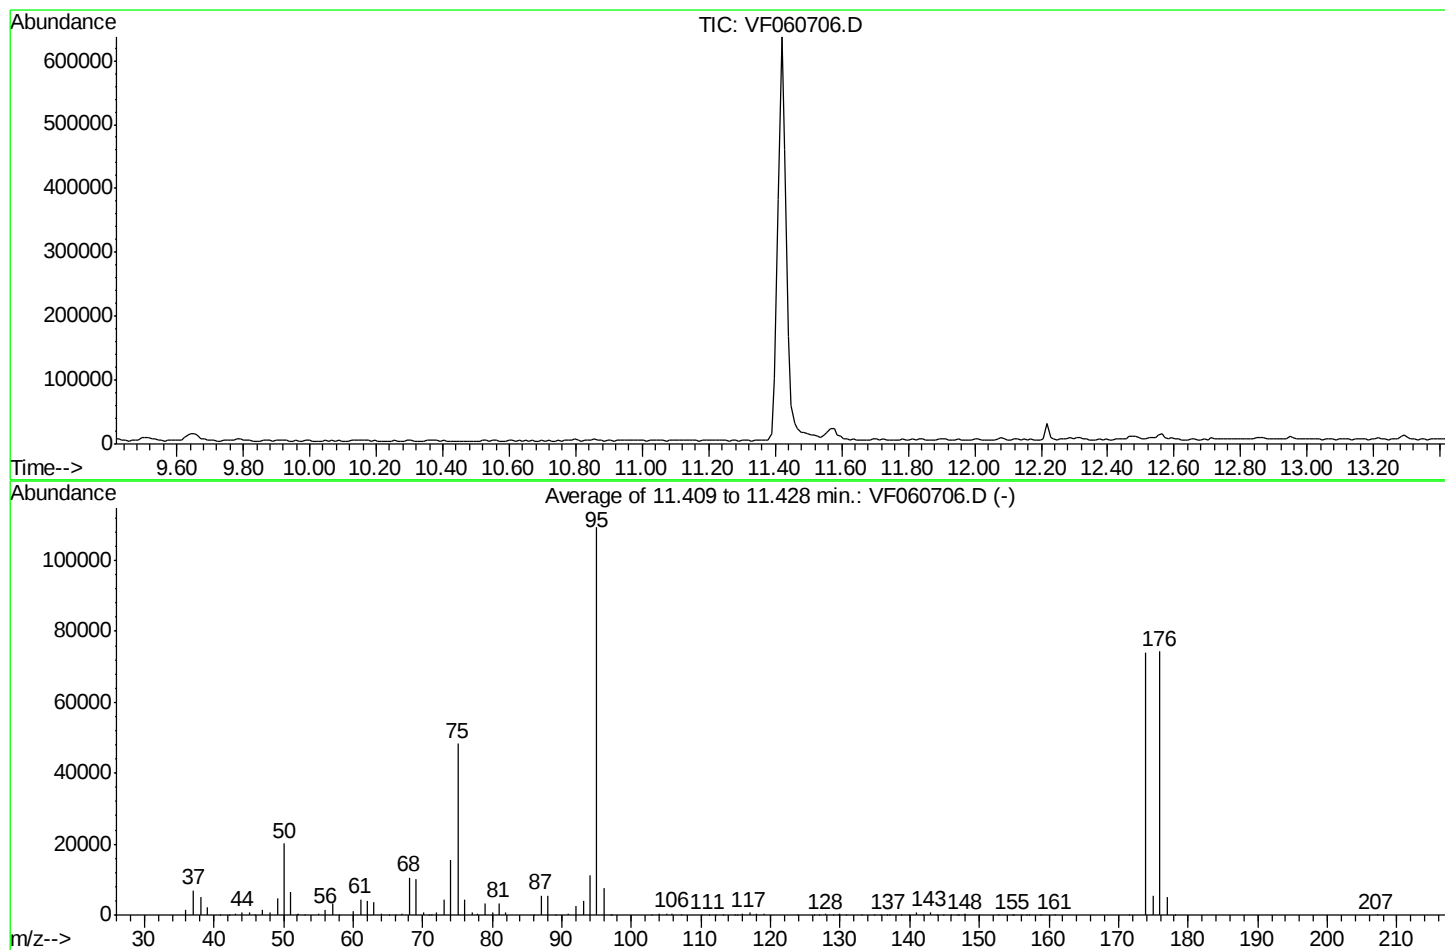

AutoFind: Scans 1093, 1094, 1095; Background Corrected with Scan 1088

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	20169	PASS
75	95	30	60	44.2	48360	PASS
95	95	100	100	100.0	109338	PASS
96	95	5	9	6.8	7452	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.7	74040	PASS
175	174	5	9	7.5	5541	PASS
176	174	95	101	100.2	74218	PASS
177	176	5	9	7.0	5204	PASS