


Data Path : Z:\voasrv\HPCHEM1\MSVOA_F\Data\VF111418\
 Data File : VF060719.D
 Acq On : 14 Nov 2018 9:42
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F111318S.M
 Title : SW846 8260
 Last Update : Wed Nov 14 03:11:14 2018

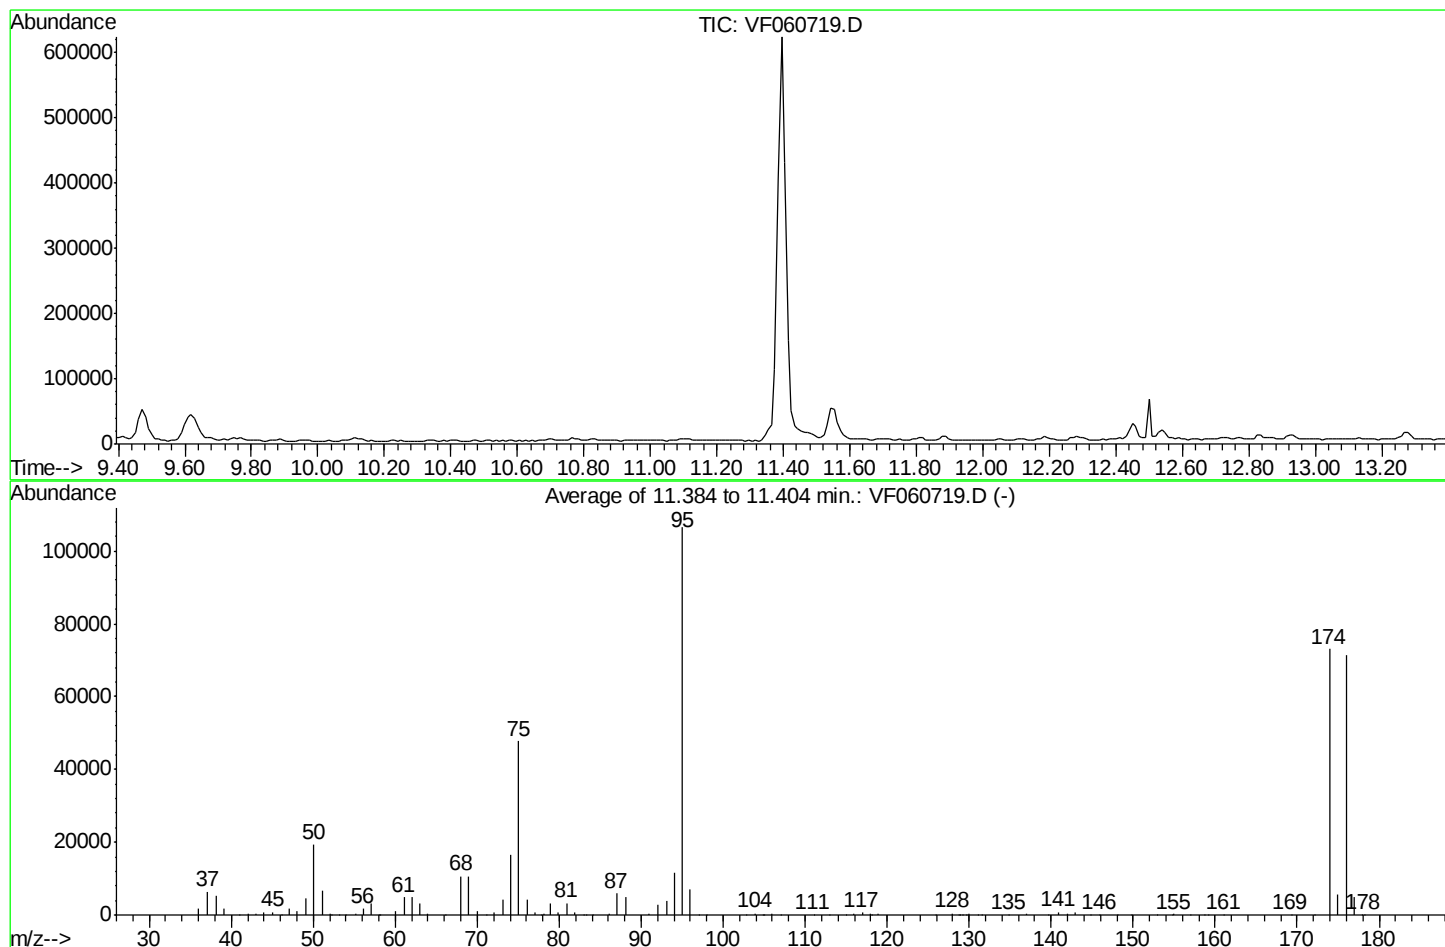

AutoFind: Scans 1090, 1091, 1092; Background Corrected with Scan 1084

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	19311	PASS
75	95	30	60	44.8	47765	PASS
95	95	100	100	100.0	106538	PASS
96	95	5	9	6.7	7157	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	68.6	73048	PASS
175	174	5	9	8.0	5809	PASS
176	174	95	101	97.6	71285	PASS
177	176	5	9	7.1	5088	PASS