

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF111518\
 Data File : VF060752.D
 Acq On : 15 Nov 2018 17:48
 Operator : VA/AP
 Sample : J5942-01
 Misc : 6.38g/5mL/MSVOA-F/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 VW-D1

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F111318S.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.064	40	44	46	rBV3	4519	10379	2.64%	0.384%
2	1.202	56	58	59	rVV2	3431	5854	1.49%	0.216%
3	1.271	63	65	66	rVV2	3370	4741	1.21%	0.175%
4	1.310	66	69	72	rVV4	3378	8167	2.08%	0.302%
5	1.379	74	76	78	rVB3	2792	4053	1.03%	0.150%
6	1.764	114	115	117	rBV2	4613	6234	1.59%	0.231%
7	1.922	129	131	134	rBV3	2602	5638	1.44%	0.208%
8	2.119	147	151	152	rBV3	2663	5079	1.29%	0.188%
9	2.178	152	157	159	rBV5	7775	19438	4.95%	0.719%
10	2.770	216	217	221	rBV4	3022	6964	1.77%	0.258%
11	2.819	221	222	226	rVB4	3371	4695	1.20%	0.174%
12	3.046	244	245	253	rVB	11720	18454	4.70%	0.682%
13	3.855	318	327	332	rBV2	5965	19718	5.02%	0.729%
14	3.993	337	341	342	rVV3	3255	6764	1.72%	0.250%
15	4.102	345	352	361	rVV2	44226	154224	39.29%	5.703%
16	4.625	399	405	408	rBV4	3264	7946	2.02%	0.294%
17	4.851	421	428	435	rBV2	114363	391795	99.80%	14.488%
18	5.404	480	484	486	rBV4	1715	4116	1.05%	0.152%
19	5.591	494	503	513	rBV	128089	362844	92.43%	13.417%
20	5.937	536	538	541	rBV4	1736	4141	1.05%	0.153%
21	7.544	696	701	706	rVV	138545	341656	87.03%	12.634%
22	7.613	706	708	717	rVB	23207	48771	12.42%	1.803%
23	8.205	764	768	771	rBV4	2493	6445	1.64%	0.238%
24	8.265	771	774	777	rVB4	2146	4152	1.06%	0.154%
25	9.488	895	898	903	rVB4	2279	4893	1.25%	0.181%
26	9.764	920	926	935	rBV	170429	392575	100.00%	14.517%
27	9.882	937	938	943	rVB3	2706	4587	1.17%	0.170%
28	10.129	959	963	965	rBV5	3077	6218	1.58%	0.230%
29	10.671	1015	1018	1019	rBV3	2772	4065	1.04%	0.150%
30	10.780	1024	1029	1031	rVV4	3230	5983	1.52%	0.221%
31	10.859	1034	1037	1040	rVB3	1796	4048	1.03%	0.150%
32	11.401	1088	1092	1101	rBV	119349	216443	55.13%	8.004%
33	11.559	1105	1108	1111	rBV3	4933	7680	1.96%	0.284%
34	11.707	1122	1123	1128	rVB4	4562	6311	1.61%	0.233%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_F\DATA\VF111518\
Data File : VF060752.D
Acq On : 15 Nov 2018 17:48
Operator : VA/AP
Sample : J5942-01
Misc : 6.38g/5mL/MSVOA-F/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
VW-D1

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F111318S.M
Title : SW846 8260

35	12.200	1170	1173	1176	rVB3	4715	7551	1.92%	0.279%
36	12.546	1204	1208	1216	rVV	217735	330976	84.31%	12.239%
37	12.703	1221	1224	1226	rBV2	4487	8059	2.05%	0.298%
38	12.812	1231	1235	1236	rVV3	2423	4925	1.25%	0.182%
39	12.930	1243	1247	1251	rBV5	2196	5960	1.52%	0.220%
40	12.999	1251	1254	1259	rBV5	5245	10338	2.63%	0.382%
41	13.285	1281	1283	1286	rVB2	3010	5381	1.37%	0.199%
42	13.710	1322	1326	1328	rBV3	6213	10207	2.60%	0.377%
43	13.867	1340	1342	1345	rVV3	3790	5027	1.28%	0.186%
44	13.956	1349	1351	1354	rBV3	2486	4992	1.27%	0.185%
45	14.084	1361	1364	1368	rBV3	9753	16753	4.27%	0.620%
46	14.163	1371	1372	1373	rBV	16535	10609	2.70%	0.392%
47	14.203	1373	1376	1378	rVV2	8557	10262	2.61%	0.379%
48	14.371	1390	1393	1398	rBV6	2590	7357	1.87%	0.272%
49	14.449	1398	1401	1405	rVV	7331	12107	3.08%	0.448%
50	14.538	1408	1410	1414	rVV	60701	92620	23.59%	3.425%
51	14.597	1414	1416	1420	rVB2	3247	7674	1.95%	0.284%
52	14.903	1445	1447	1450	rBV2	3761	5908	1.50%	0.218%
53	15.278	1483	1485	1487	rVB2	8803	13295	3.39%	0.492%
54	15.396	1495	1497	1501	rVV4	7174	12382	3.15%	0.458%
55	15.761	1531	1534	1538	rBV3	3674	9768	2.49%	0.361%
56	15.998	1555	1558	1560	rBV3	3825	7052	1.80%	0.261%


Sum of corrected areas: 2704274

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_F\DATA\VF111518\
Data File : VF060752.D
Acq On : 15 Nov 2018 17:48
Operator : VA/AP
Sample : J5942-01
Misc : 6.38g/5mL/MSV0A-F/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSV0A_F
ClientSampled :
VW-D1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_F\METHODS\82F111318S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

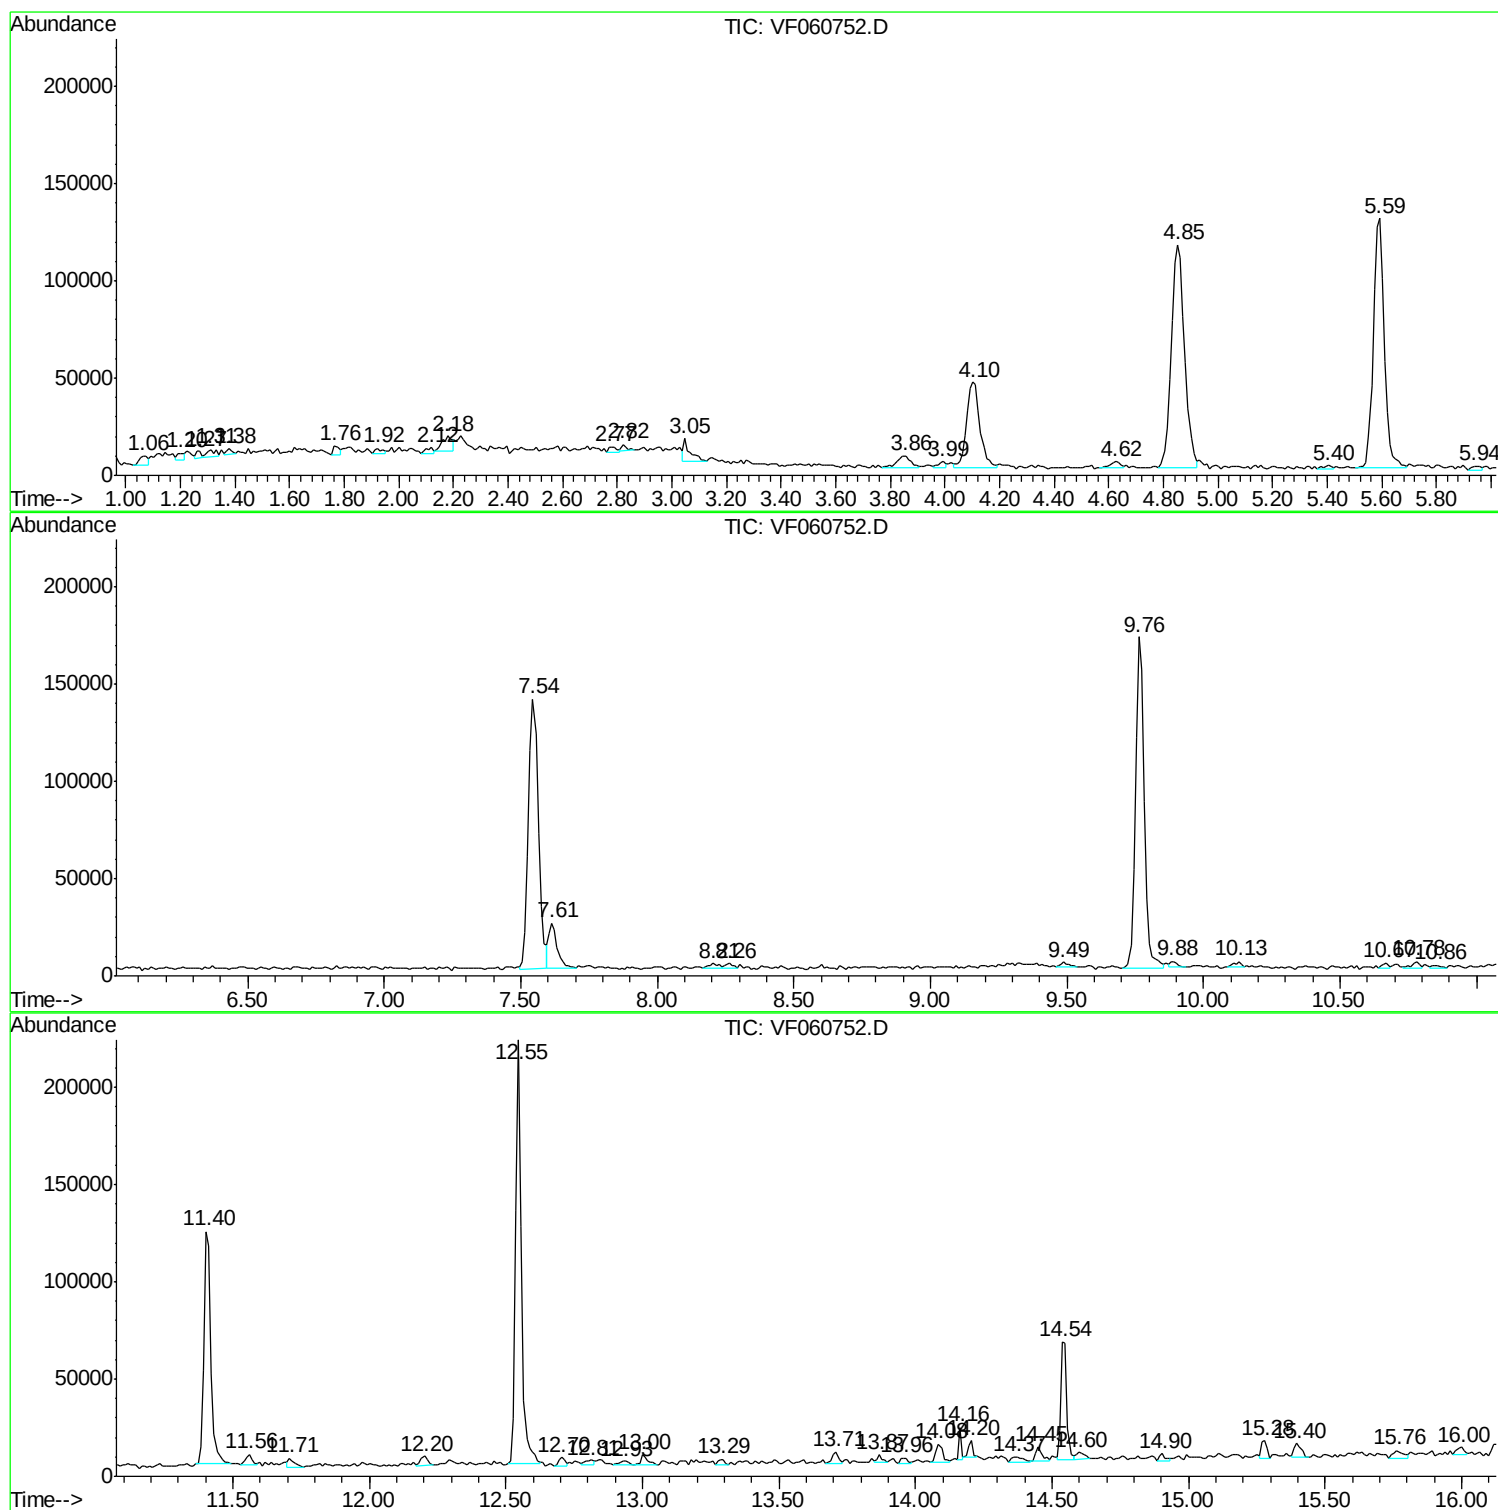

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_F\DATA\VF111518\
Data File : VF060752.D
Acq On : 15 Nov 2018 17:48
Operator : VA/AP
Sample : J5942-01
Misc : 6.38g/5mL/MSV0A-F/SOIL
ALS Vial : 17 Sample Multiplier: 1










Instrument :
MSV0A_F
ClientSampleId :
VW-D1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_F\METHODS\82F111318S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 N,N-Diethylaniline Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.54	13.99 ug/l	92620	1,4-Dichlorobenzene-d4	12.55
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1		N,N-Diethylaniline	149 C10H15N	000091-66-7 95
2		Benzenamine, 2-(1,1-dimethylethyl)-	149 C10H15N	006310-21-0 59
3		2-Coumaranone	134 C8H6O2	000553-86-6 53
4		3-Pyridinecarbonitrile, 1,4-dihy...	134 C7H6N2O	000767-98-6 53
5		3-Methylisoxazolo[5,4-b]pyridine	134 C7H6N2O	058035-50-0 50

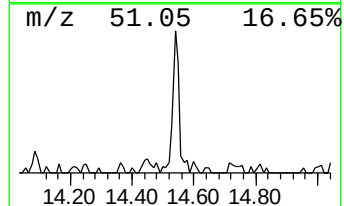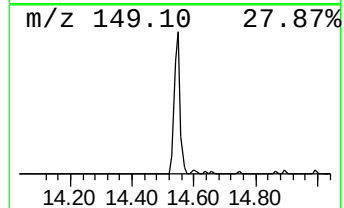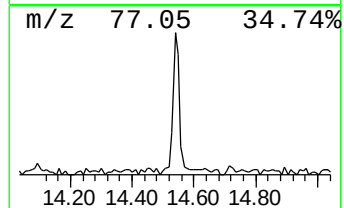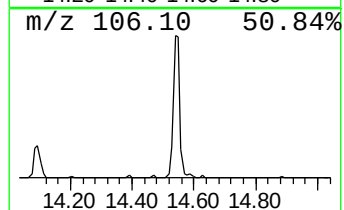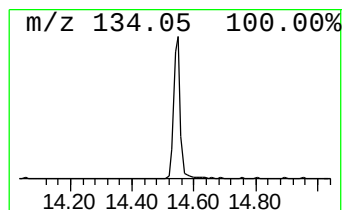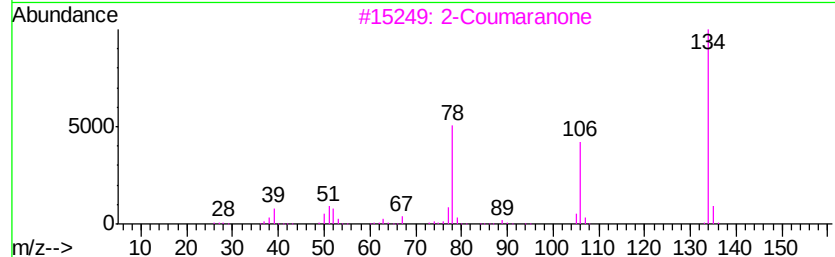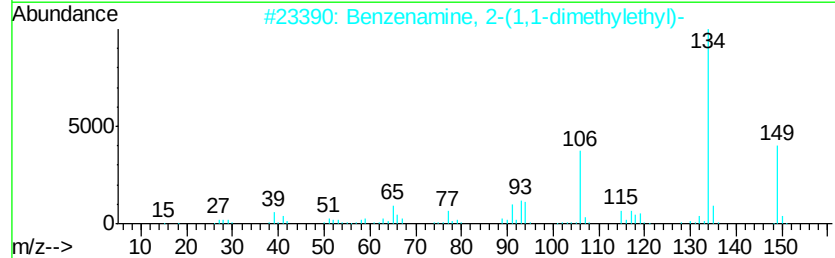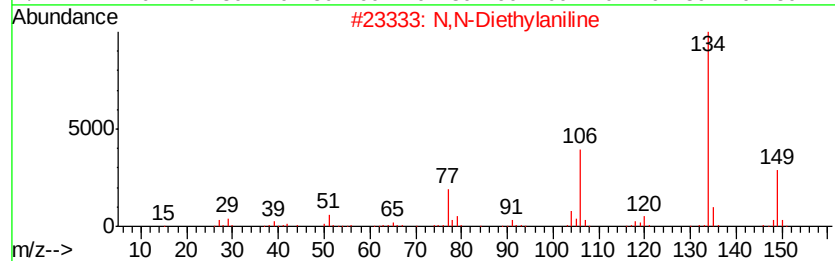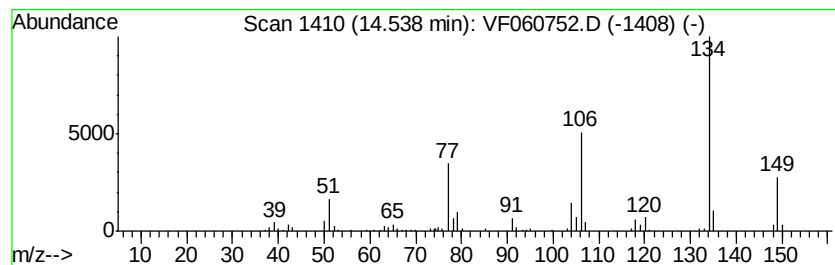

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_F\DATA\VF111518\
Data File : VF060752.D
Acq On : 15 Nov 2018 17:48
Operator : VA/AP
Sample : J5942-01
Misc : 6.38g/5mL/MSVOA-F/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
VW-D1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F111318S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
N,N-Diethylaniline	14.54	14.0	ug/l	92620	4	12.55	330976	50.0