


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_F\DATA\VF111518\
Data File : VF060738.D
Acq On : 15 Nov 2018 9:37
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_F\METHODS\82F111318S.M
Title : SW846 8260
Last Update : Wed Nov 14 03:11:14 2018

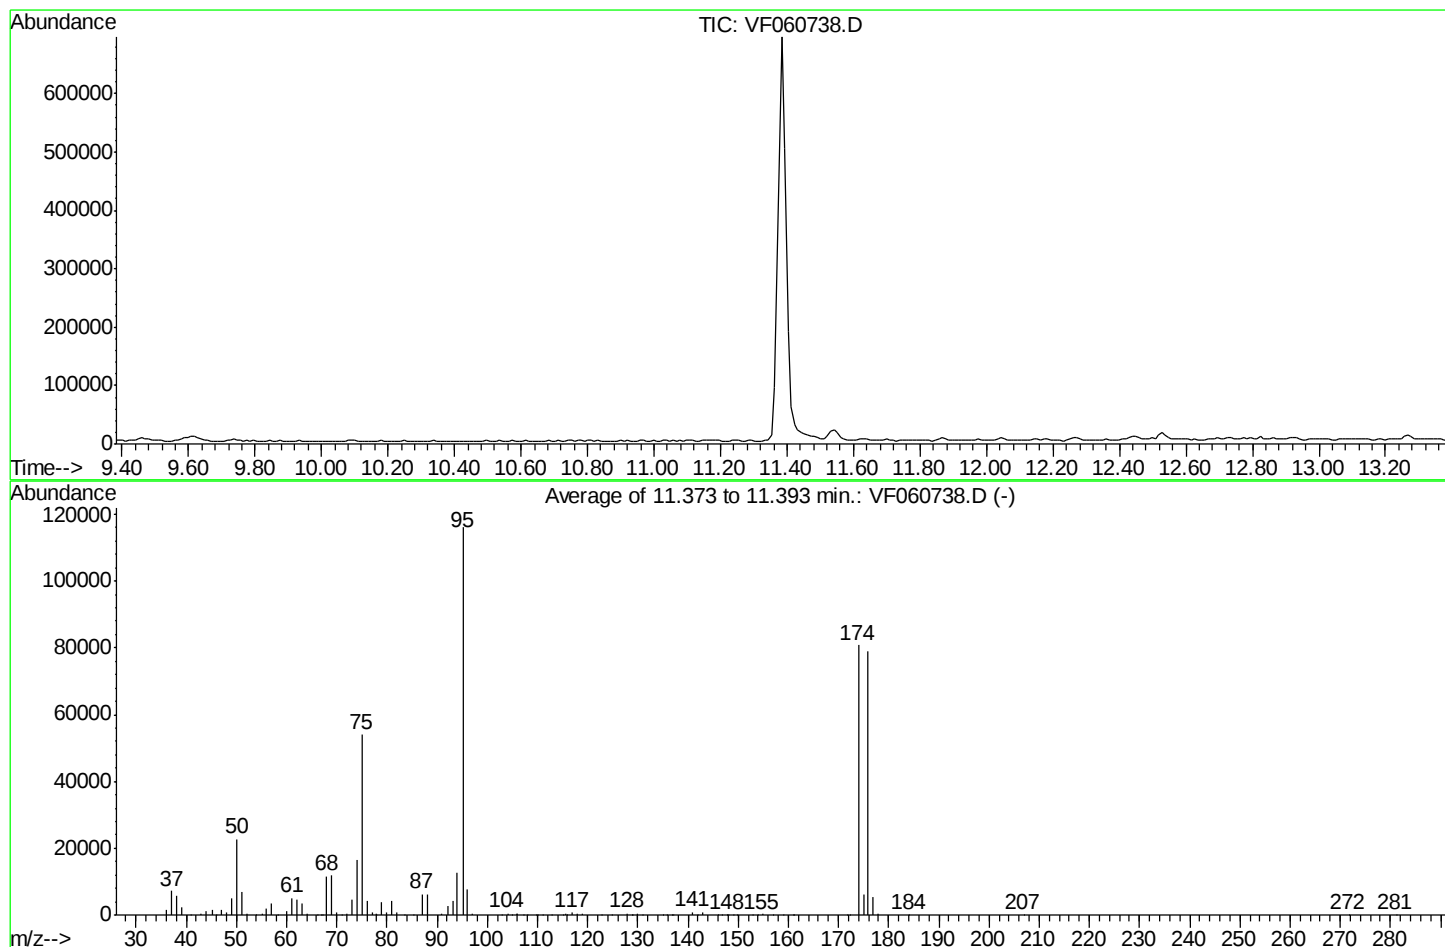

AutoFind: Scans 1089, 1090, 1091; Background Corrected with Scan 1082

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	22634	PASS
75	95	30	60	46.4	53925	PASS
95	95	100	100	100.0	116098	PASS
96	95	5	9	6.7	7810	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.6	80757	PASS
175	174	5	9	7.5	6046	PASS
176	174	95	101	97.7	78912	PASS
177	176	5	9	6.9	5413	PASS