


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF111618\
 Data File : VF060760.D
 Acq On : 16 Nov 2018 10:15
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F111318S.M
 Title : SW846 8260
 Last Update : Wed Nov 14 03:11:14 2018

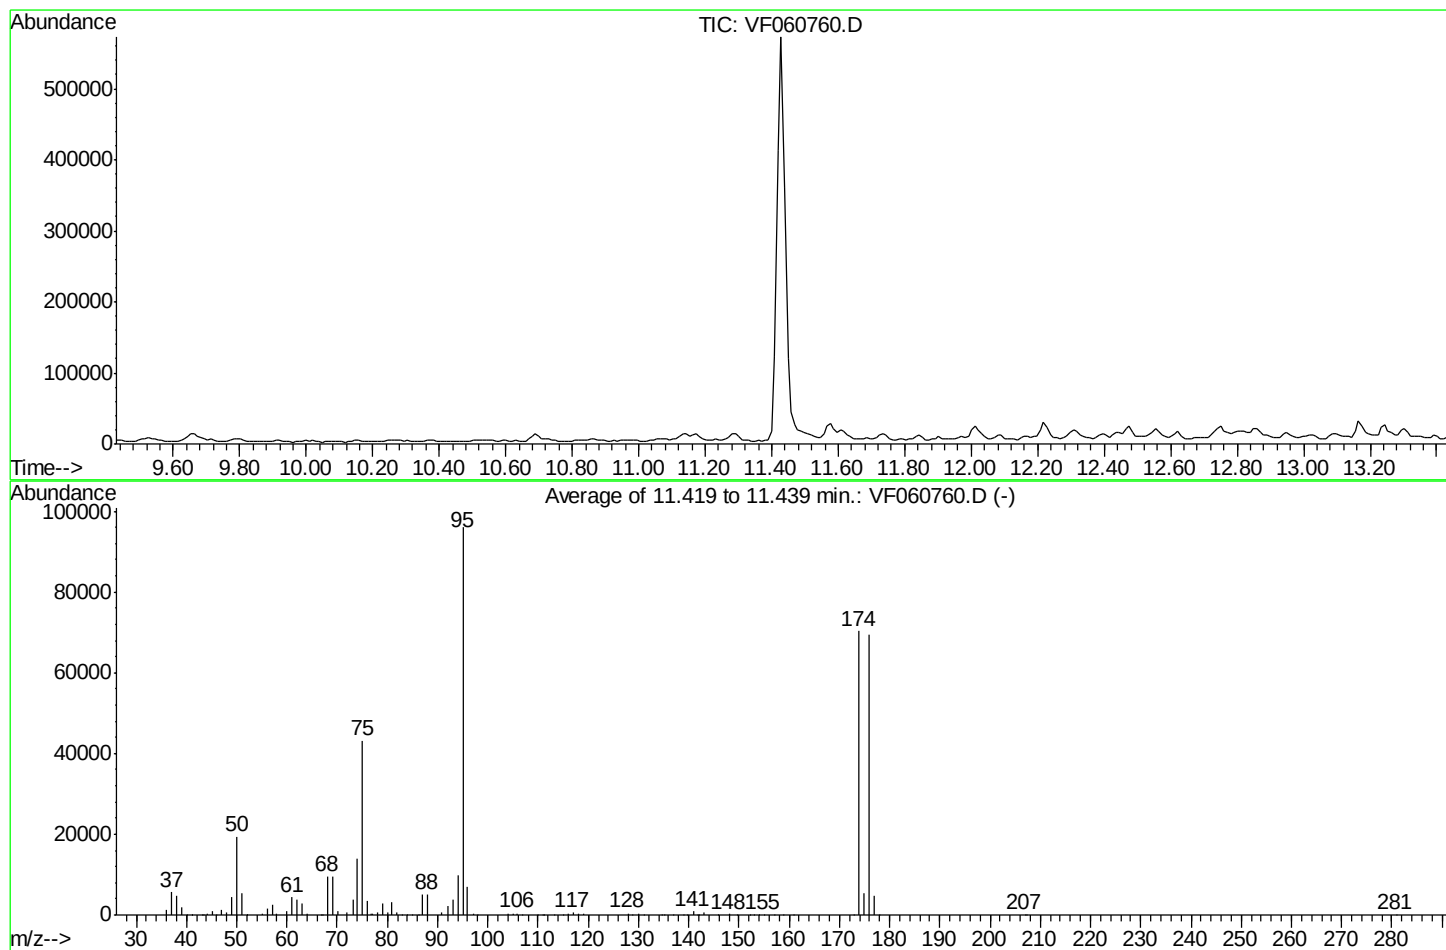

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1088

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	19345	PASS
75	95	30	60	45.0	43221	PASS
95	95	100	100	100.0	96018	PASS
96	95	5	9	7.3	7037	PASS
173	174	0.00	2	0.1	83	PASS
174	95	50	100	73.3	70381	PASS
175	174	5	9	7.9	5544	PASS
176	174	95	101	98.7	69490	PASS
177	176	5	9	6.6	4610	PASS