


Data Path : Z:\voasrv\HPCHEM1\MSVOA F\Data\VF111918\
 Data File : VF060779.D
 Acq On : 19 Nov 2018 15:21
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA-F/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_F
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F111318S.M
 Title : SW846 8260
 Last Update : Wed Nov 14 03:11:14 2018

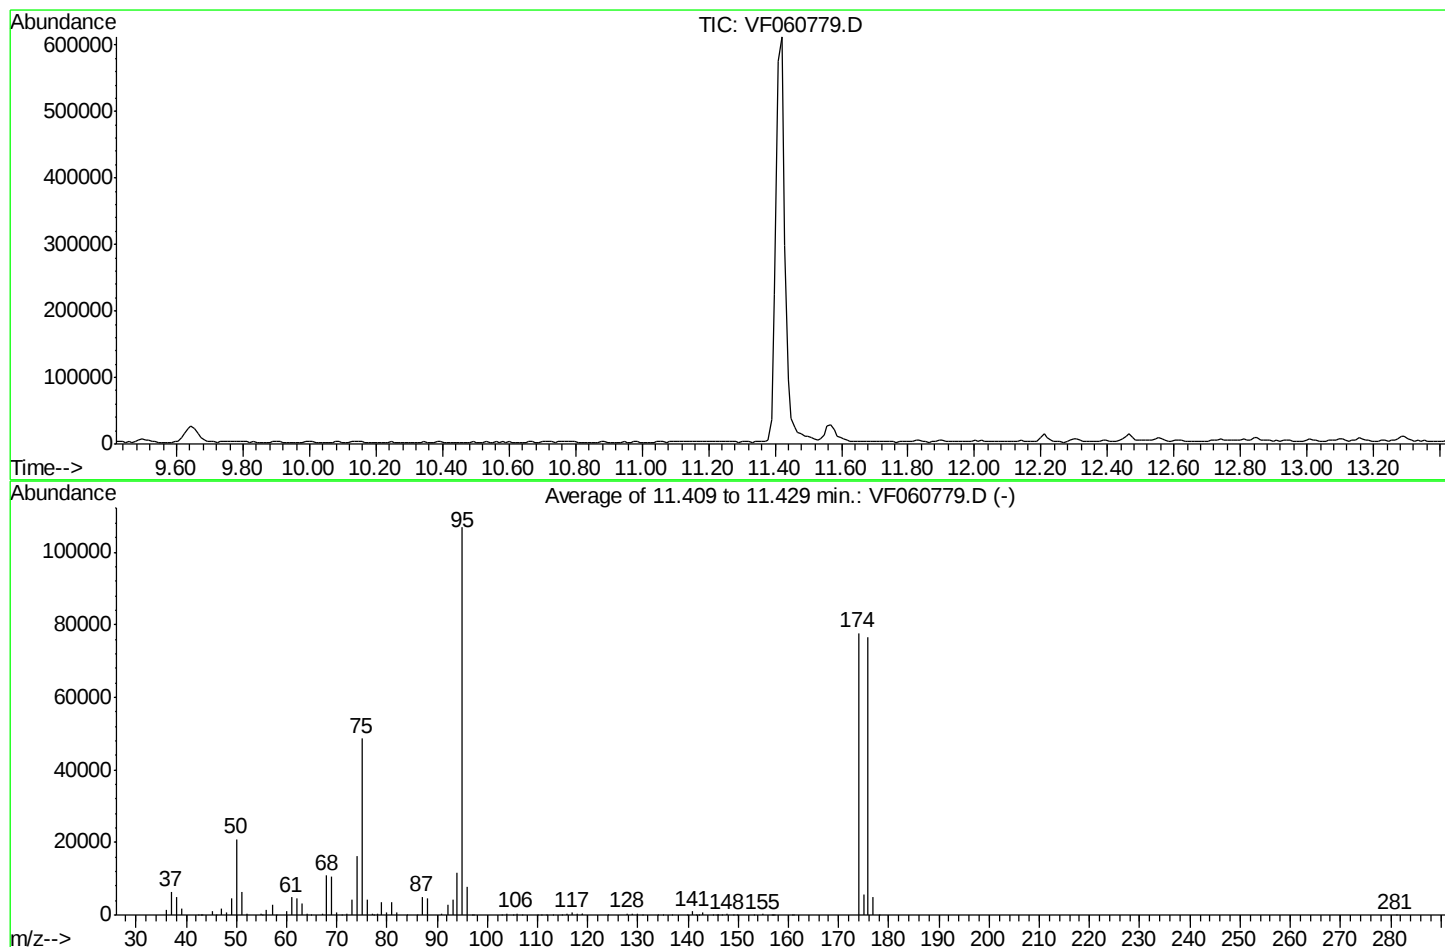

AutoFind: Scans 1093, 1094, 1095; Background Corrected with Scan 1087

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	20914	PASS
75	95	30	60	45.4	48520	PASS
95	95	100	100	100.0	106826	PASS
96	95	5	9	7.4	7914	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.8	77728	PASS
175	174	5	9	7.4	5780	PASS
176	174	95	101	98.5	76570	PASS
177	176	5	9	6.3	4848	PASS