


Data Path : Z:\VOASRV\HPCHEM1\MSVOA F\DATA\VF112618\
Data File : VF060825.D
Acq On : 26 Nov 2018 16:00
Operator : VA/AP
Sample : BFB
Misc : 5.00µ/5mL/MSVOA-F/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_F
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_F\METHODS\82F112618S.M
Title : SW846 8260
Last Update : Tue Nov 27 01:36:26 2018

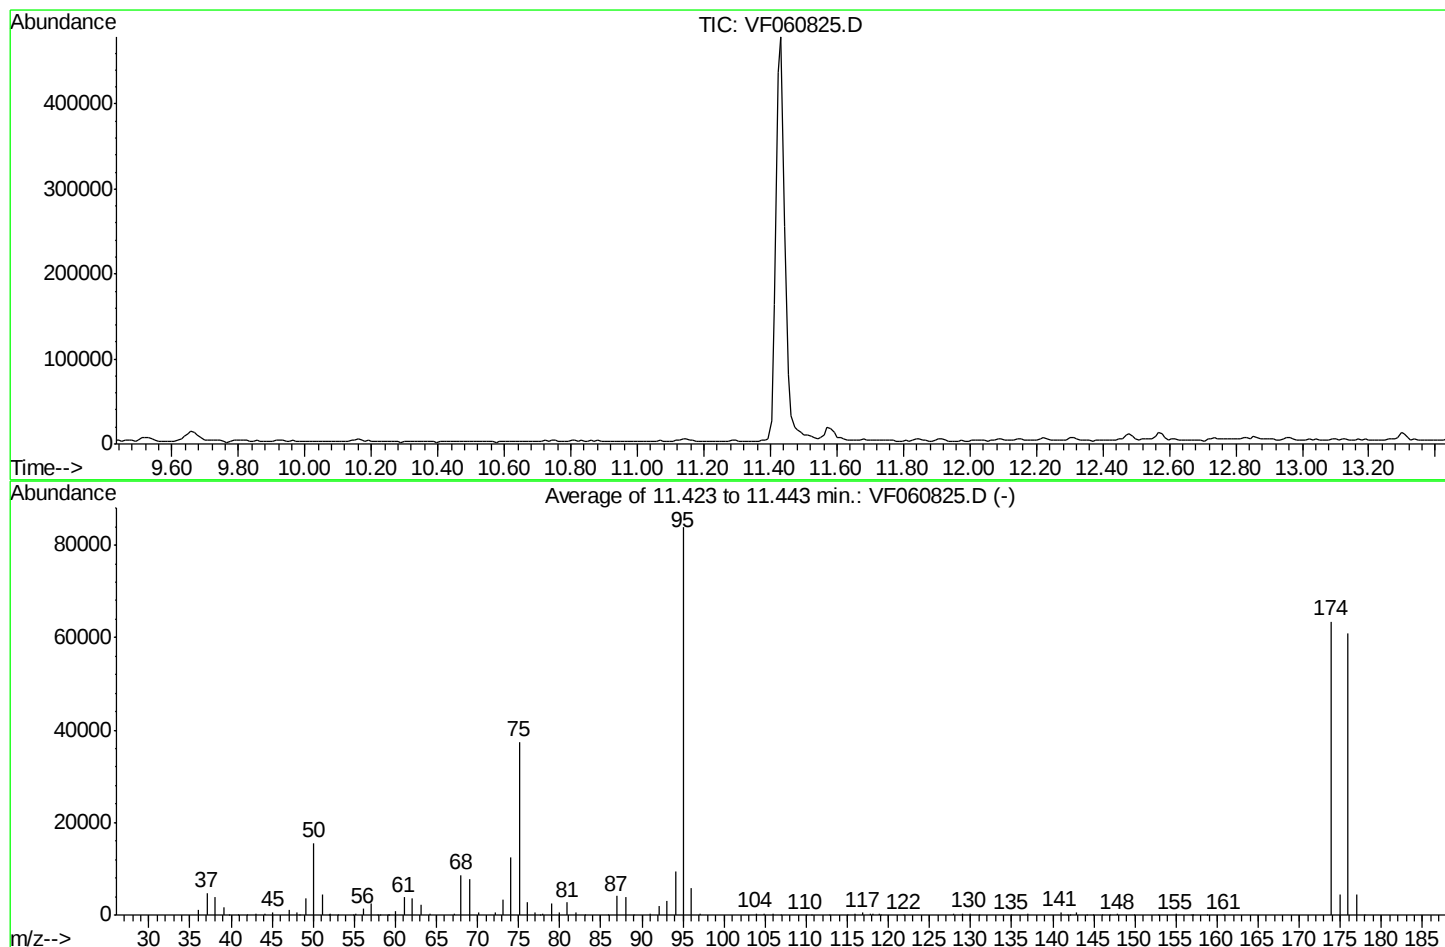

AutoFind: Scans 1094, 1095, 1096; Background Corrected with Scan 1088

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	15604	PASS
75	95	30	60	44.6	37389	PASS
95	95	100	100	100.0	83864	PASS
96	95	5	9	6.9	5787	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.7	63456	PASS
175	174	5	9	7.1	4490	PASS
176	174	95	101	95.9	60877	PASS
177	176	5	9	7.1	4328	PASS